

Method 508 MODDate Extracted 4/18/02Page 66

At

#GCM5-18287

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	
L.B.		500 ml		1 ml			1 ml	9B	7		
Ref. 1					1 ml			6A			
Ref. 2					1 ml			4B			
9391								8B			✓
9392								4A			
9393								10A			
9394	F.B.							7A			
9395								10B			
9396								8A			
9397								7B			
9398	F.B.	↓		↓			↓	9A	↓		✓
1											
Remarks											
Reviewed by, <i>CB 8/16/02</i>											
drip rate must be between 5-15 ml/min for liq-liq extractors											
drip rate -											
Extraction type - SEP. FWA Solv. lot# X05E10 NaCl lot# V39614 Na2SO4 lot# 146648											
STANDARD	INT STD LOG#										
CALIBRATION	HP05DL02										
REF SPIKE	2193										
MDL/MDRF											
Q. CHECK											
INT. STD.	15042602										
SURROGATE											
LPC											
ENDRIN/DDT											

Analyst A.D.
revision 4/12/01Verified by mgReviewed by DM
Date 5/9/02

Comment:
Operator:
Data Path: C:\HPCHEM\1\DATA\MAY0102\
Pre-Seq Cmd:
Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0501	
2	Sample	2	CAL40	GCMS0501	
3	Sample	3	8264	GCMS0501	gc/ms scan 4/23
4	Sample	4	9565	GCMS0501	gc/ms scan 4/23
5	Sample	5	9566	GCMS0501	gc/ms scan 4/23
6	Sample	6	9567	GCMS0501	gc/ms scan 4/23
7	Sample	7	LB	GCMS0501	gc/ms scan 4/18
8	Sample	8	REF1	GCMS0501	gc/ms scan 4/18
9	Sample	9	REF2	GCMS0501	gc/ms scan 4/18
10	Sample	10	9391	GCMS0501	gc/ms scan 4/18
11	Sample	11	9393	GCMS0501	gc/ms scan 4/18
12	Sample	12	9394	GCMS0501	gc/ms scan 4/18 fb
13	Sample	13	9395	GCMS0501	gc/ms scan 4/18
14	Sample	14	9396	GCMS0501	gc/ms scan 4/18
15	Sample	15	9397	GCMS0501	gc/ms scan 4/18
16	Sample	16	9398	GCMS0501	gc/ms scan 4/18 fb

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY0102\DFTPP.D
 Acq On : 1 May 2002 8:03 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

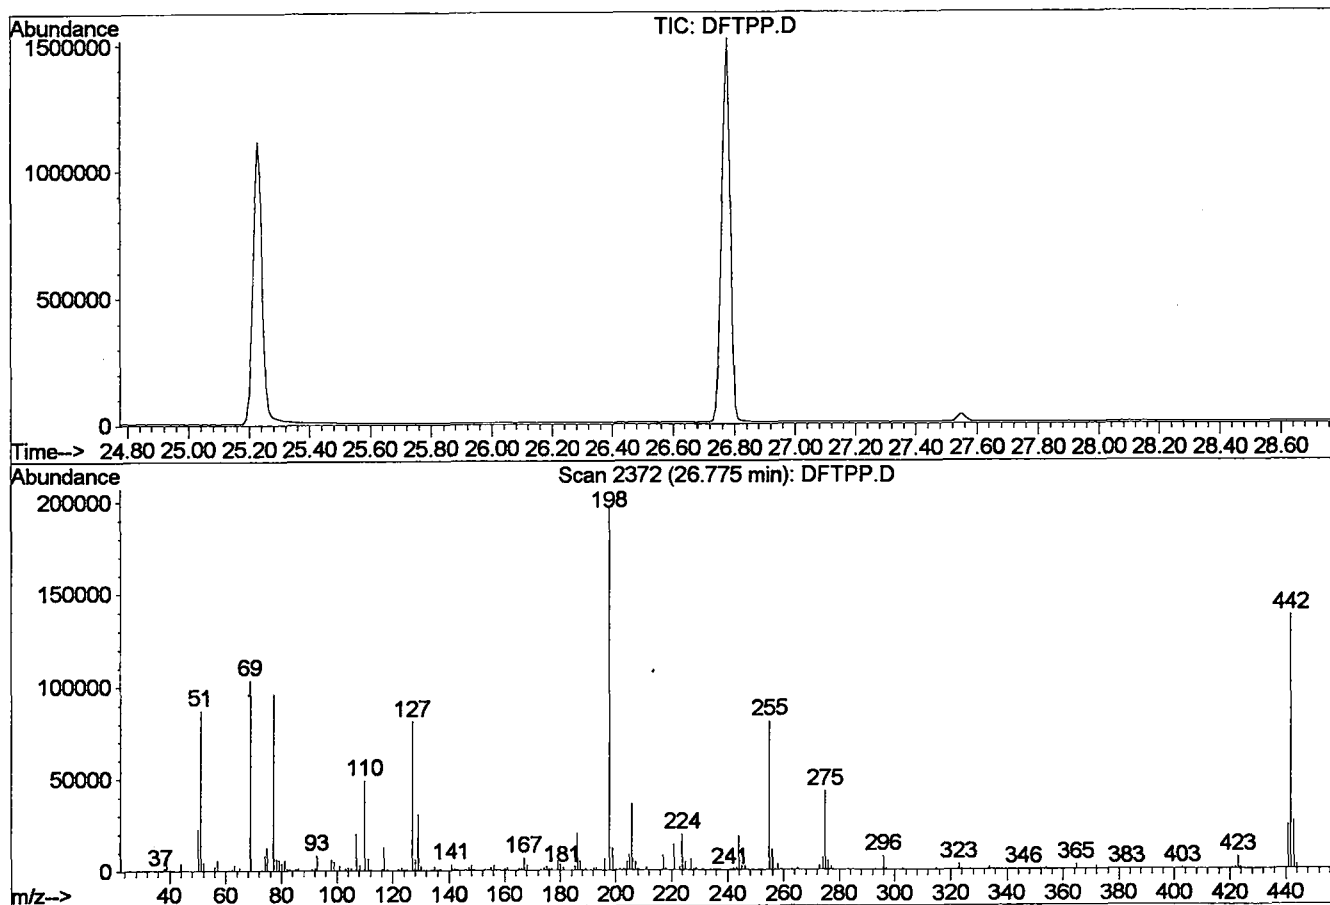

Spectrum Information: Scan 2372

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.2	87240	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.4	103312	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.1	81056	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	197248	PASS
199	198	5	9	6.4	12685	PASS
275	198	10	30	21.7	42816	PASS
365	198	1	100	1.5	3045	PASS
441	443	0.01	100	91.1	24128	PASS
442	198	40	110	69.6	137344	PASS
443	442	17	23	19.3	26488	PASS

DFTPP.D GCMS0501.M

Thu May 02 11:36:04 2002