

Method 508 mod

Date Extracted 4-19-02

Page 68

Ref

#6CMS-18295

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Sol add	IS add	Final vol.	T.V. pos.	pH	Count		
<u>UB</u>		<u>500ml</u>		<u>1ml</u>	<u>1ml</u>		<u>1ml</u>	<u>2A</u>	<u>7</u>			
<u>9446</u>	<u>* See 4/22</u>							<u>3B</u>				
<u>9447</u>								<u>2A</u>				
<u>9448</u>								<u>3A</u>				
<u>9449</u>								<u>1A</u>				
<u>9450</u>								<u>4A</u>				
<u>9451</u>								<u>5A</u>				
								<u>5B</u>				
								<u>1A</u>				

Remarks
* sample #9446 was loss due to broken Turbo vap tube.

Review by sy
5/28/02

drip rate must be between 5-15 ml/min for liq-liq extractors
Extraction type - SPE Fun Solv. lot# 4L470 NaCl lot# V39614 Na2SO4 lot# V46648

STANDARD	INT STD LOG#
CALIBRATION	<u>11205022</u>
REP SPIKE	<u>2279E</u>
MDL/MDRF	
Q. CHECK	
INT. STD.	<u>15072602</u>
SURROGATE	<u>2279E</u> <u>GEMS</u> <u>TCMX</u> <u>4/18</u>
LPC	
ENDRIN/DDT	

Analyst EH.
Revision 4/12/01


Verified by ny

Reviewed by DN
Date 5/8/02

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY0202\DFTPP.D
 Acq On : 2 May 2002 5:29 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

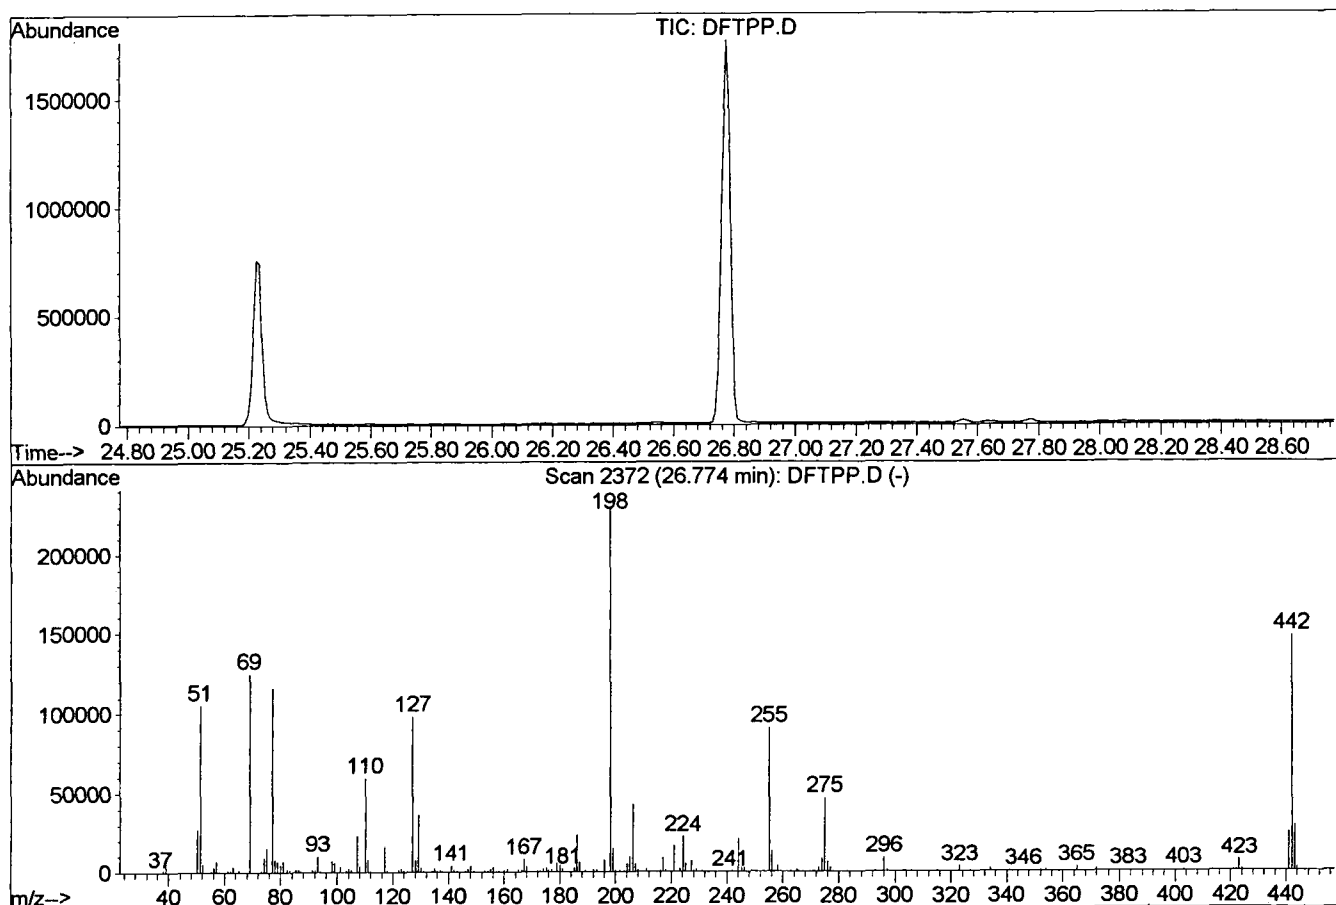

Spectrum Information: Scan 2372

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	46.0	105608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	54.3	124809	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.7	98200	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	229824	PASS
199	198	5	9	6.7	15377	PASS
275	198	10	30	20.6	47304	PASS
365	198	1	100	1.4	3205	PASS
441	443	0.01	100	87.4	25584	PASS
442	198	40	110	64.4	148032	PASS
443	442	17	23	19.8	29288	PASS