

Method 508 Mod.

Date Extracted

4/22/02

Page

70

#GCM5-18305


Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ml		1ml				2B	7			
Ref. 1					1ml			4A				
Ref. 2					1ml			5B				
6048								5A				
8481	<i>Matched w/ other samples</i>							4B				
8209	"							4A				
9452								3B				
9453	FB							3A				
9521								2B				
9522								2A				
9523								1B				
9524	FB							1A				
Remarks												
Reviewed by <u>CB</u> 8/16/02												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - <u>SEP. Fun</u>		Solv. lot# <u>X06E27</u>		NaCl lot# <u>V39614</u>		Na2SO4 lot# <u>V46648</u>						
STANDARD	INT STD LOG#											
CALIBRATION	<u>HP050202</u>											
REF SPIKE	<u>2279 E</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>042602</u>											
SURROGATE	<u>TCMX</u>											
LPC												
ENDRIN/DDT												

Analyst K.B.
revision 4/12/01Verified by MyReviewed by DM
Date 5/6/02

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY0202\DFTPP.D
 Acq On : 2 May 2002 5:29 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

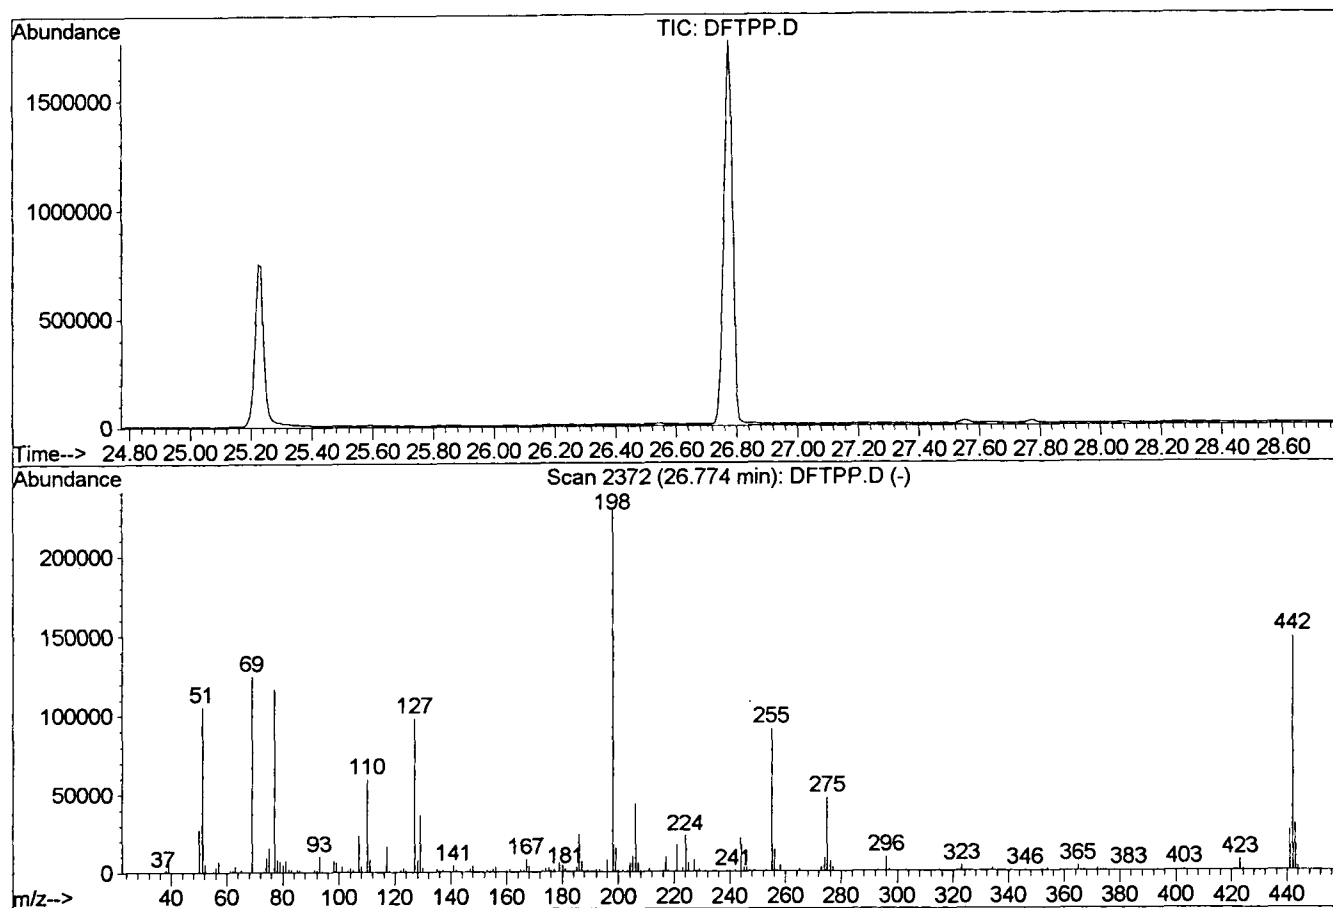

Spectrum Information: Scan 2372

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	46.0	105608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	54.3	124809	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.7	98200	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	229824	PASS
199	198	5	9	6.7	15377	PASS
275	198	10	30	20.6	47304	PASS
365	198	1	100	1.4	3205	PASS
441	443	0.01	100	87.4	25584	PASS
442	198	40	110	64.4	148032	PASS
443	442	17	23	19.8	29288	PASS