

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/06/2002 Time: 10:52:01

Sample: AE09522
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/6/02 10:51 Ended: 5/6/02 10:51 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		94		10.0

Comments for Sample AE09522 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-06-2002 Time: 10:52:32

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0202\9522.D
 Acq On : 3 May 2002 9:38 am
 Sample : GC/MS SCAN 4/22
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 3 10:41 2002

Vial: 20
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0501

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	362149	40.00	ug/l	-0.02
10) Naphthalene-d8	15.83	136	1321347	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.14	164	715489	40.00	ug/l	-0.01
30) Phenanthrene-d10	25.58	188	989686	40.00	ug/l	-0.01
38) Chrysene-d12	33.65	240	628573	40.00	ug/l	-0.02
44) Perylene-d12	37.87	264	406548	40.00	ug/l	-0.01

System Monitoring Compounds

28) TCMX	23.28	209	32715	9.39	ug/L	-0.01
Spiked Amount	10.000		Recovery	=	93.90%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	13.43	77	752	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.89	128	278	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.61	149	909	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	

(#) = qualifier out of range (m) = manual integration

9522.D GCMS0501.M Fri May 03 10:42:16 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0202\9522.D

Vial: 20

Acq On : 3 May 2002 9:38 am

Operator:

Sample : GC/MS SCAN 4/22

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 3 10:41 2002

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed May 01 10:40:31 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0501

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	0.00	178	0	N.D.		
36) Di-n-butylphthalate	27.55	149	5073	N.D.		
37) Fluoranthene	29.28	202	226	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.65	228	2341	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.87	149	2709	N.D.		
43) Chrysene	33.72	228	2024	N.D.		
45) Di-n-Octylphthalate	35.61	149	862	N.D.		
46) Benzo(b)fluoranthene	36.69	252	1350	N.D.		
47) Benzo(k)fluoranthene	36.76	252	1682	N.D.		
48) Benzo(a)pyrene	37.87	252	1627	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

9522.D GCMS0501.M

Fri May 03 10:42:17 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY0202\9522.D
 Acq On : 3 May 2002 9:38 am
 Sample : GC/MS SCAN 4/22
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 3 10:41 2002

Vial: 20
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration

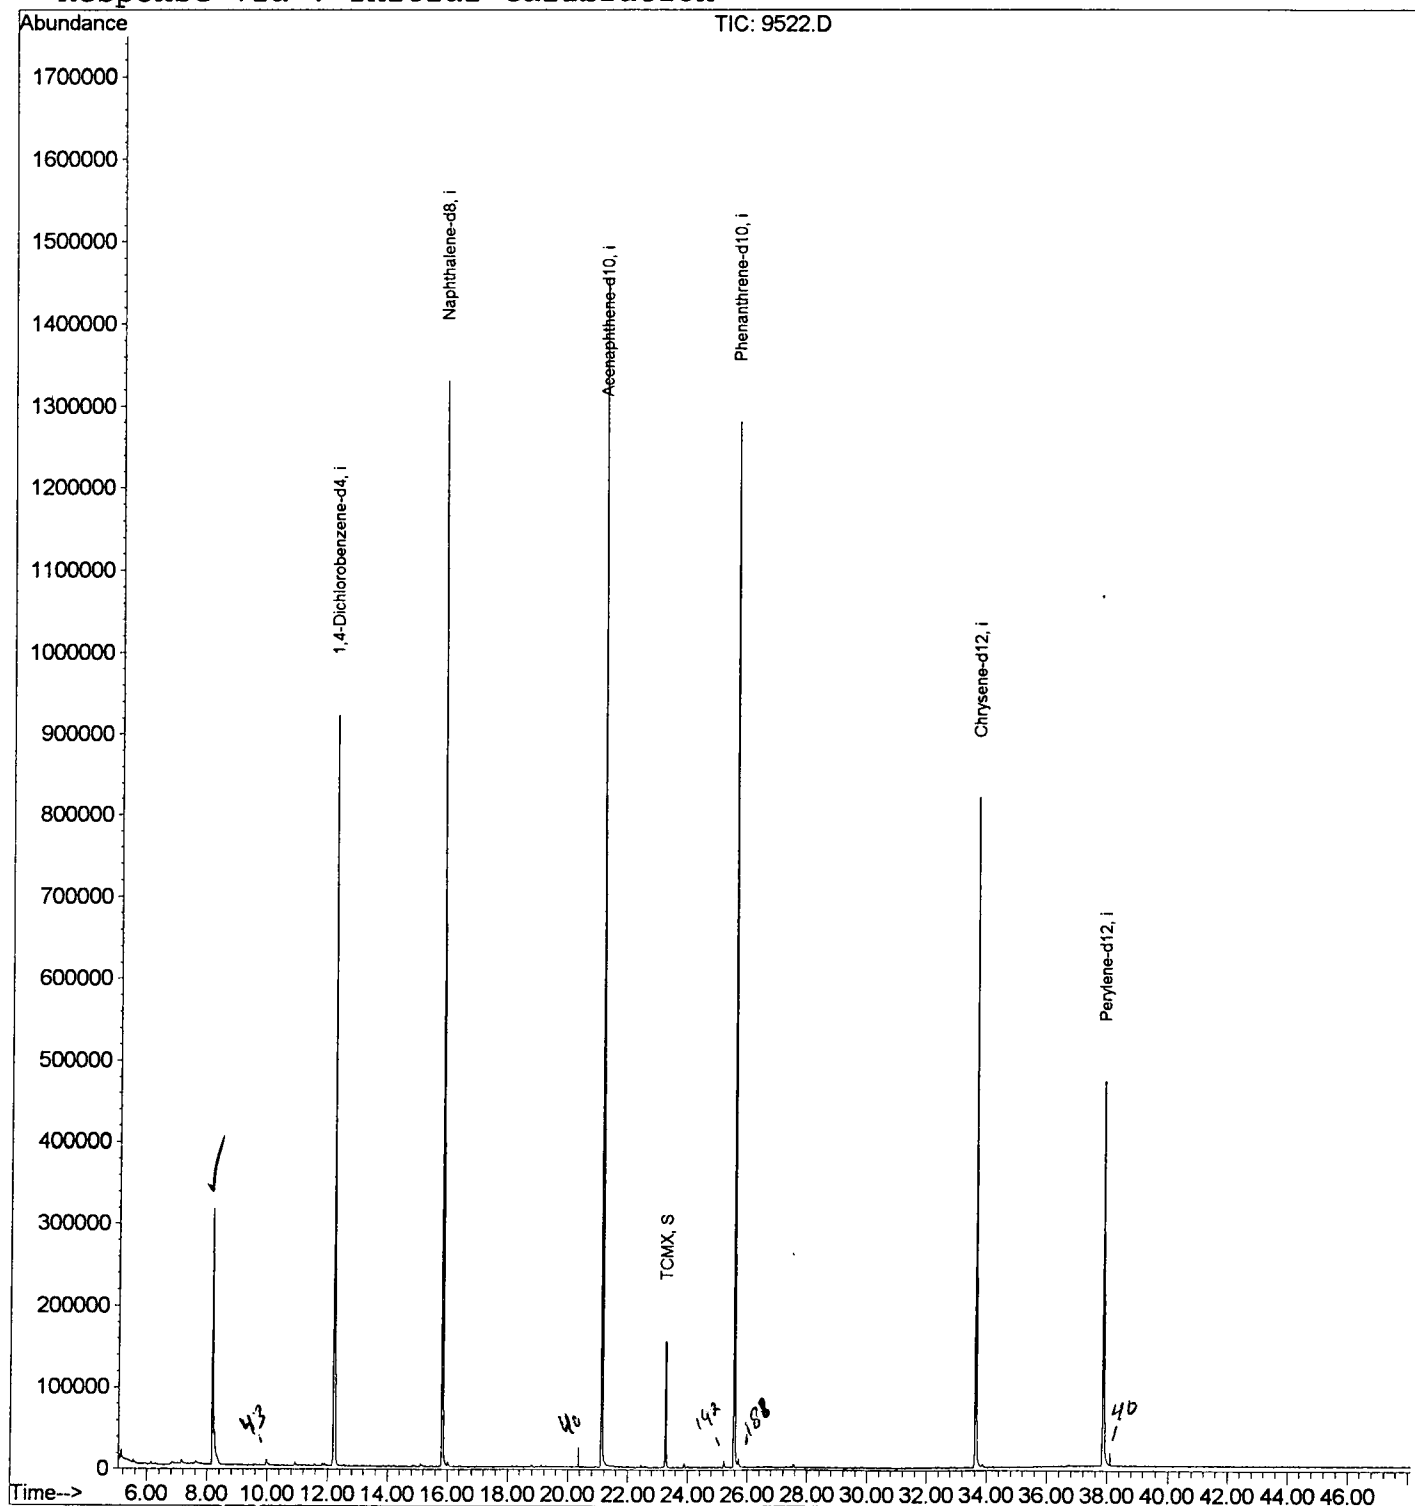

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY0202\9522.D

Vial: 20

Acq On : 3 May 2002 9:38 am

Operator:

Sample : GC/MS SCAN 4/22

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.171	338	342	347	rBV	312882	635172	21.64%	4.343%
2	12.194	776	781	795	rVB	918181	2101261	71.60%	14.366%
3	15.832	1172	1178	1194	rBV	1327154	2652958	90.40%	18.138%
4	21.138	1751	1757	1771	rBV	1453866	2934593	100.00%	20.063%
5	23.273	1984	1990	1996	rBV	154444	314733	10.72%	2.152%
6	25.582	2235	2242	2253	rBV2	1278675	2680713	91.35%	18.328%
7	33.646	3115	3122	3134	rBV2	820052	1877769	63.99%	12.838%
8	37.871	3575	3583	3600	rBV2	470159	1429423	48.71%	9.773%




Sum of corrected areas: 14626622

9522.D GCMS0501.M

Fri May 03 12:24:00 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0202\9522.D
 Operator :
 Acquired : 3 May 2002 9:38 am using AcqMethod GCMS0501
 Instrument : 209
 Sample Name: GC/MS SCAN 4/22
 Misc Info :
 Vial Number: 20
 Quant File :GCMS0501.RES (RTE Integrator)

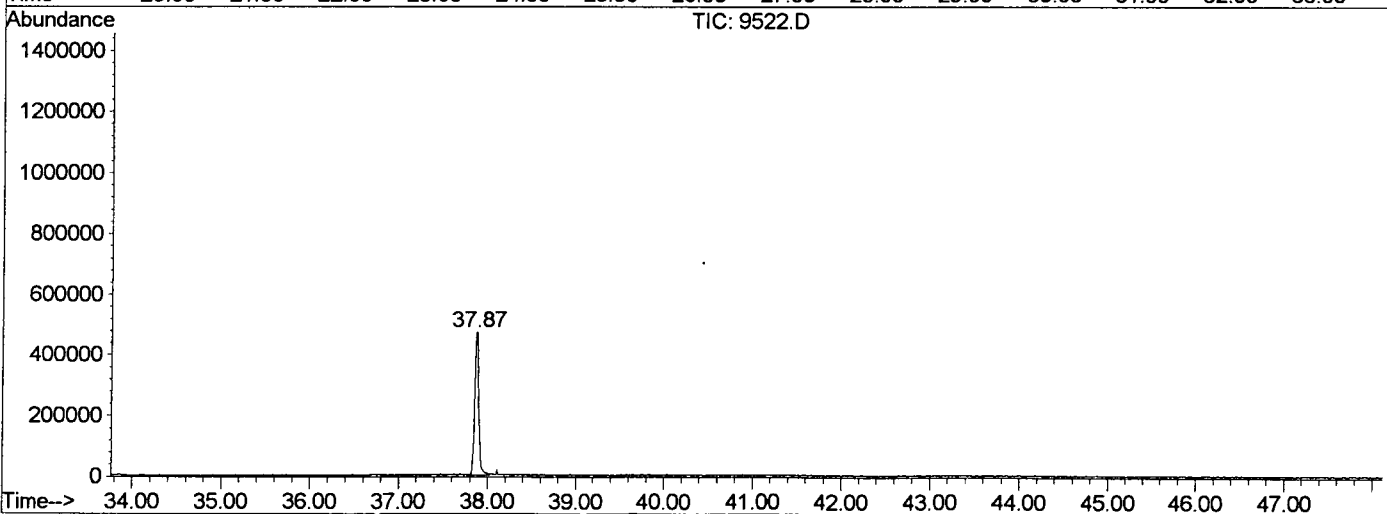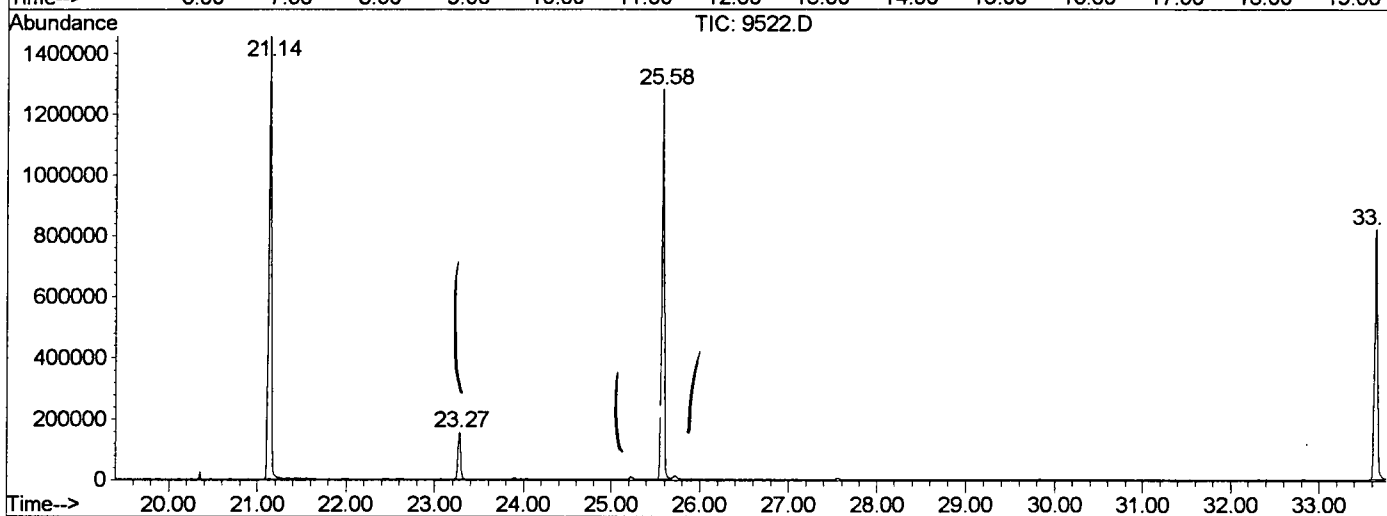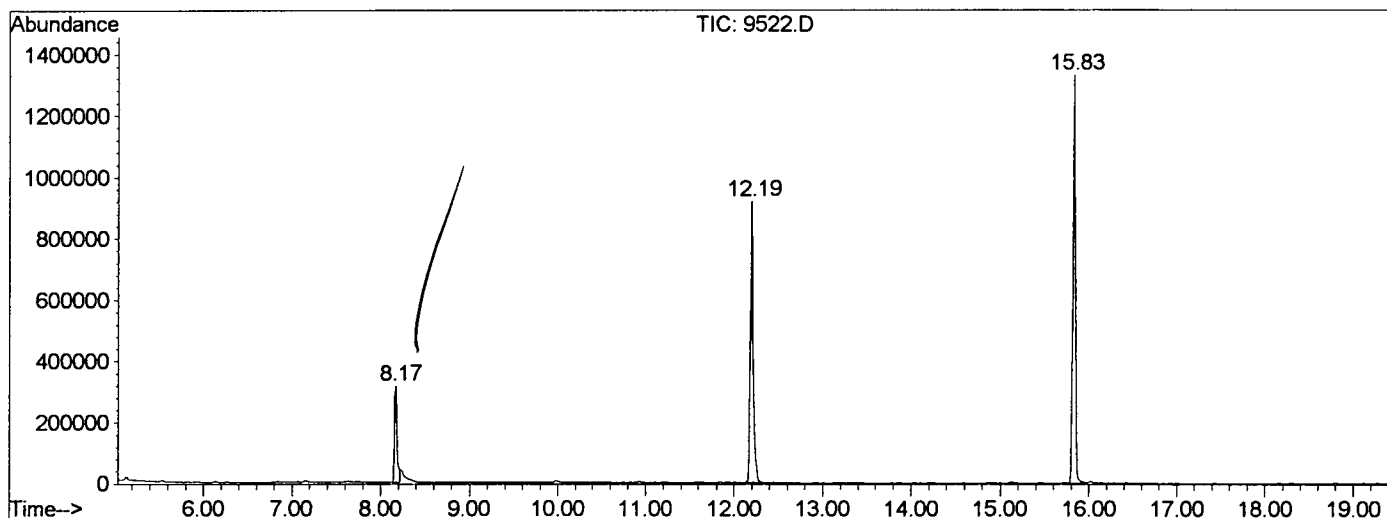

9522.D GCMS0501.M Fri May 03 12:24:01 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0202\9522.D
 Acq On : 3 May 2002 9:38 am
 Sample : GC/MS SCAN 4/22
 Misc :
 MS Integration Params: LSCINT.P


Vial: 20
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.17	12.09 ug/l	635172	1,4-Dichlorobenzene-d4	12.19

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78	
2	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9	
3	N,N'-Bis(2-methyl-2-nitrosopentan-4	258	C12H22N2O4	094514-30-4	9	
4	Acetic acid, 2-methylpropyl ester	116	C6H12O2	000110-19-0	9	

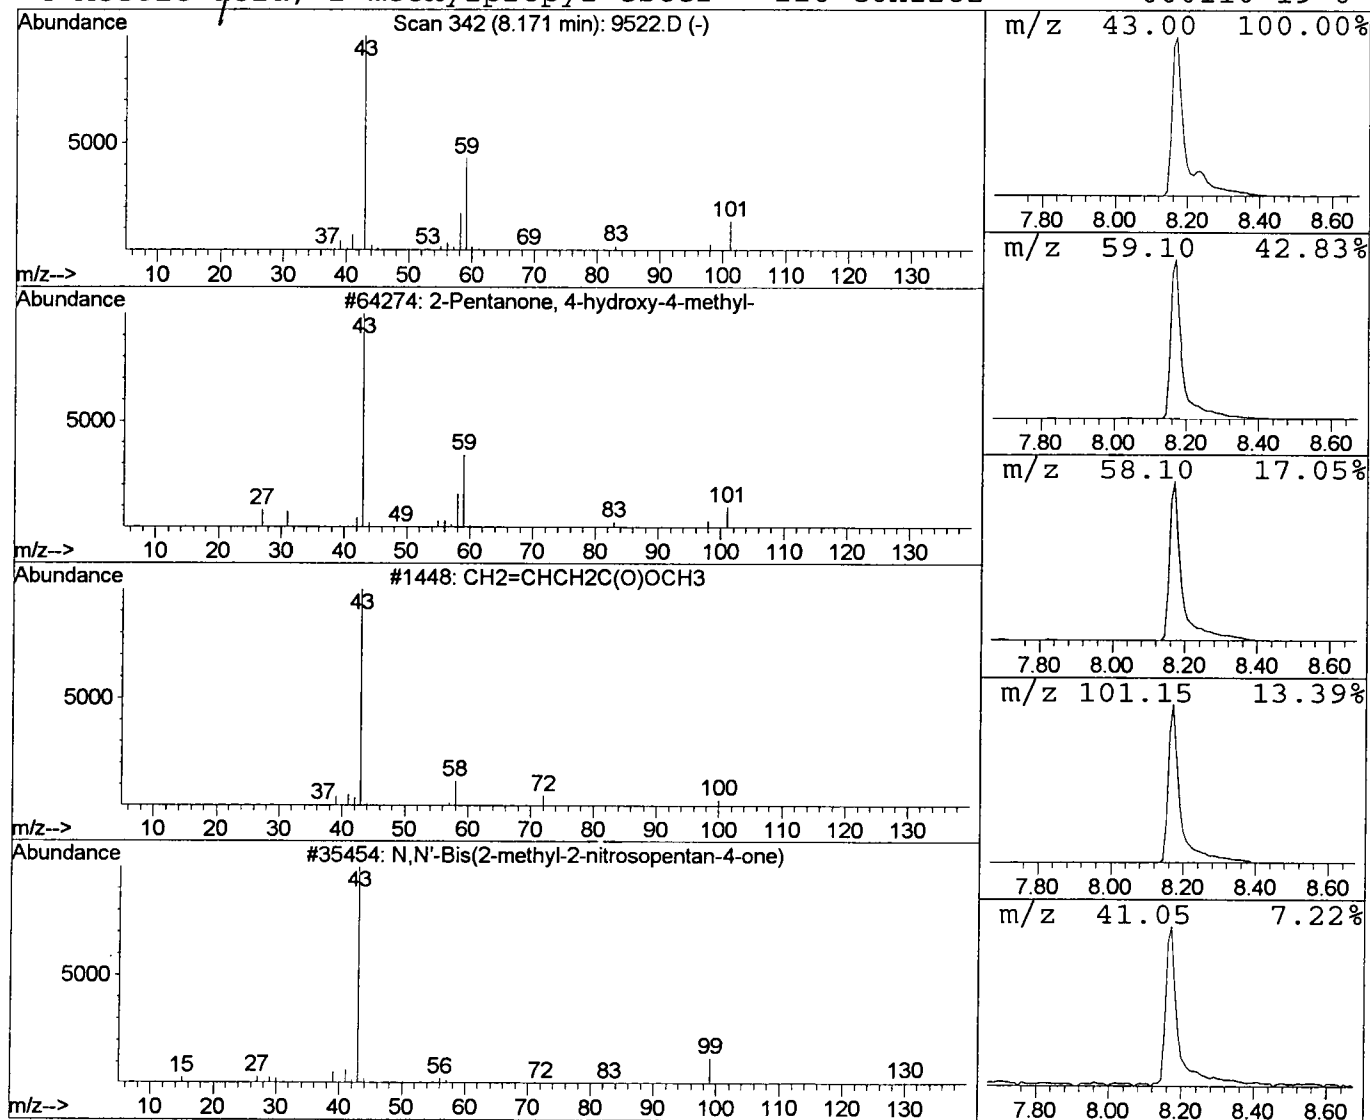

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 3 May 2002 9:38 am
Data File: C:\HPCHEM\1\DATA\MAY0202\9522.D
Name: GC/MS SCAN 4/22
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.17	12.1	ug/l	635172	ISTD01	12.19	2101260	40.0
9522.D GCMS0501.M	Fri May 03 12:24:02	2002						