

Method 508mod Date Extracted 4-23-02Page 71

Ref #GCM5-18171


Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
<u>LB</u>		<u>500ml</u>		<u>1ml</u>			<u>1ml</u>	<u>1B</u>	<u>7</u>			
<u>661</u>					<u>1ml</u>			<u>1A</u>				
<u>662</u>					<u>↓</u>			<u>3B</u>				
<u>7001</u>								<u>5B</u>				
<u>7002</u>	<u>FB</u>							<u>10B</u>				
<u>7066</u>								<u>9A</u>				
<u>7067</u>								<u>4B</u>				
<u>7068</u>	<u>FB</u>							<u>4A</u>				
<u>7005</u>								<u>5A</u>				
<u>7106</u>								<u>2B</u>				
<u>7107</u>								<u>3A</u>				
<u>7108</u>	<u>FB</u>							<u>2A</u>				
<u>7109</u>								<u>10A</u>				
Remarks <u>This batch was a Reextraction</u> <u>mf</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type <u>2up fw</u> Solv. lot# <u>X06E27</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V46648</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>V041002</u>											
REF SPIKE	<u>2279E</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>TCMX 4/18</u>											
LPC												
ENDRIN/DDT												

Analyst EH
Revision 4/12/01Verified by mfReviewed by DV
Date 4/29/02

DFTPP

Data File : C:\HPCHEM\1\DATA\APR2402\DFTPP.D
 Acq On : 24 Apr 2002 3:52 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

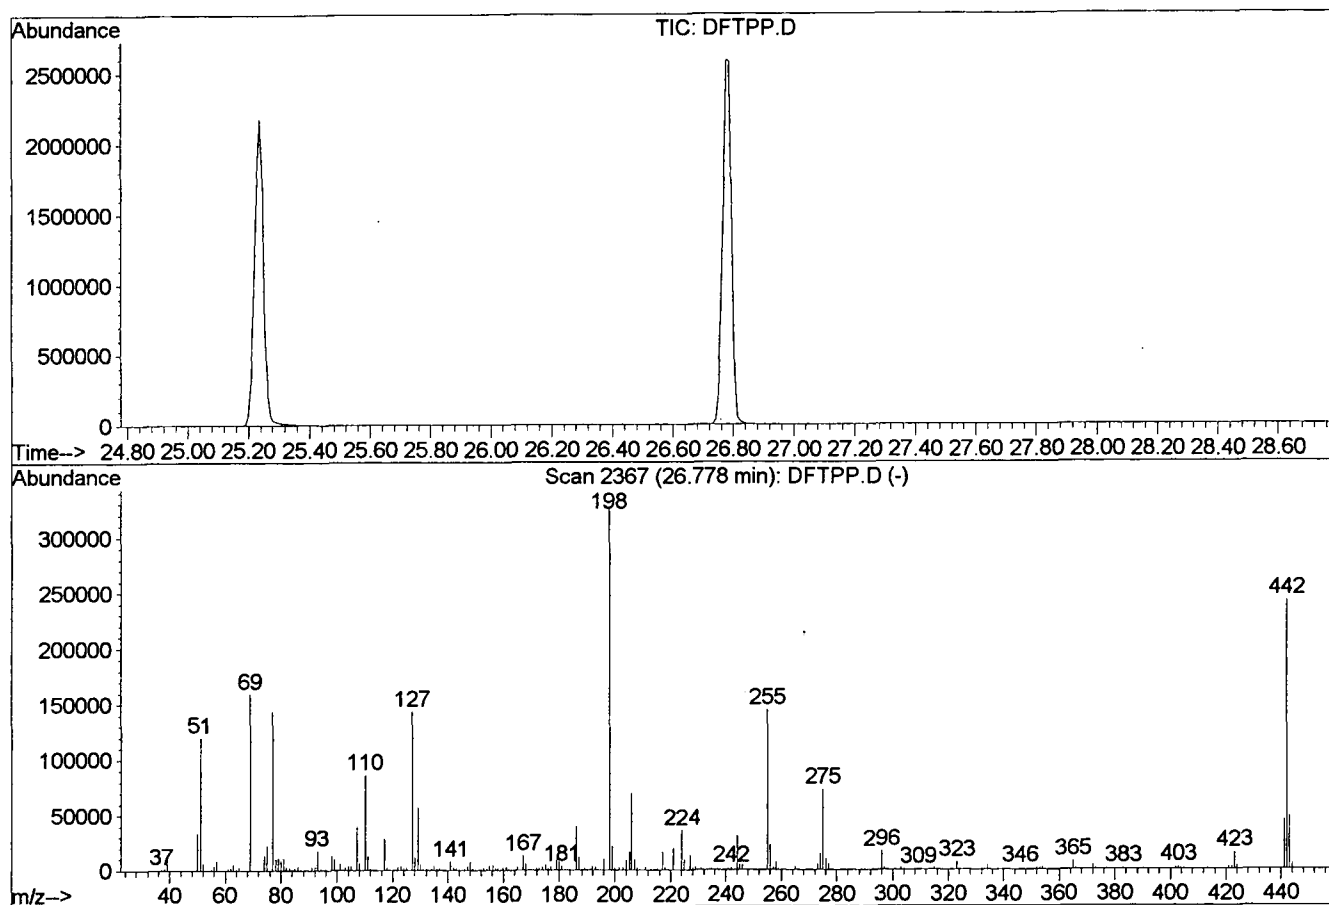

Spectrum Information: Scan 2367

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.6	119838	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.8	159434	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	43.8	143168	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	327027	PASS
199	198	5	9	6.6	21640	PASS
275	198	10	30	22.3	72800	PASS
365	198	1	100	2.1	6993	PASS
441	443	0.01	100	92.2	43728	PASS
442	198	40	110	73.9	241777	PASS
443	442	17	23	19.6	47432	PASS