

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/29/2002 Time: 14:46:16

Sample: AE07001
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/29/02 14:43 Ended: 4/29/02 14:43 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		74		10.0

Comments for Sample AE07001 - Analysis \$GCMS

Westchester Dept. of Labs & Research
User: Vinci, David L
Date: 04-29-2002 Time: 14:47:19

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recoveries for 5 of the 43 compounds in the LCS Standard were low.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2402\7001.D
 Acq On : 24 Apr 2002 8:41 pm
 Sample : gc/ms scan 4/23
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 25 10:59 2002

Vial: 6
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 17 11:48:30 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	497947	20.00	ug/l	-0.03
10) Naphthalene-d8	15.84	136	1822224	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.14	164	1016343	20.00	ug/l	-0.03
30) Phenanthrene-d10	25.58	188	1480918	20.00	ug/l	-0.03
39) Chrysene-d12	33.64	240	949548	20.00	ug/l	-0.03
45) Perylene-d12	37.87	264	589006	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	23.28	209	37492	7.36	ug/L	-0.05
Spiked Amount	10.000		Recovery	=	73.60%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.63	149	789	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

7001.D GCMS0412.M Thu Apr 25 11:01:02 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2402\7001.D Vial: 6
Acq On : 24 Apr 2002 8:41 pm Operator:
Sample : gc/ms scan 4/23 Inst : 209
Misc : Multiplr: 1.00
MS Integration Params: GOOFY.P
Quant Time: Apr 25 10:59 2002 Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Apr 17 11:48:30 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.58	178	289	N.D.		
35) Anthracene	25.58	178	289	N.D.		
36) Di-n-butylphthalate	27.56	149	4044	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.64	228	3144	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.86	149	1198	N.D.		
44) Chrysene	33.71	228	1204	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	36.68	252	500	N.D.		
48) Benzo(k)fluoranthene	36.75	252	977	N.D.		
49) Benzo(a)pyrene	37.87	252	2317	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR2402\7001.D
 Acq On : 24 Apr 2002 8:41 pm
 Sample : gc/ms scan 4/23
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 25 10:59 2002

Vial: 6
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 17 11:48:30 2002
 Response via : Initial Calibration

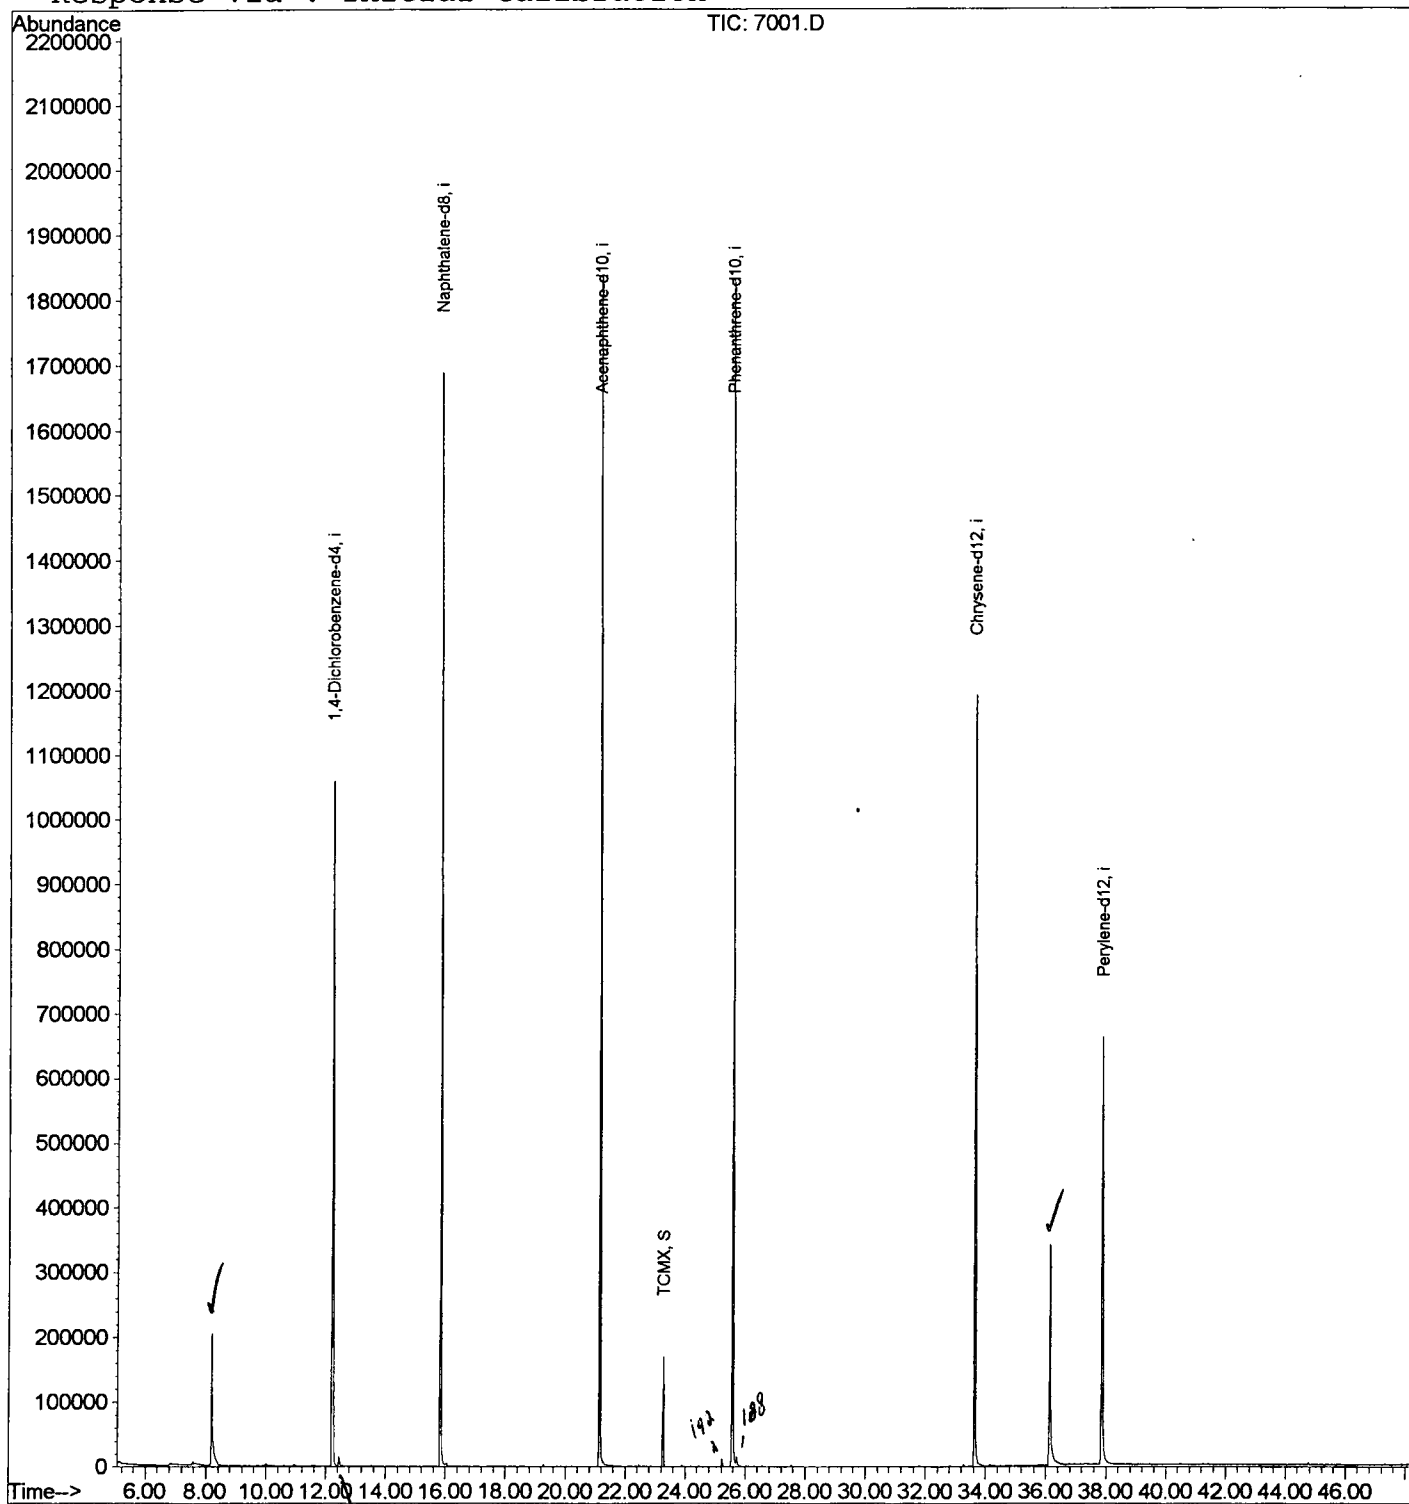

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR2402\7001.D
 Acq On : 24 Apr 2002 8:41 pm
 Sample : gc/ms scan 4/23
 Misc :
 MS Integration Params: LSCINT.P

Vial: 6
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.188	338	342	368	rBV	203207	536659	13.86%	2.636%
2	12.209	775	780	798	rBV	1058266	2695050	69.60%	13.238%
3	15.844	1170	1176	1193	rBV	1687894	3456947	89.28%	16.980%
4	21.141	1747	1753	1763	rBV	1838579	3872083	100.00%	19.019%
5	23.280	1978	1986	1993	rVB	169999	337592	8.72%	1.658%
6	25.584	2230	2237	2248	rBV2	1830228	3738611	96.55%	18.364%
7	33.645	3108	3115	3132	rBV	1190494	2742232	70.82%	13.470%
8	36.123	3380	3385	3408	rBV	340240	996007	25.72%	4.892%
9	37.867	3567	3575	3590	rBV2	659113	1983450	51.22%	9.743%

Sum of corrected areas: 20358631

7001.D GCMS0412.M Thu Apr 25 11:15:19 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR2402\7001.D
 Operator :
 Acquired : 24 Apr 2002 8:41 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: gc/ms scan 4/23
 Misc Info :
 Vial Number: 6
 Quant File :GCMS0412.RES (RTE Integrator)

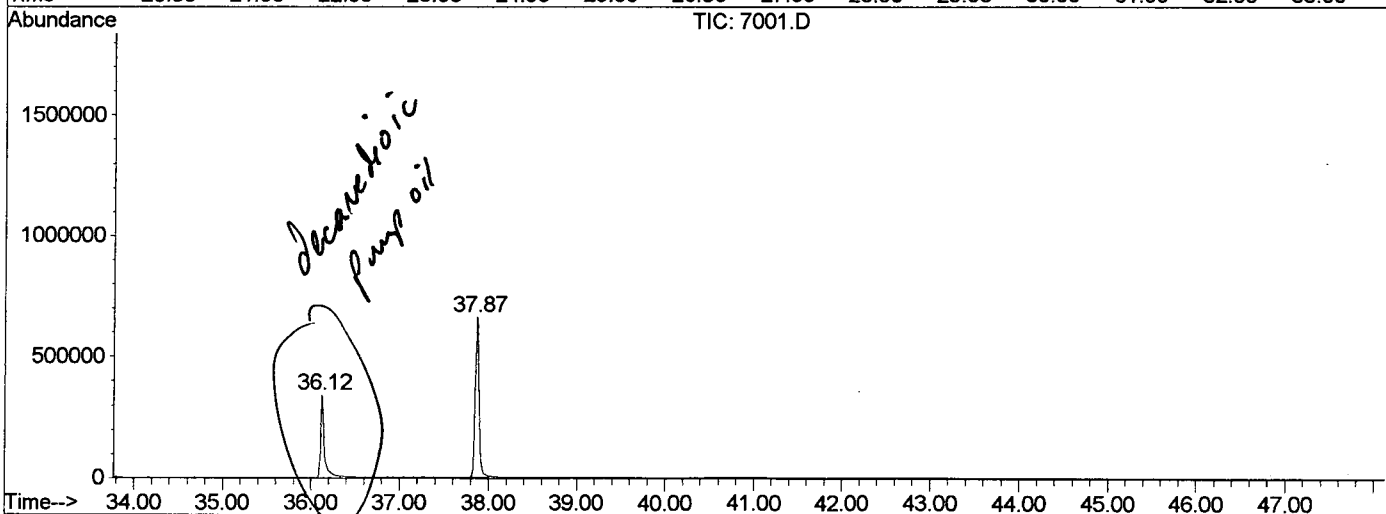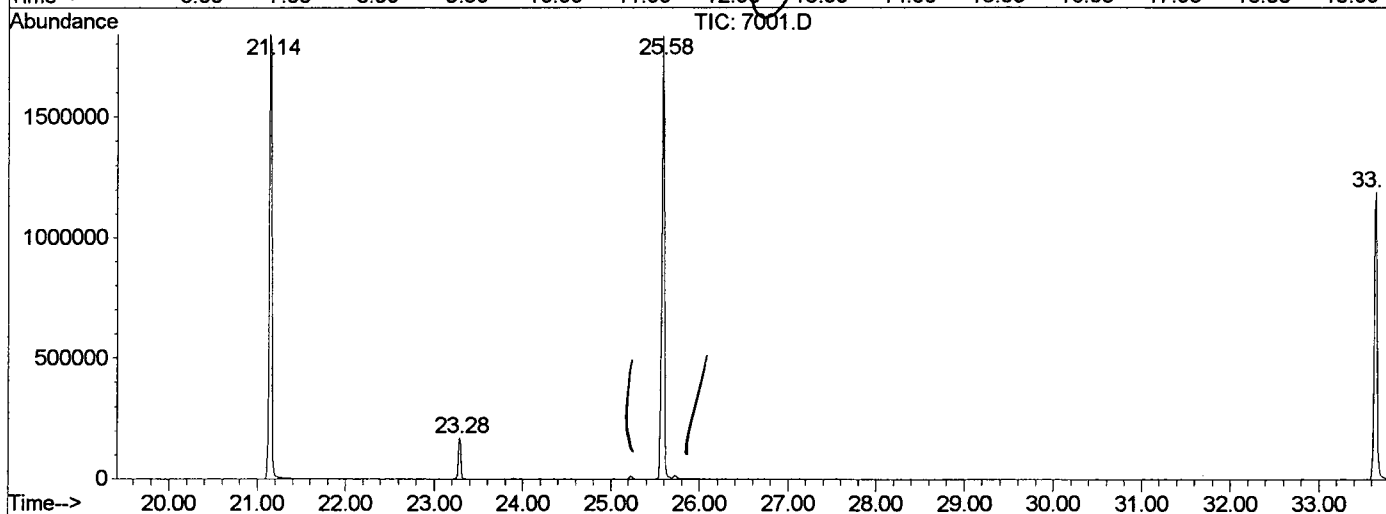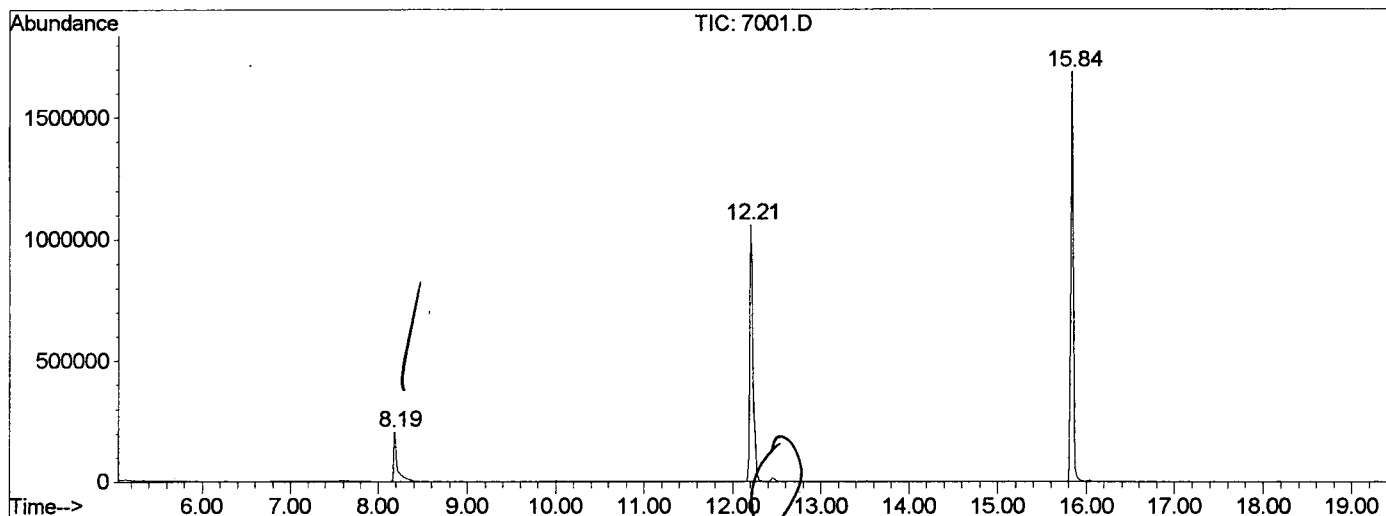

7001.D GCMS0412.M Thu Apr 25 11:15:21 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR2402\7001.D
Acq On : 24 Apr 2002 8:41 pm
Sample : gc/ms scan 4/23
Misc :
MS Integration Params: LSCINT.P









Vial: 6
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.19	3.98 ug/l	536659	1,4-Dichlorobenzene-d4	12.21

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone	4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50	
2	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33		
3	2-Propanol	2-methyl-	74	C4H10O	000075-65-0	17	
4	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	10		

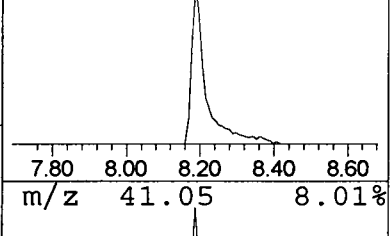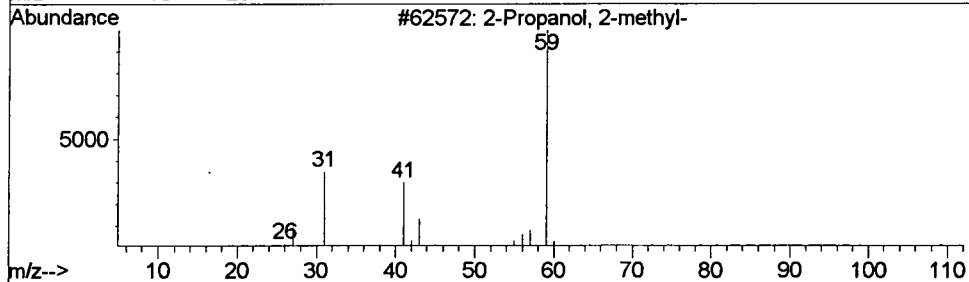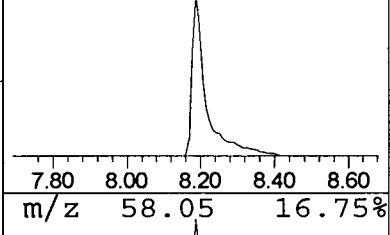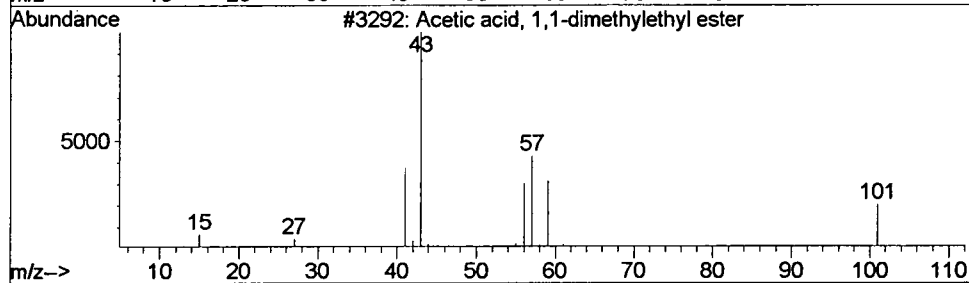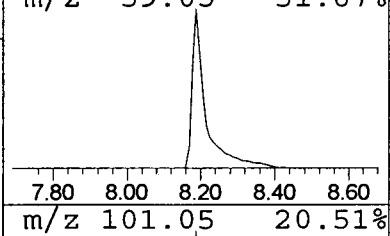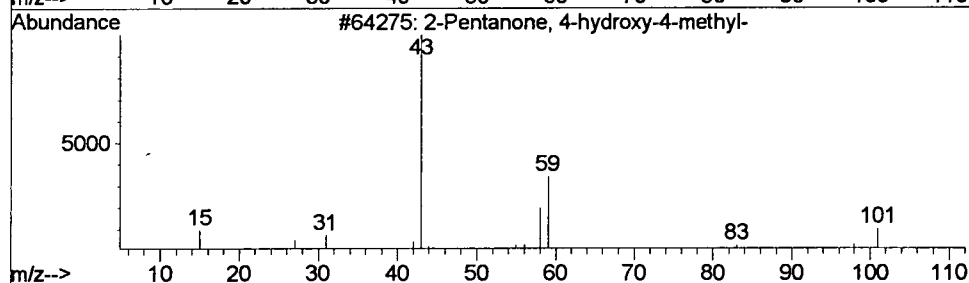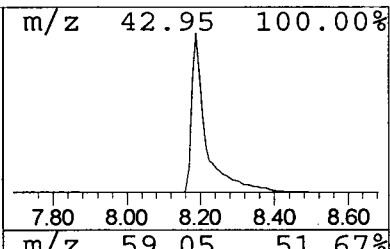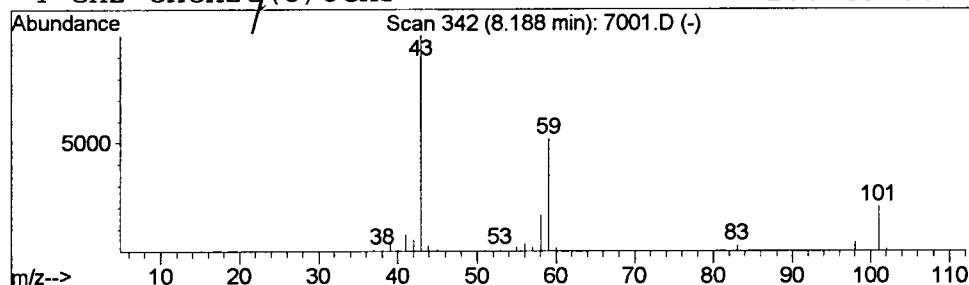

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR2402\7001.D
 Acq On : 24 Apr 2002 8:41 pm
 Sample : gc/ms scan 4/23
 Misc :
 MS Integration Params: LSCINT.P


Vial: 6
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Decanedioic acid, bis(2-ethylh Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
36.12	10.04 ug/l	996007	Perylene-d12	37.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Decanedioic acid, bis(2-ethylhexyl)	426	C26H50O4	000122-62-3	76
2		[1,1'-Biphenyl]-4-ol, 3-amino-	185	C12H11NO	001134-36-7	38
3		2,4,6(1H,3H,5H)-Pyrimidinetrione, 5	240	C12H20N2O3	051209-93-9	25
4		Pyridine, 4-[4-methoxyphenyl]-	185	C12H11NO	000000-00-0	17

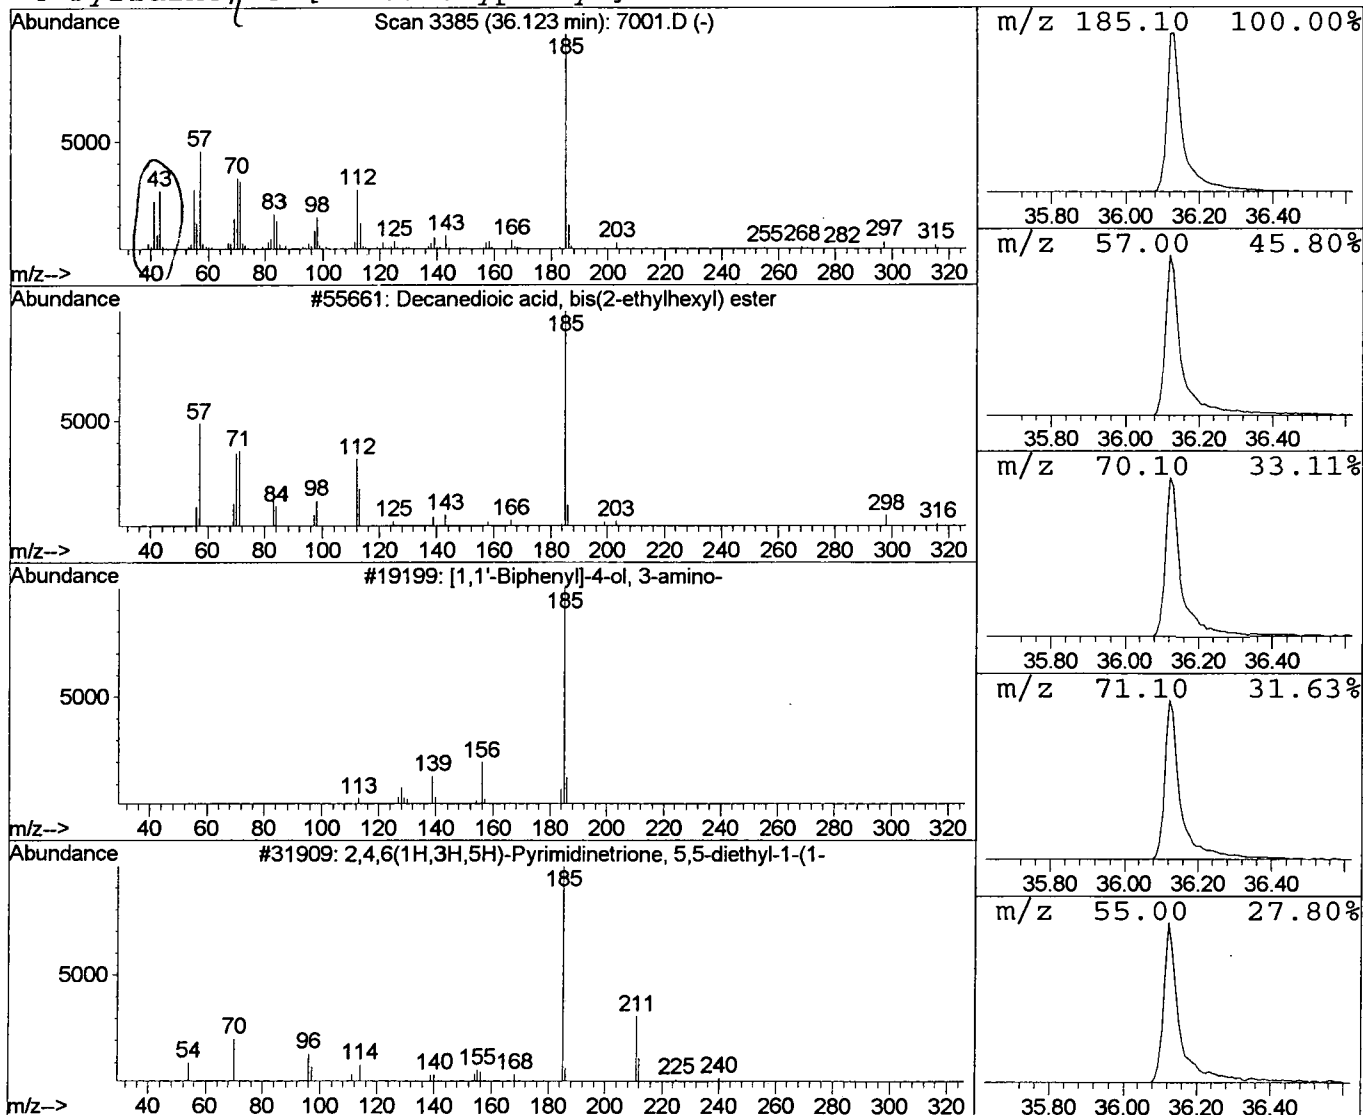

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 24 Apr 2002 8:41 pm
 Data File: C:\HPCHEM\1\DATA\APR2402\7001.D
 Name: gc/ms scan 4/23
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.19	4.0	ug/l	536659	ISTD01	12.21	2695050	20.0
Decanedioic acid, bi	36.12	10.0	ug/l	996007	ISTD06	37.87	1983450	20.0

7001.D GCMS0412.M Thu Apr 25 11:15:23 2002