

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/29/2002 Time: 15:01:04

Sample: AE07068
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/29/02 15:00 Ended: 4/29/02 15:00 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		80		
2	Surr_2,4-DDD				10.0

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/29/2002 Time: 15:01:14

Sample: AE07068
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/29/02 15:00 Ended: 4/29/02 15:00 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		80		10.0

Comments for Sample AE07068 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-29-2002 Time: 15:01:39

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

The recoveries for 5 of the 43 compounds in the LCS Standard were low.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2402\7068.D
 Acq On : 25 Apr 2002 12:34 am
 Sample : gc/ms scan 4/23 fb
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 25 8:31 2002

Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 17 11:48:30 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	530365	20.00	ug/l	-0.03
10) Naphthalene-d8	15.84	136	1929775	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.15	164	1082802	20.00	ug/l	-0.02
30) Phenanthrene-d10	25.58	188	1567770	20.00	ug/l	-0.03
39) Chrysene-d12	33.64	240	1045943	20.00	ug/l	-0.03
45) Perylene-d12	37.87	264	682329	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	23.28	209	43365	7.99	ug/L	-0.05
Spiked Amount	10.000		Recovery	=	79.90%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.90	128	185	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.62	149	836	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

7068.D GCMS0412.M Thu Apr 25 11:05:21 2002

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2402\7068.D

Vial: 10

Acq On : 25 Apr 2002 12:34 am

Operator:

Sample : gc/ms scan 4/23 fb

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 25 8:31 2002

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Apr 17 11:48:30 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.59	178	485	N.D.		
35) Anthracene	25.59	178	485	N.D.		
36) Di-n-butylphthalate	27.56	149	4144	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.64	228	2262	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.86	149	2317	N.D.		
44) Chrysene	33.64	228	2262	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	0.00	252	0	N.D.		
48) Benzo(k)fluoranthene	0.00	252	0	N.D.		
49) Benzo(a)pyrene	37.88	252	2736	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

7068.D GCMS0412.M

Thu Apr 25 11:05:22 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR2402\7068.D
Acq On : 25 Apr 2002 12:34 am
Sample : gc/ms scan 4/23 fb
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 25 8:31 2002

Vial: 10
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Apr 17 11:48:30 2002
Response via : Initial Calibration

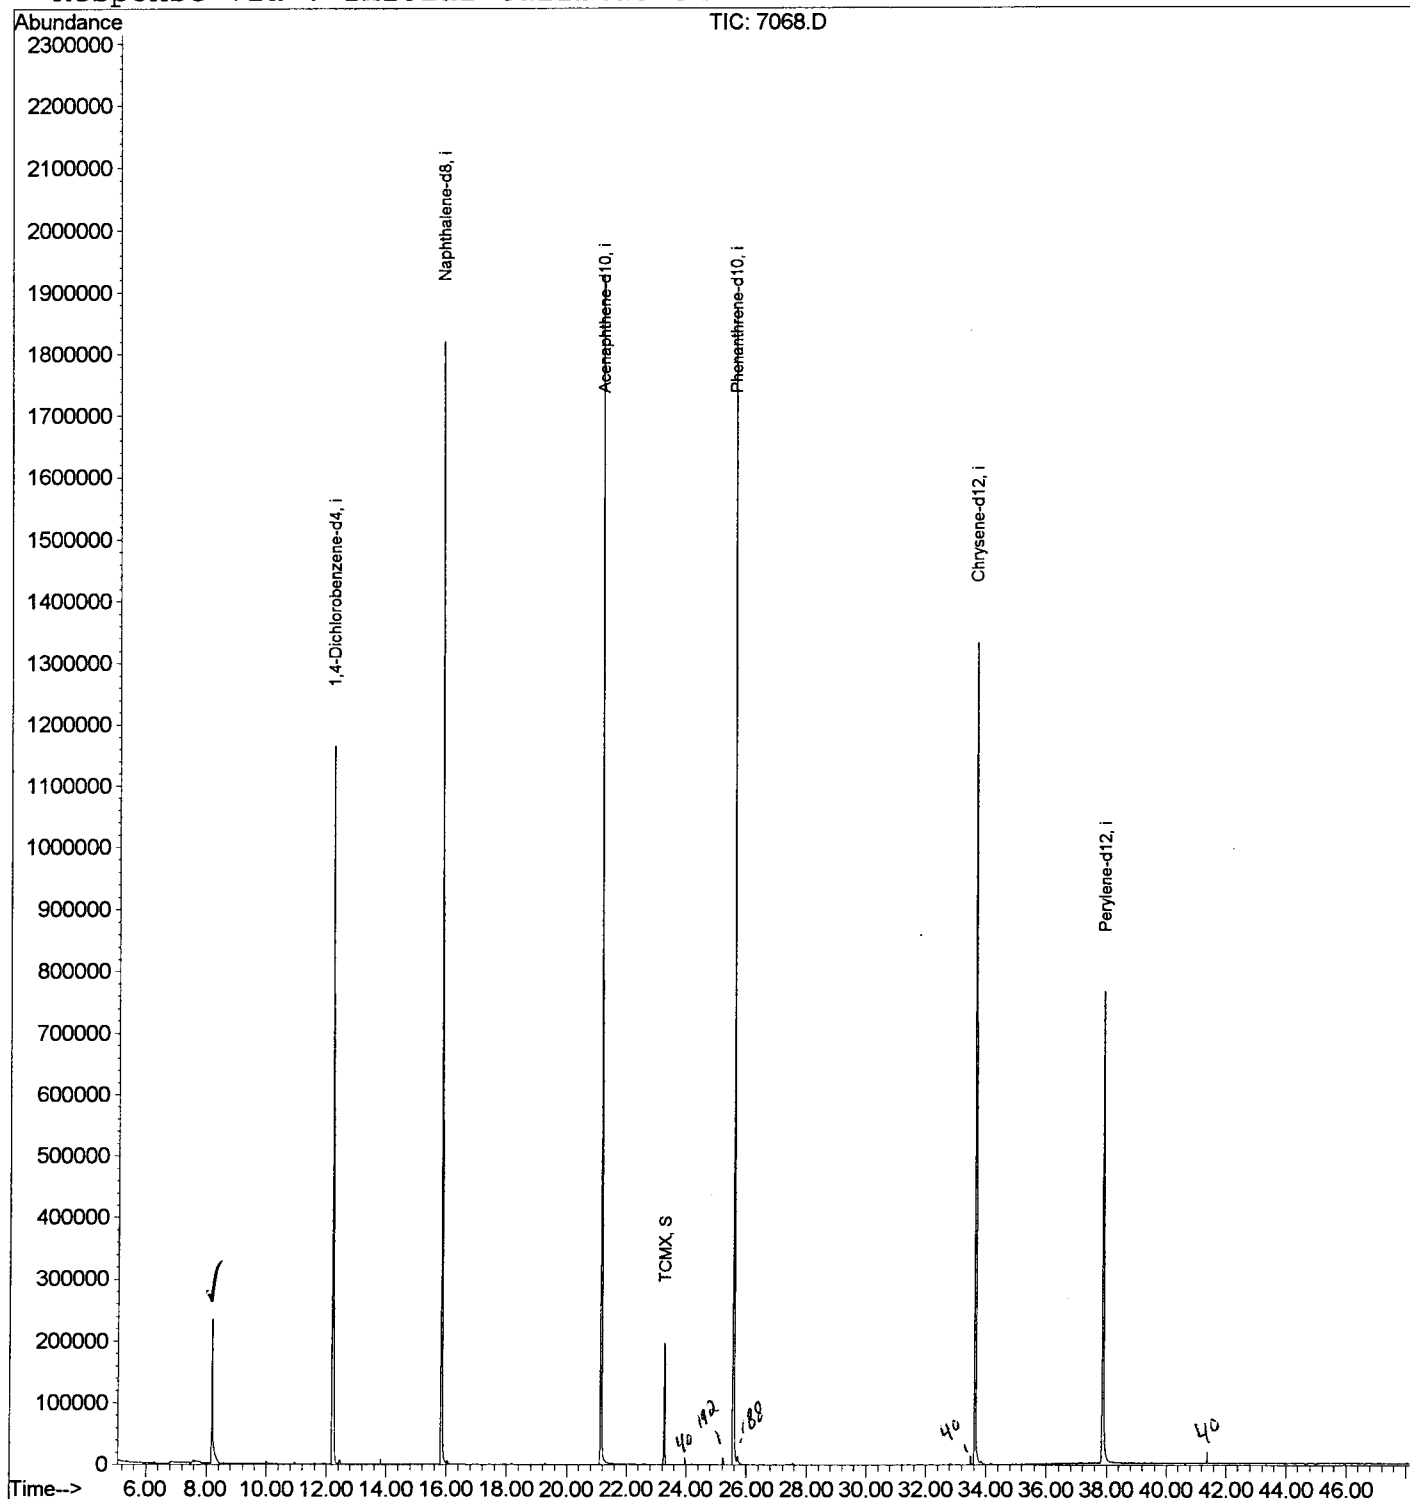

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR2402\7068.D

Vial: 10

Acq On : 25 Apr 2002 12:34 am

Operator:

Sample : gc/ms scan 4/23 fb

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.187	338	342	371	rVB	233146	577898	14.15%	2.779%
2	12.208	775	780	798	rVB	1163151	2853160	69.85%	13.720%
3	15.844	1170	1176	1190	rBV	1820240	3647766	89.31%	17.541%
4	21.150	1747	1754	1765	rBV	1928298	4084615	100.00%	19.642%
5	23.280	1978	1986	1993	rBV	197900	387386	9.48%	1.863%
6	25.584	2230	2237	2248	rBV2	1872918	3927732	96.16%	18.887%
7	33.644	3108	3115	3132	rBV	1332661	3007305	73.63%	14.461%
8	37.877	3567	3576	3600	rBV2	763763	2309755	56.55%	11.107%




Sum of corrected areas: 20795617

7068.D GCMS0412.M

Thu Apr 25 11:16:10 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR2402\7068.D
 Operator :
 Acquired : 25 Apr 2002 12:34 am using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: gc/ms scan 4/23 fb
 Misc Info :
 Vial Number: 10
 Quant File :GCMS0412.RES (RTE Integrator)

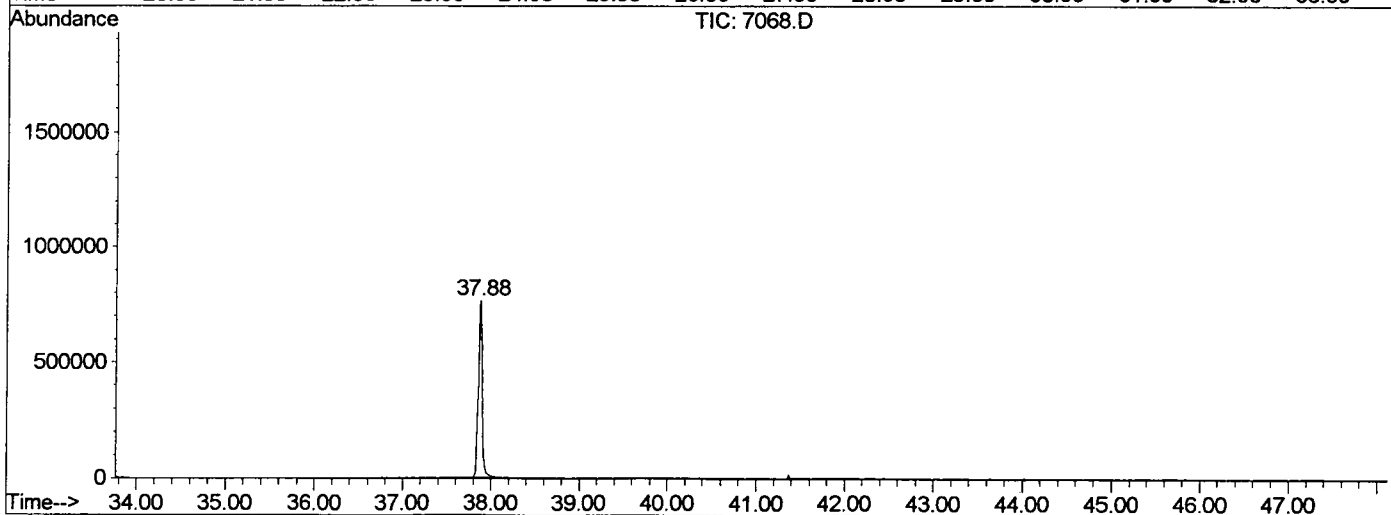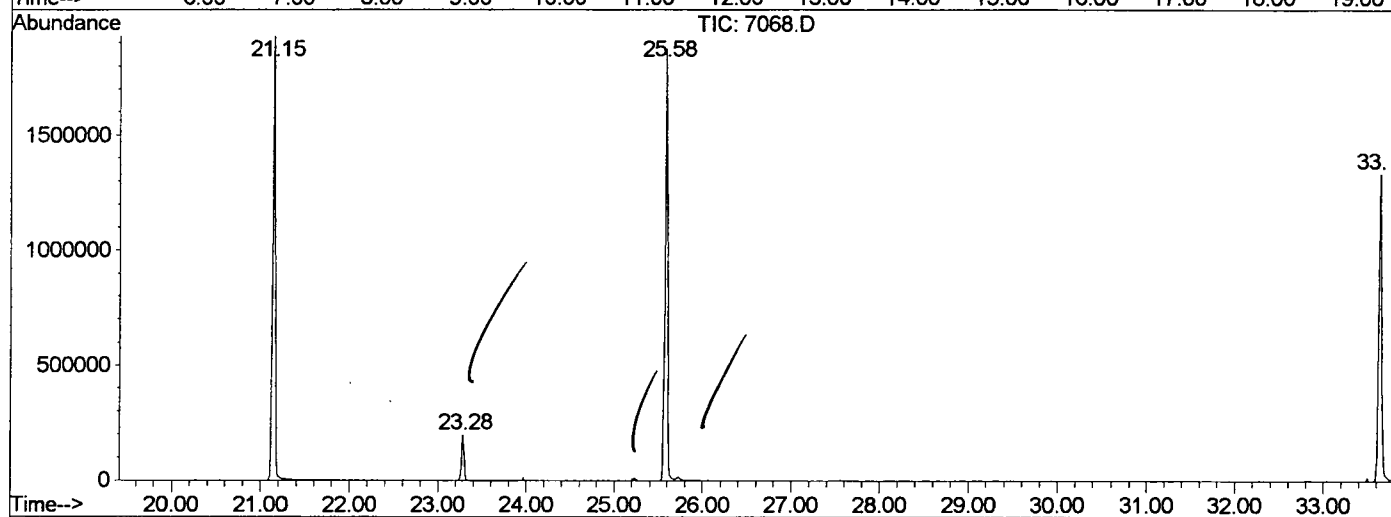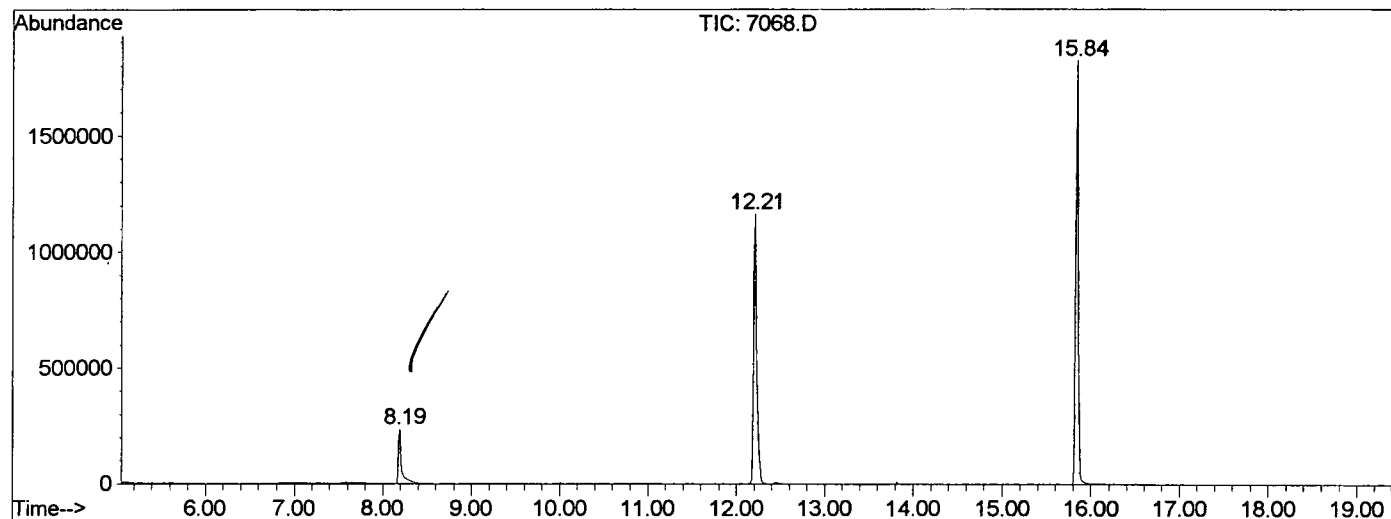

7068.D GCMS0412.M Thu Apr 25 11:16:11 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR2402\7068.D
Acq On : 25 Apr 2002 12:34 am
Sample : gc/ms scan 4/23 fb
Misc :
MS Integration Params: LSCINT.P


Vial: 10
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.19	4.05 ug/l	577898	1,4-Dichlorobenzene-d4	12.21

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33		
3	Acetic acid, cyano-, 1,1-dimethylet	141	C7H11NO2	001116-98-9	17		
4	3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9		

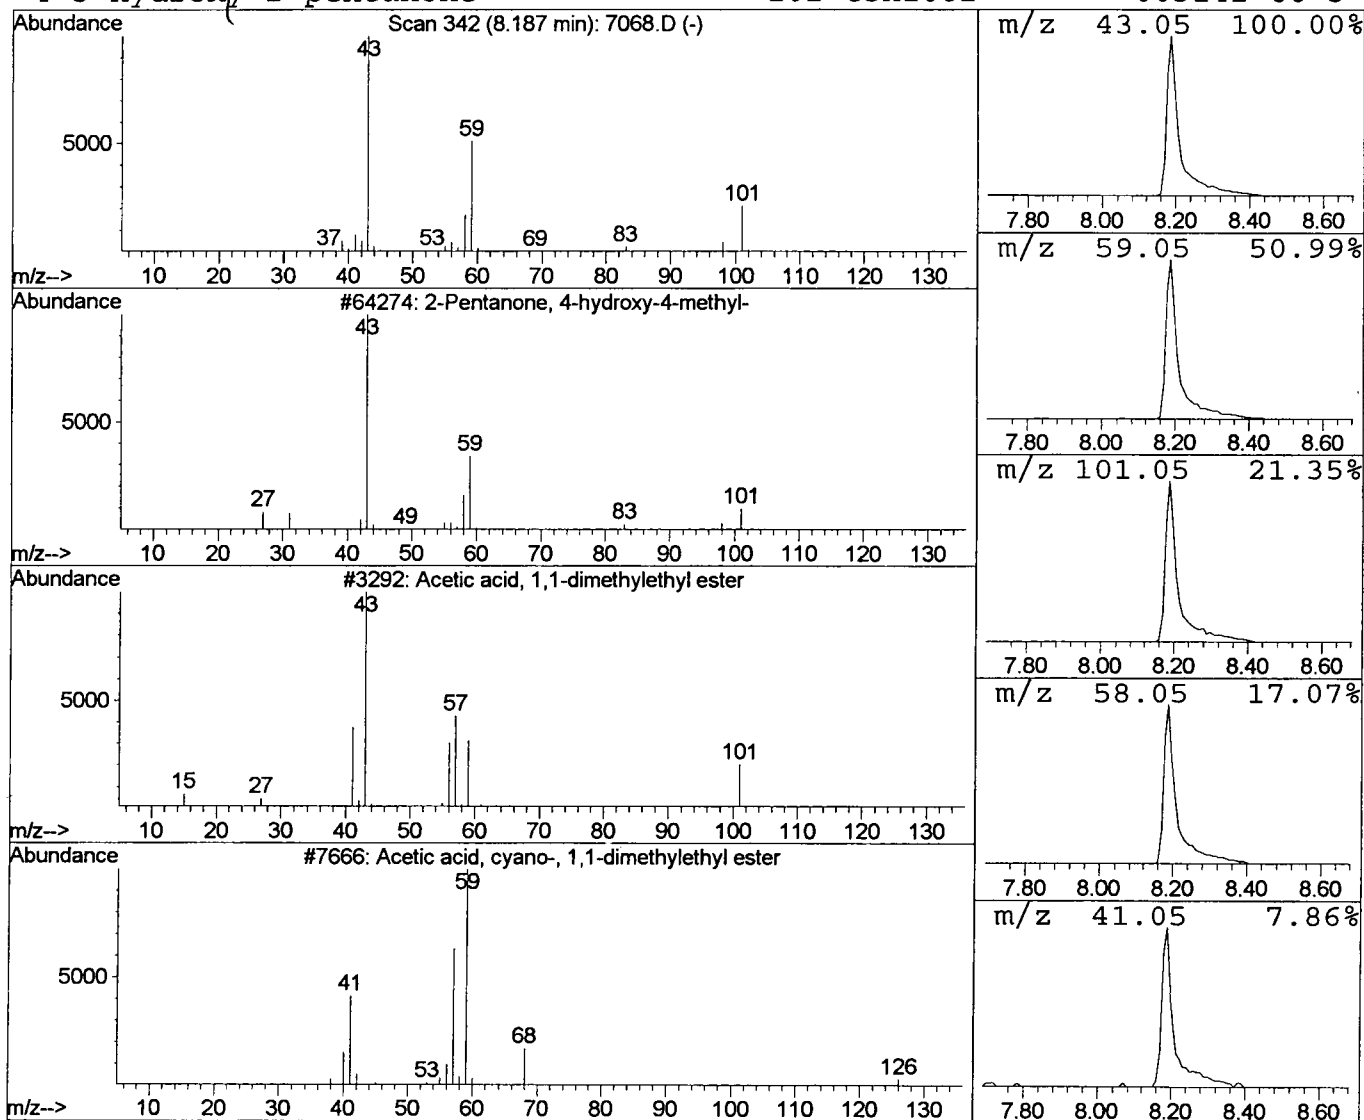

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 25 Apr 2002 12:34 am
Data File: C:\HPCHEM\1\DATA\APR2402\7068.D
Name: gc/ms scan 4/23 fb
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.19	4.1	ug/l	577898	ISTD01	12.21	2853160	20.0

7068.D GCMS0412.M Thu Apr 25 11:16:12 2002