

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1802\DFTPP.D

Acq On : 18 Apr 2002 11:31 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : 209

Multiplr: 1.00

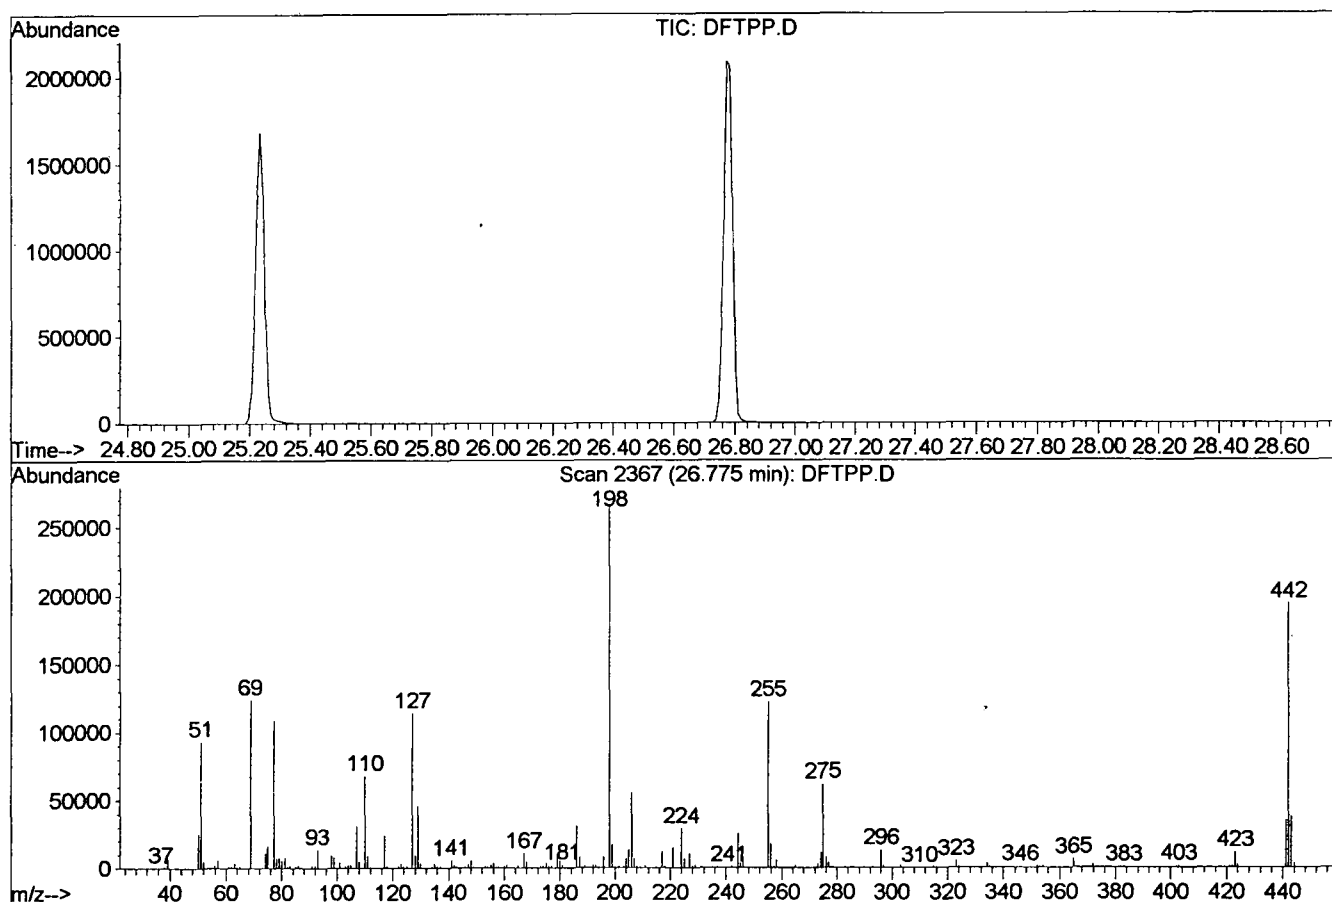

Spectrum Information: Scan 2367

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.1	93440	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.7	124192	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.9	114088	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	266048	PASS
199	198	5	9	6.6	17464	PASS
275	198	10	30	23.1	61480	PASS
365	198	1	100	2.3	6070	PASS
441	443	0.01	100	93.0	35192	PASS
442	198	40	110	72.9	193984	PASS
443	442	17	23	19.5	37840	PASS

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1802\DFTPP2.D

Acq On : 19 Apr 2002 12:36 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : 209

Multiplr: 1.00

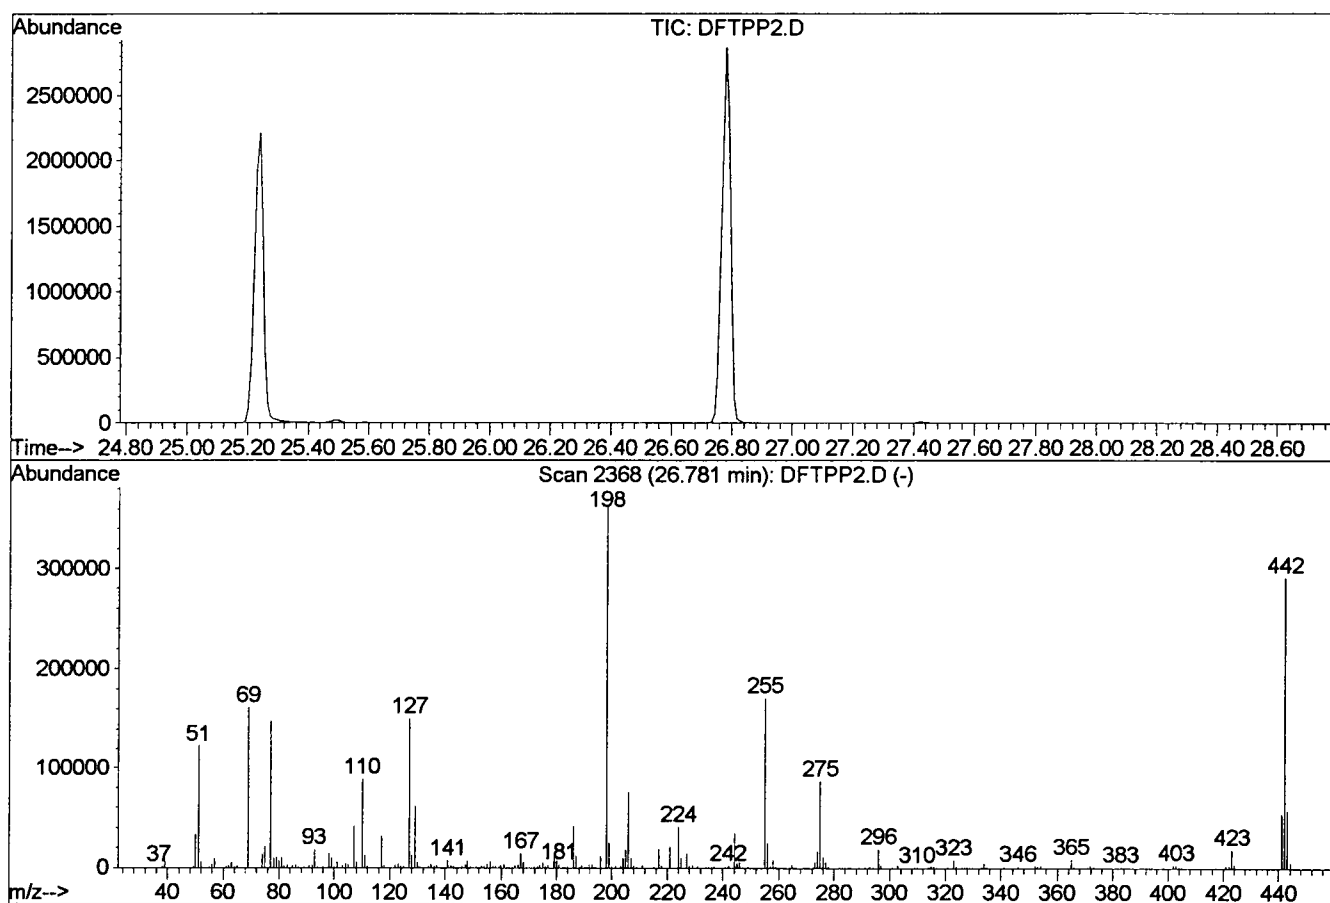

Spectrum Information: Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.8	122864	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.3	161280	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.3	150400	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	363904	PASS
199	198	5	9	6.9	25048	PASS
275	198	10	30	23.8	86720	PASS
365	198	1	100	2.4	8736	PASS
441	443	0.01	100	93.5	53632	PASS
442	198	40	110	80.0	291200	PASS
443	442	17	23	19.7	57360	PASS