

Method 508 MOD.

Date Extracted 4/25/02

Page 80

Ref GCMS - 18465 / 05/13/02

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	
L.B.		500ml		1ml			1ml	3B	7		
Ref 1					1ml			3A			
Ref 2					1ml			1A			
9683								6B			✓
9684 • F.B.								6A			✓
9764								7B			✓
9765								1B			✓
9766								8B			✓
9767								9B			
9768								7A			
9769								8A			
9770								9A			✓
Remarks											
Reviewed by <u>SPB 8/21/02</u>											
drip rate must be between 5-15 ml/min for liq-liq extractors											
drip rate -											
Extraction type - <u>SEP. FUM.</u> Solv. lot# <u>X05E10</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V46648</u>											
STANDARD	INT STD LOG#										
CALIBRATION											
REF SPIKE	<u>2279E</u>										
MDL/MORF											
Q. CHECK											
INT. STD.	<u>2286</u>										
SURROGATE	<u>GCMS ?</u>										
LPC											
ENDRIN/DDT											

Analyst A.D.
Revision 4/12/01

Verified by _____

Reviewed by SPB
Date 5/15/02


Sequence Name: C:\MSDCHEM\1\SEQUENCE\020507.S
Comment: GCMS scan
Operator: Nefliu
Data Path: C:\MSDchem\1\DATA\020507\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	508FAST	
2	Sample	2	0507C2	508SCAN1	ccv
3	Sample	3	0425LB	508SCAN1	04/25 lab blk
4	Sample	4	0426LB	508SCAN1	04/26 lab blk
5	Sample	5	0425REF1	508SCAN1	04/25 ref
6	Sample	6	0425REF2	508SCAN1	04/25 ref
7	Sample	7	0426REF1	508SCAN1	04/26 ref
8	Sample	8	0426REF2	508SCAN1	04/26 ref
9	Sample	9	09683	508SCAN1	sample
10	Sample	10	09684	508SCAN1	sample
11	Sample	11	09764	508SCAN1	sample
12	Sample	12	09765	508SCAN1	sample
13	Sample	13	09766	508SCAN1	sample
14	Sample	14	09767	508SCAN1	sample
15	Sample	15	09768	508SCAN1	sample
16	Sample	16	09769	508SCAN1	sample
17	Sample	17	09770	508SCAN1	sample
18	Sample	18	10019	508SCAN1	sample
19	Sample	19	10020	508SCAN1	sample
20	Sample	20	10021	508SCAN1	sample
21	Sample	21	10022	508SCAN1	sample
22	Sample	22	10023	508SCAN1	sample
23	Sample	23	10024	508SCAN1	sample
24	Sample	24	10025	508SCAN1	sample
25	Sample	25	10061	508SCAN1	sample
26	Sample	26	10066	508SCAN1	sample
27	Sample	27	10067	508SCAN1	sample

DFTPP

Data File : C:\MSDchem\1\DATA\020507\Snapshot\DFTPP.D Vial: 1
 Acq On : 7 May 2002 11:26 am Operator: Nefliu
 Sample : Inst : Instrume
 Misc : Multiplr: 1.00
 MS Integration Params: lscint.e
 Method : C:\MSDCHEM\1\METHODS\SCAN020507.M (RTE Integrator)
 Title : Method 508 GC/MS Scan

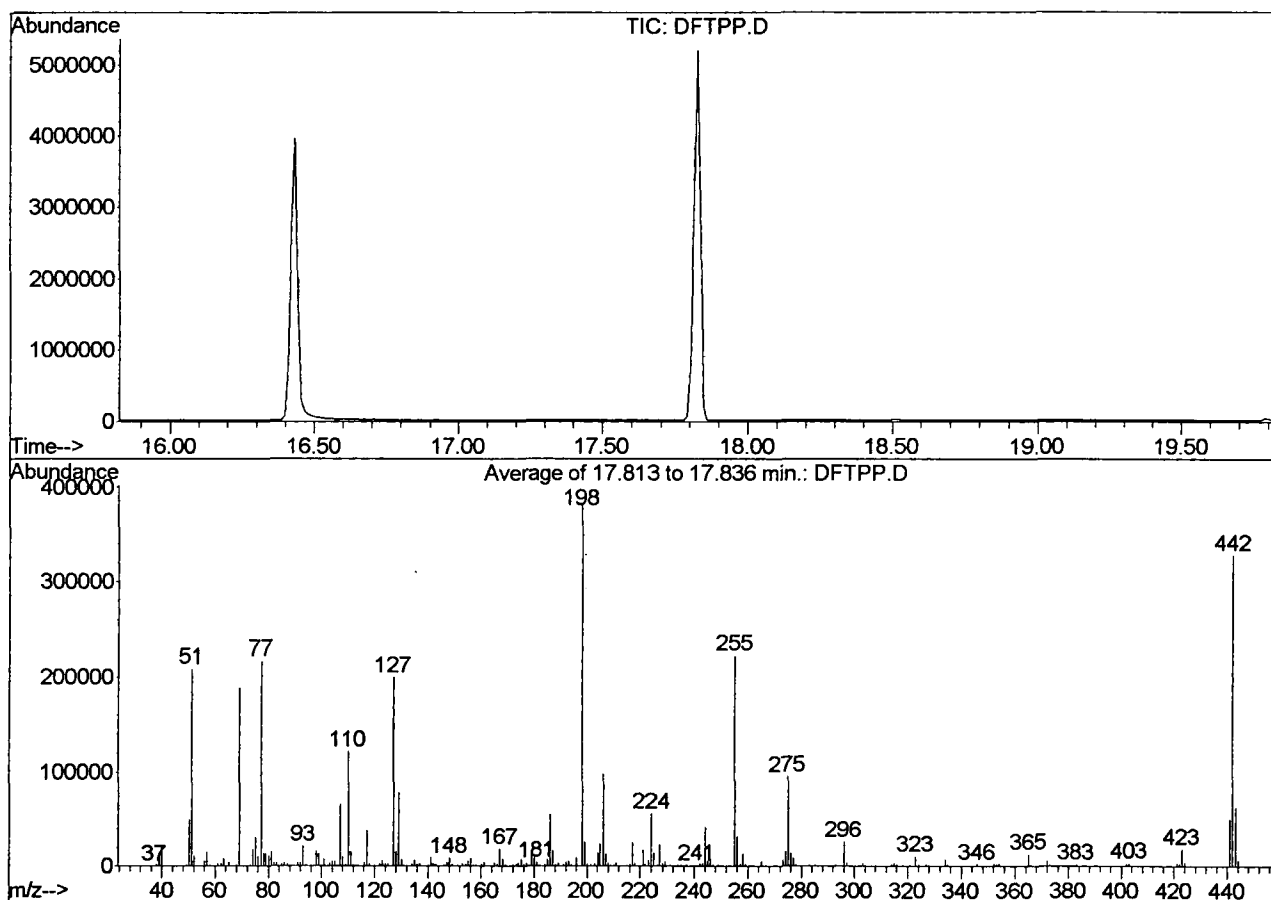

Spectrum Information: Average of 17.813 to 17.836 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	54.5	208624	PASS
68	69	0.00	2	0.8	1425	PASS
69	198	0.00	100	49.4	189221	PASS
70	69	0.00	2	0.5	1016	PASS
127	198	40	60	52.3	200162	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	382656	PASS
199	198	5	9	6.7	25746	PASS
275	198	10	30	25.0	95653	PASS
365	198	1	99	3.2	12406	PASS
441	443	1	100	79.3	49528	PASS
442	198	40	110	85.8	328341	PASS
443	442	17	23	19.0	62485	PASS