

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 05/06/2002 Time: 12:02:25

Sample: AE07485
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 5/6/02 12:01 Ended: 5/6/02 12:01 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		107		10.0

Comments for Sample AE07485 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-06-2002 Time: 12:02:51

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was low.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2502\7485.D

Vial: 8

Acq On : 27 Apr 2002 12:12 am

Operator:

Sample : gc/ms scan 4/23

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 1 11:28 2002

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Thu Apr 25 15:21:43 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0412

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	435486	20.00	ug/l	-0.03
10) Naphthalene-d8	15.84	136	1591265	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.14	164	896893	20.00	ug/l	-0.03
30) Phenanthrene-d10	25.58	188	1300143	20.00	ug/l	-0.03
39) Chrysene-d12	33.64	240	835118	20.00	ug/l	-0.04
45) Perylene-d12	37.87	264	531019	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	23.28	209	48545	10.71	ug/L	-0.05
Spiked Amount	10.000		Recovery	=	107.10%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.90	128	301	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.63	149	999	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#)=qualifier out of range (m)=manual integration

7485.D GCMS0412.M Wed May 01 11:31:28 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2502\7485.D

Vial: 8

Acq On : 27 Apr 2002 12:12 am

Operator:

Sample : gc/ms scan 4/23

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 1 11:28 2002

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Thu Apr 25 15:21:43 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0		N.D.	
34) Phenanthrene	25.59	178	323		N.D.	
35) Anthracene	25.59	178	323		N.D.	
36) Di-n-butylphthalate	27.56	149	5162		N.D.	
37) Fluoranthene	0.00	202	0		N.D.	
40) Pyrene	0.00	202	0		N.D.	
41) Butylbenzylphthalate	0.00	149	0		N.D.	
42) Benzo(a)anthracene	33.64	228	1805		N.D.	
43) Bis(2-ethylhexyl)phthalate	33.86	149	1352		N.D.	
44) Chrysene	33.64	228	1804		N.D.	
46) Di-n-Octylphthalate	0.00	149	0		N.D.	
47) Benzo(b)fluoranthene	0.00	252	0		N.D.	
48) Benzo(k)fluoranthene	0.00	252	0		N.D.	
49) Benzo(a)pyrene	37.88	252	1983		N.D.	
50) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
51) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
52) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

(#) = qualifier out of range (m) = manual integration

7485.D GCMS0412.M Wed May 01 11:31:29 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR2502\7485.D
Acq On : 27 Apr 2002 12:12 am
Sample : gc/ms scan 4/23
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 1 11:28 2002

Vial: 8
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu Apr 25 15:21:43 2002
Response via : Initial Calibration

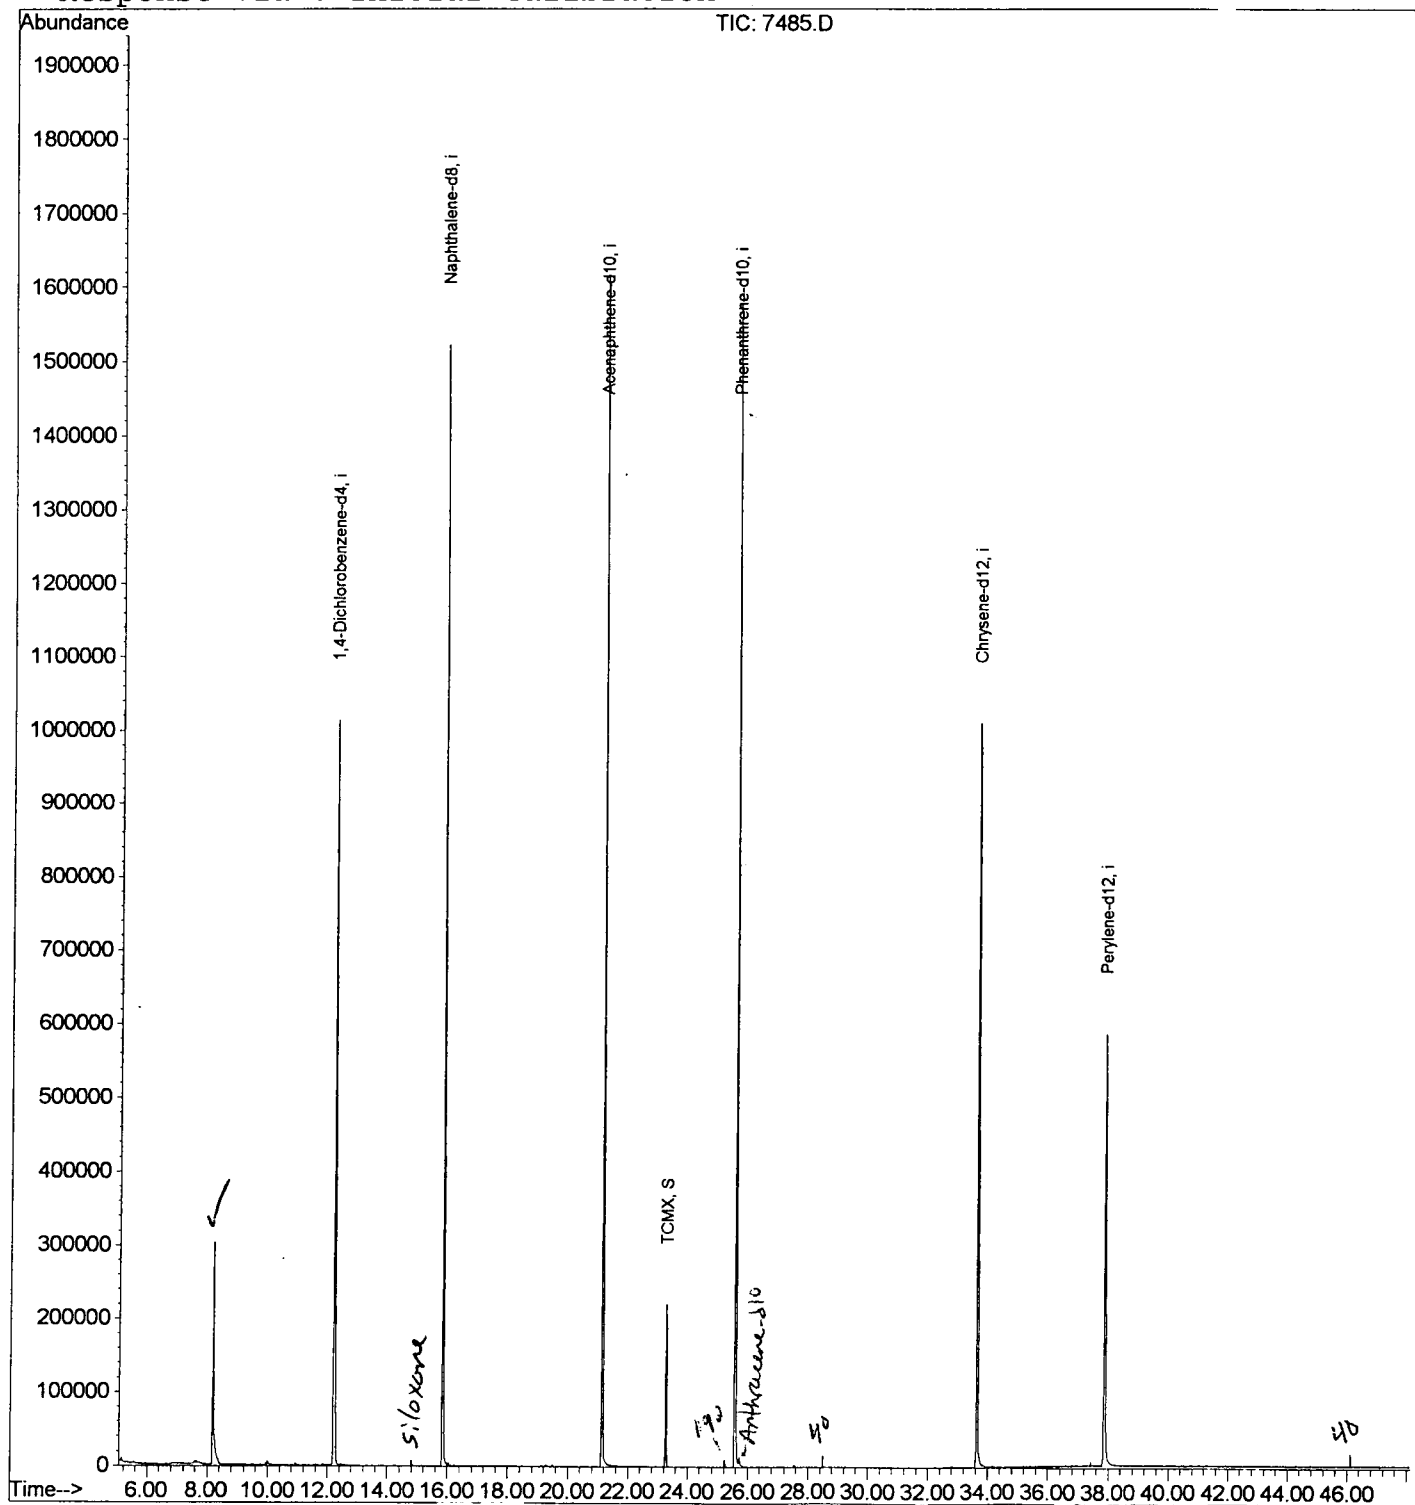

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR2502\7485.D
 Acq On : 27 Apr 2002 12:12 am
 Sample : gc/ms scan 4/23
 Misc :
 MS Integration Params: LSCINT.P

Vial: 8
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.187	338	342	367	rBV	301773	737598	21.47%	4.235%
2	12.208	775	780	795	rVB	1011415	2388203	69.52%	13.713%
3	15.844	1170	1176	1192	rBV	1522314	3023952	88.02%	17.364%
4	21.141	1747	1753	1772	rBV	1616357	3435365	100.00%	19.726%
5	23.280	1979	1986	1992	rBV	220472	431371	12.56%	2.477%
6	25.584	2231	2237	2249	rBV2	1575827	3259565	94.88%	18.717%
7	33.635	3108	3114	3131	rBV2	1011620	2382408	69.35%	13.680%
8	37.867	3567	3575	3597	rBV2	584674	1756795	51.14%	10.088%

Sum of corrected areas: 17415257

7485.D GCMS0412.M Thu May 02 05:34:30 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR2502\7485.D
 Operator :
 Acquired : 27 Apr 2002 12:12 am using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: gc/ms scan 4/23
 Misc Info :
 Vial Number: 8
 Quant File :GCMS0412.RES (RTE Integrator)

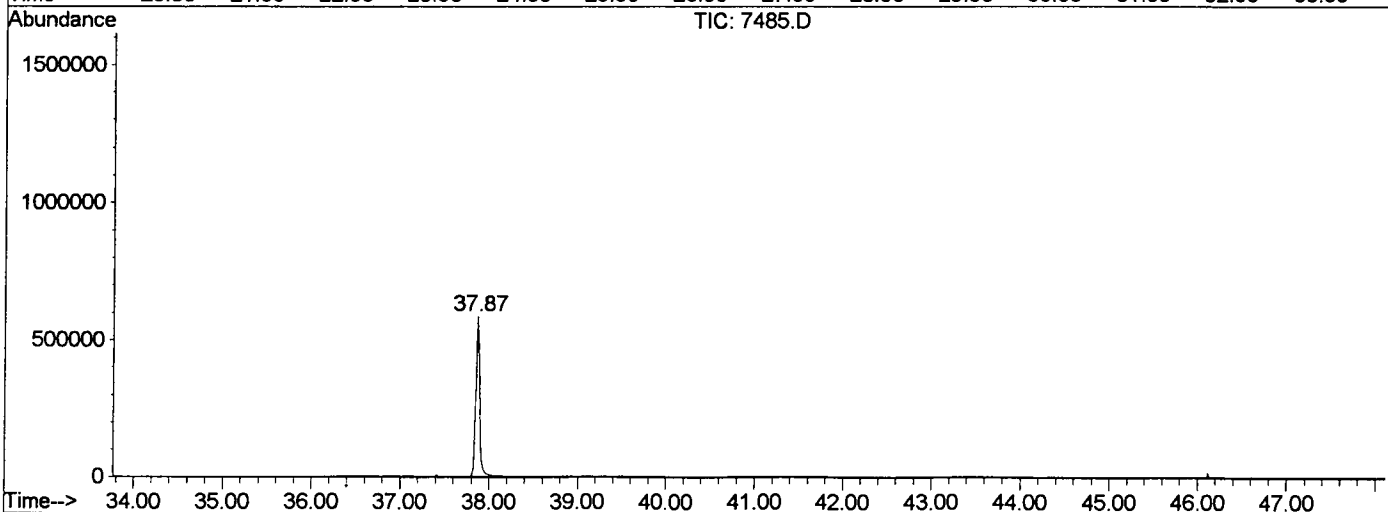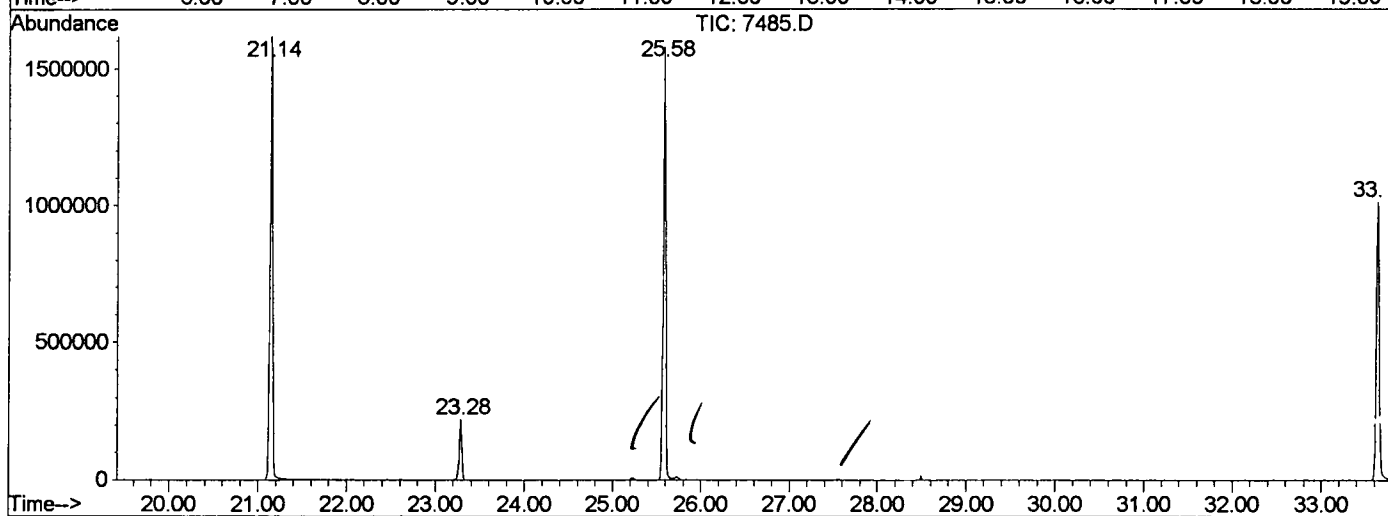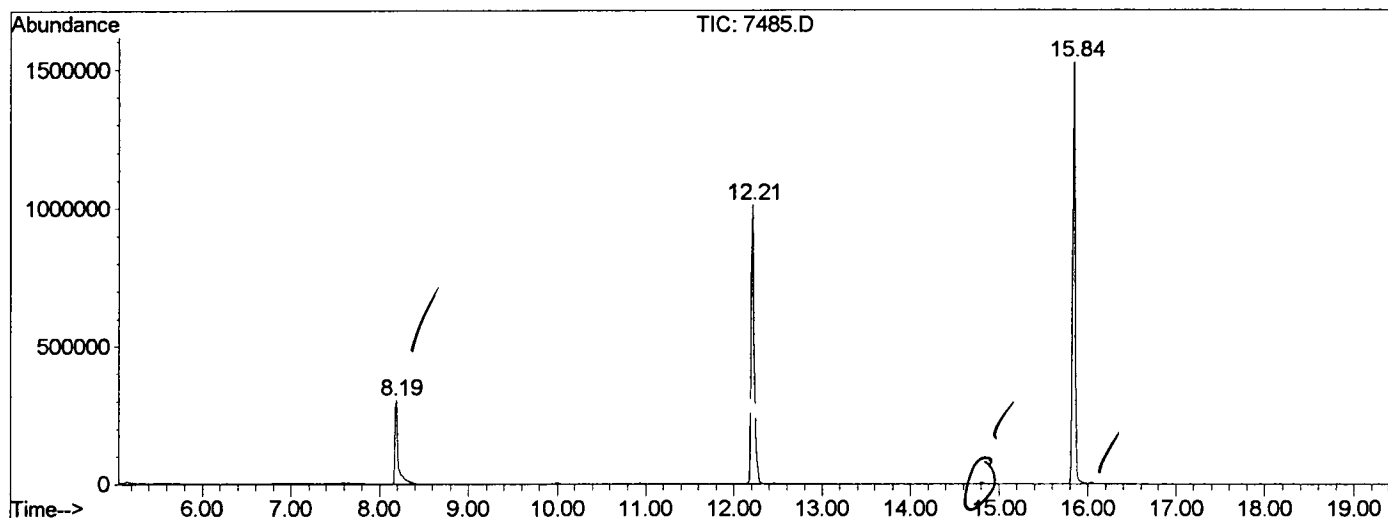

7485.D GCMS0412.M Thu May 02 05:34:30 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR2502\7485.D
Acq On : 27 Apr 2002 12:12 am
Sample : gc/ms scan 4/23
Misc :
MS Integration Params: LSCINT.P


Vial: 8
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.19	6.18 ug/l	737598	1,4-Dichlorobenzene-d4	12.21

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33
3			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
4			5-Hexen-2-one	98	C6H10O	000109-49-9	9

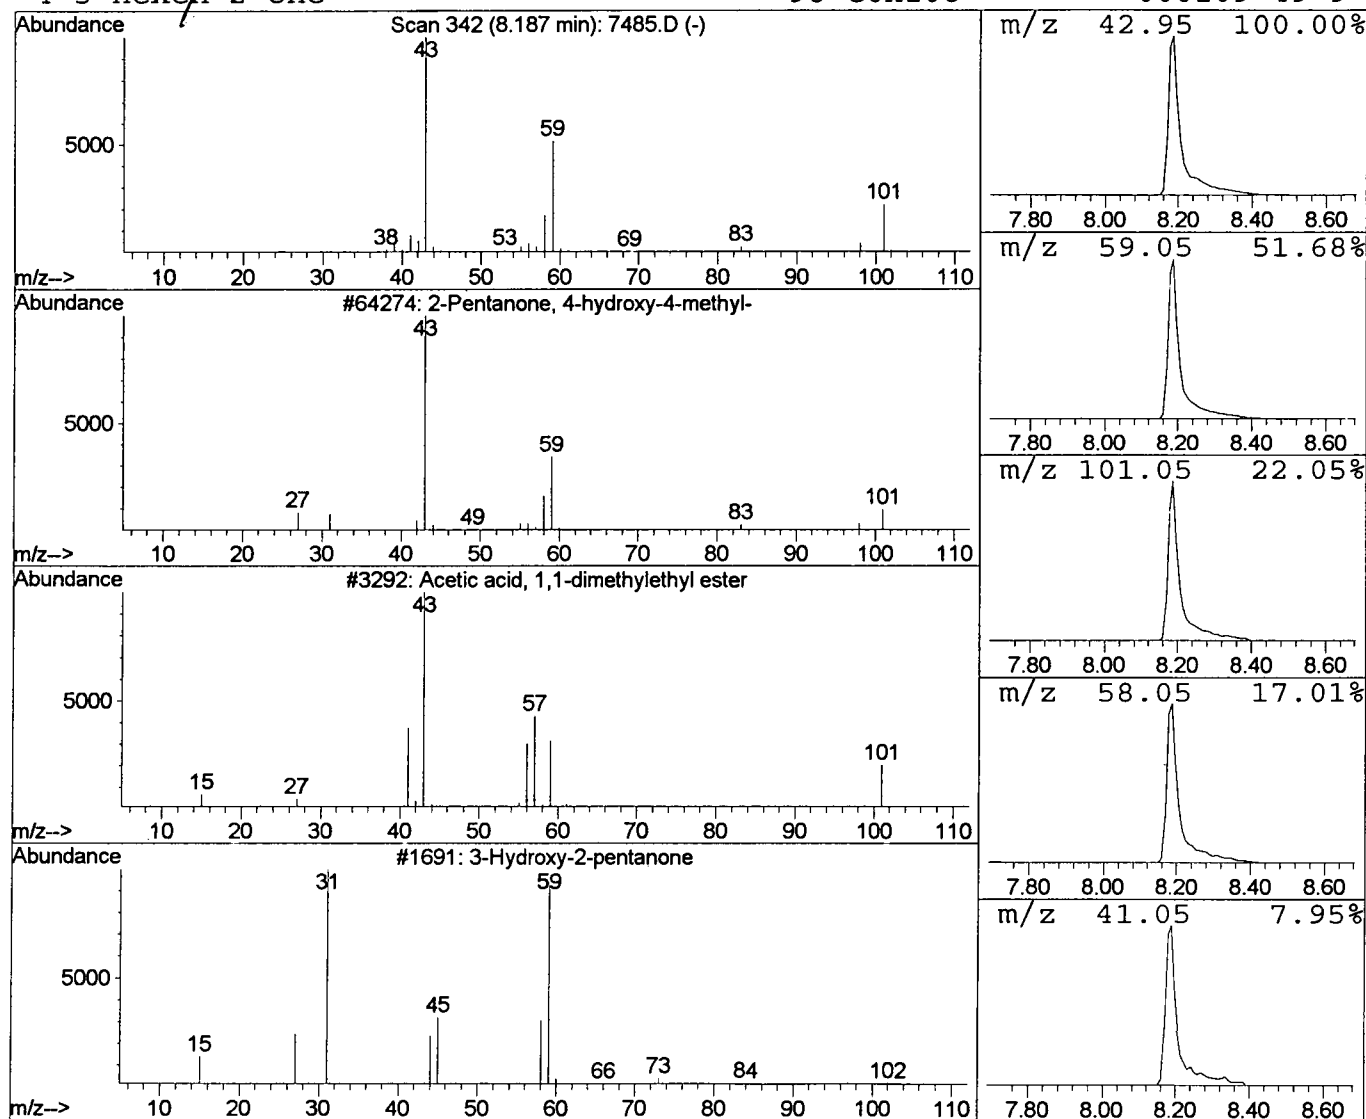

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 27 Apr 2002 12:12 am
 Data File: C:\HPCHEM\1\DATA\APR2502\7485.D
 Name: gc/ms scan 4/23
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.19	6.2	ug/l	737598	ISTD01	12.21	2388200	20.0
7485.D GCMS0412.M	Thu May 02 05:34:32 2002							