

Data File : C:\HPCHEM\1\DATA\APR2502\9333.D
 Acq On : 25 Apr 2002 9:28 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 26 7:46 2002

Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Thu Apr 25 15:21:43 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

*original
LSC poor
sample OK*

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	673507	20.00	ug/l	-0.03
10) Naphthalene-d8	15.85	136	2467783	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.15	164	1394416	20.00	ug/l	-0.03
30) Phenanthrene-d10	25.59	188	2060394	20.00	ug/l	-0.03
39) Chrysene-d12	33.65	240	1300663	20.00	ug/l	-0.03
45) Perylene-d12	37.87	264	801905	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	23.28	209	47930	^{8.54} 6.80	ug/L	-0.05
Spiked Amount	10.000		Recovery	=	68.00%	85%
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	5.44	74	107	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.89	128	284	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	21.44	165	604	N.D.	
25) Diethylphthalate	22.62	149	1393	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

9333.D GCMS0412.M Fri Apr 26 07:46:51 2002

Page 1

Data File : C:\HPCHEM\1\DATA\APR2502\9333.D
 Acq On : 25 Apr 2002 9:28 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 26 7:46 2002

Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Thu Apr 25 15:21:43 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.64	178	370	N.D.		
35) Anthracene	25.66	178	370	N.D.		
36) Di-n-butylphthalate	27.55	149	5051	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.64	228	2853	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.86	149	2350	N.D.		
44) Chrysene	33.64	228	2853	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	0.00	252	0	N.D.		
48) Benzo(k)fluoranthene	0.00	252	0	N.D.		
49) Benzo(a)pyrene	37.88	252	3363	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

9333.D GCMS0412.M Fri Apr 26 07:46:52 2002


Page 2

Data File : C:\HPCHEM\1\DATA\APR2502\9333.D
Acq On : 25 Apr 2002 9:28 pm
Sample : gc/ms scan 4/18
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 26 7:46 2002

Vial: 10
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu Apr 25 15:21:43 2002
Response via : Initial Calibration

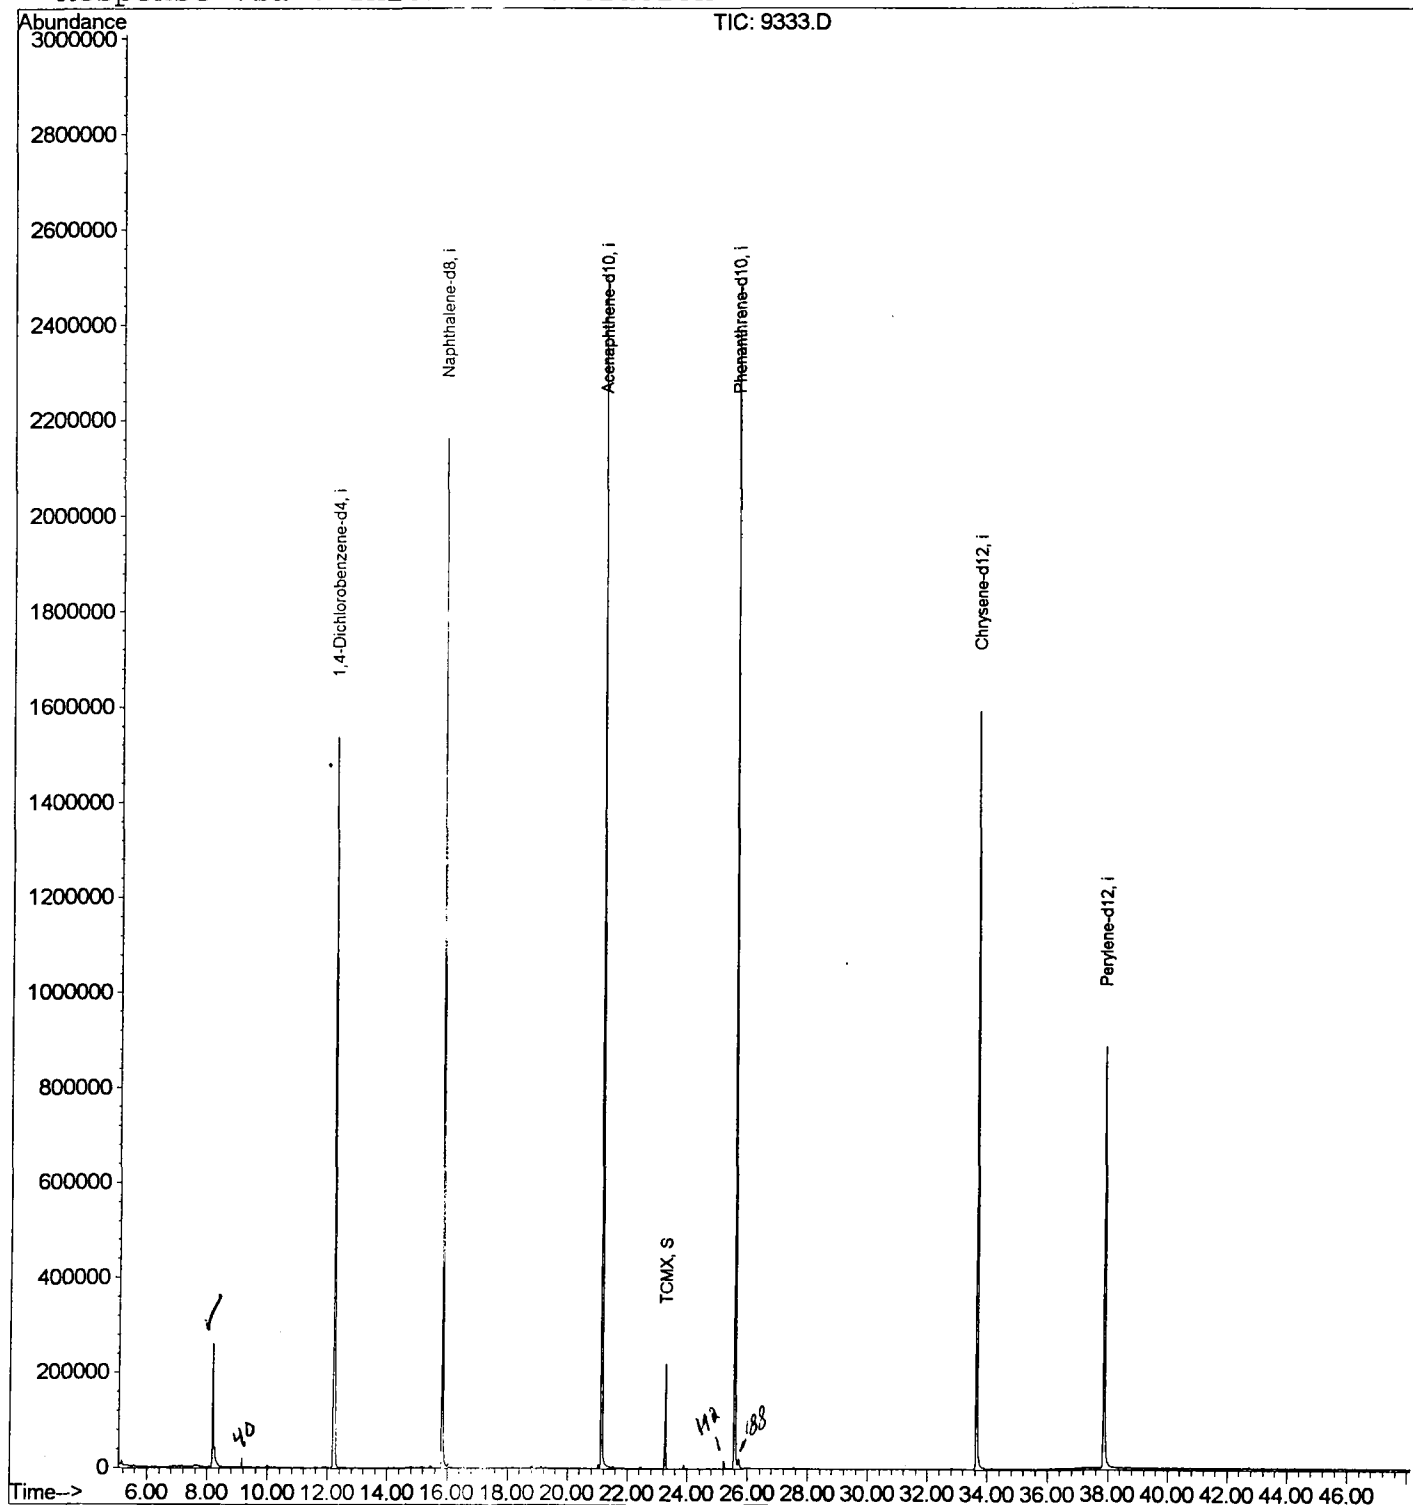

9333.D GCMS0412.M

Fri Apr 26 07:46:54 2002

Page 3

Data File : C:\HPCHEM\1\DATA\APR2502\9333.D
 Acq On : 25 Apr 2002 9:28 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: LSCINT.P

Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.183	339	342	347	rBV	258518	512834	9.68%	1.964%
2	12.213	775	781	798	rVB	1535298	3611501	68.20%	13.834%
3	15.848	1170	1177	1193	rBV	2162651	4652874	87.87%	17.823%
4	21.145	1748	1754	1775	rBV	2506212	5295227	100.00%	20.283%
5	23.284	1979	1987	1992	rBV	219688	432976	8.18%	1.659%
6	25.589	2231	2238	2249	rBV2	2389920	5146192	97.19%	19.712%
7	33.649	3108	3116	3134	rBV	1593457	3748811	70.80%	14.360%
8	37.872	3566	3576	3596	rBV2	884630	2706008	51.10%	10.365%

Sum of corrected areas: 26106423

9333.D GCMS0412.M Fri Apr 26 08:18:55 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR2502\9333.D
 Operator :
 Acquired : 25 Apr 2002 9:28 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: gc/ms scan 4/18
 Misc Info :
 Vial Number: 10
 Quant File :GCMS0412.RES (RTE Integrator)

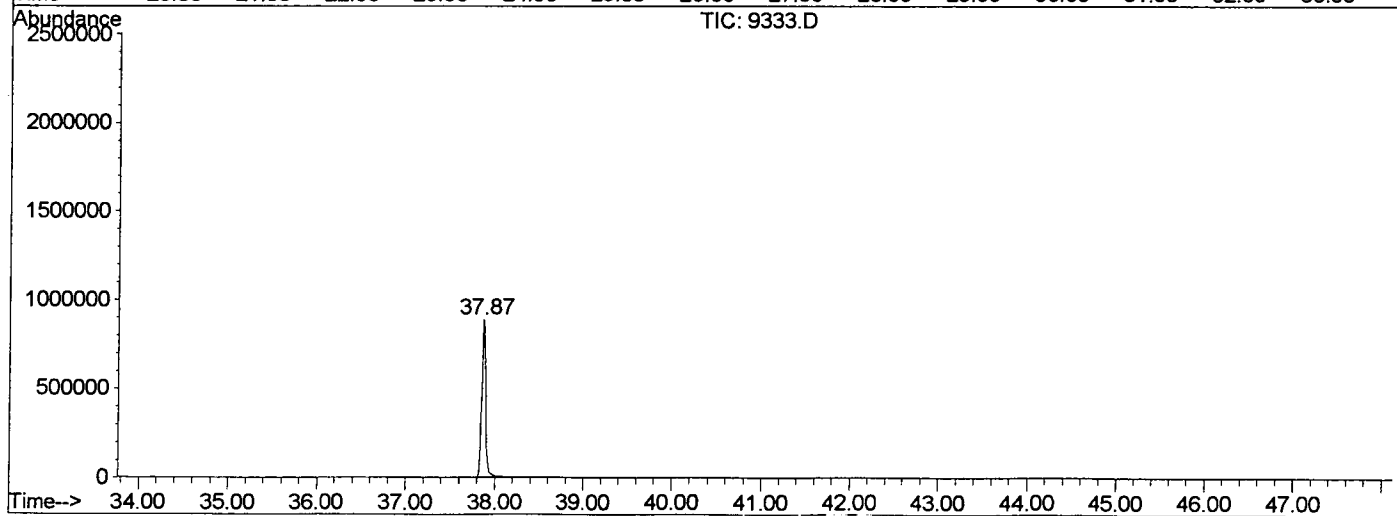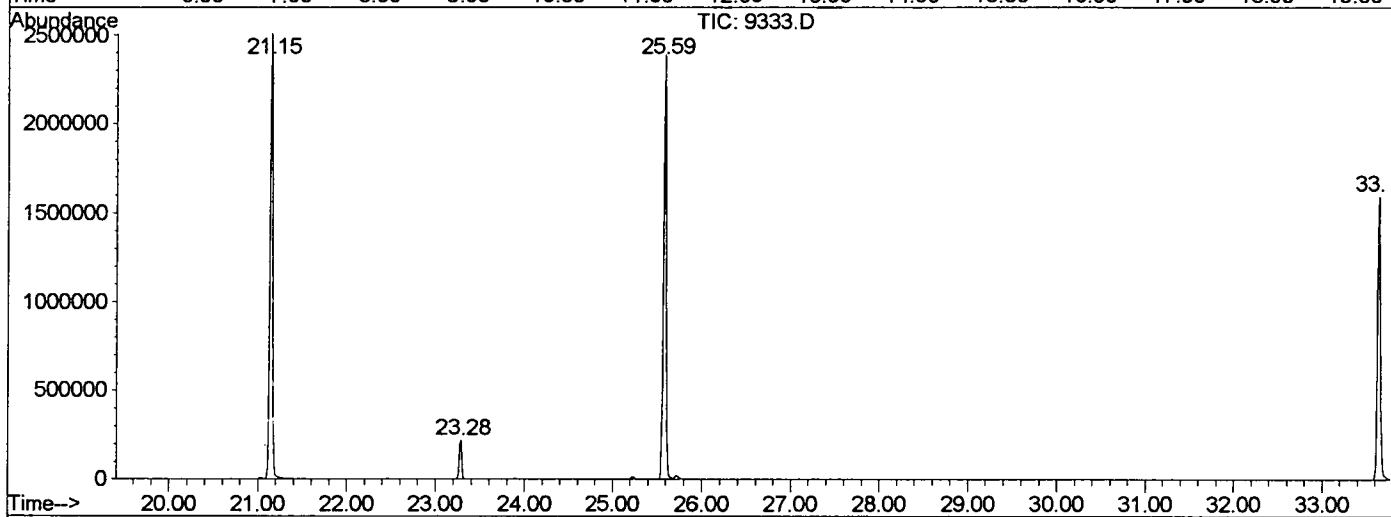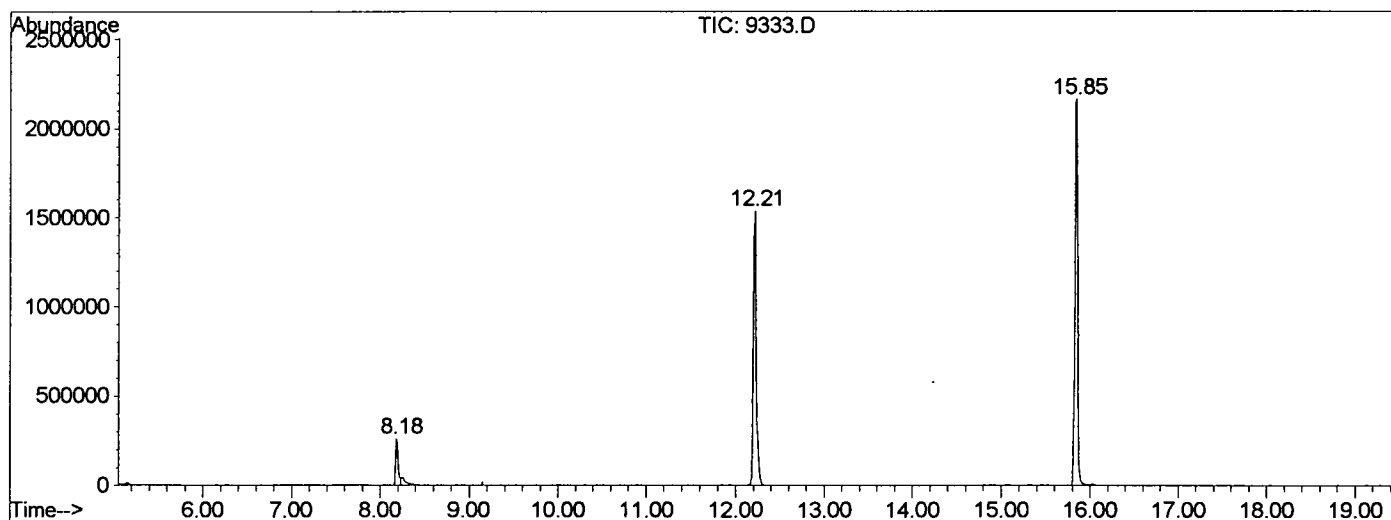

9333.D GCMS0412.M Fri Apr 26 08:18:56 2002

Data File : C:\HPCHEM\1\DATA\APR2502\9333.D
 Acq On : 25 Apr 2002 9:28 pm
 Sample : gc/ms scan 4/18
 Misc :
 MS Integration Params: LSCINT.P


Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.18	2.84 ug/l	512834	1,4-Dichlorobenzene-d4	12.21

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	39
2			CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	10
3			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
4			Acetone	58	C3H6O	000067-64-1	9

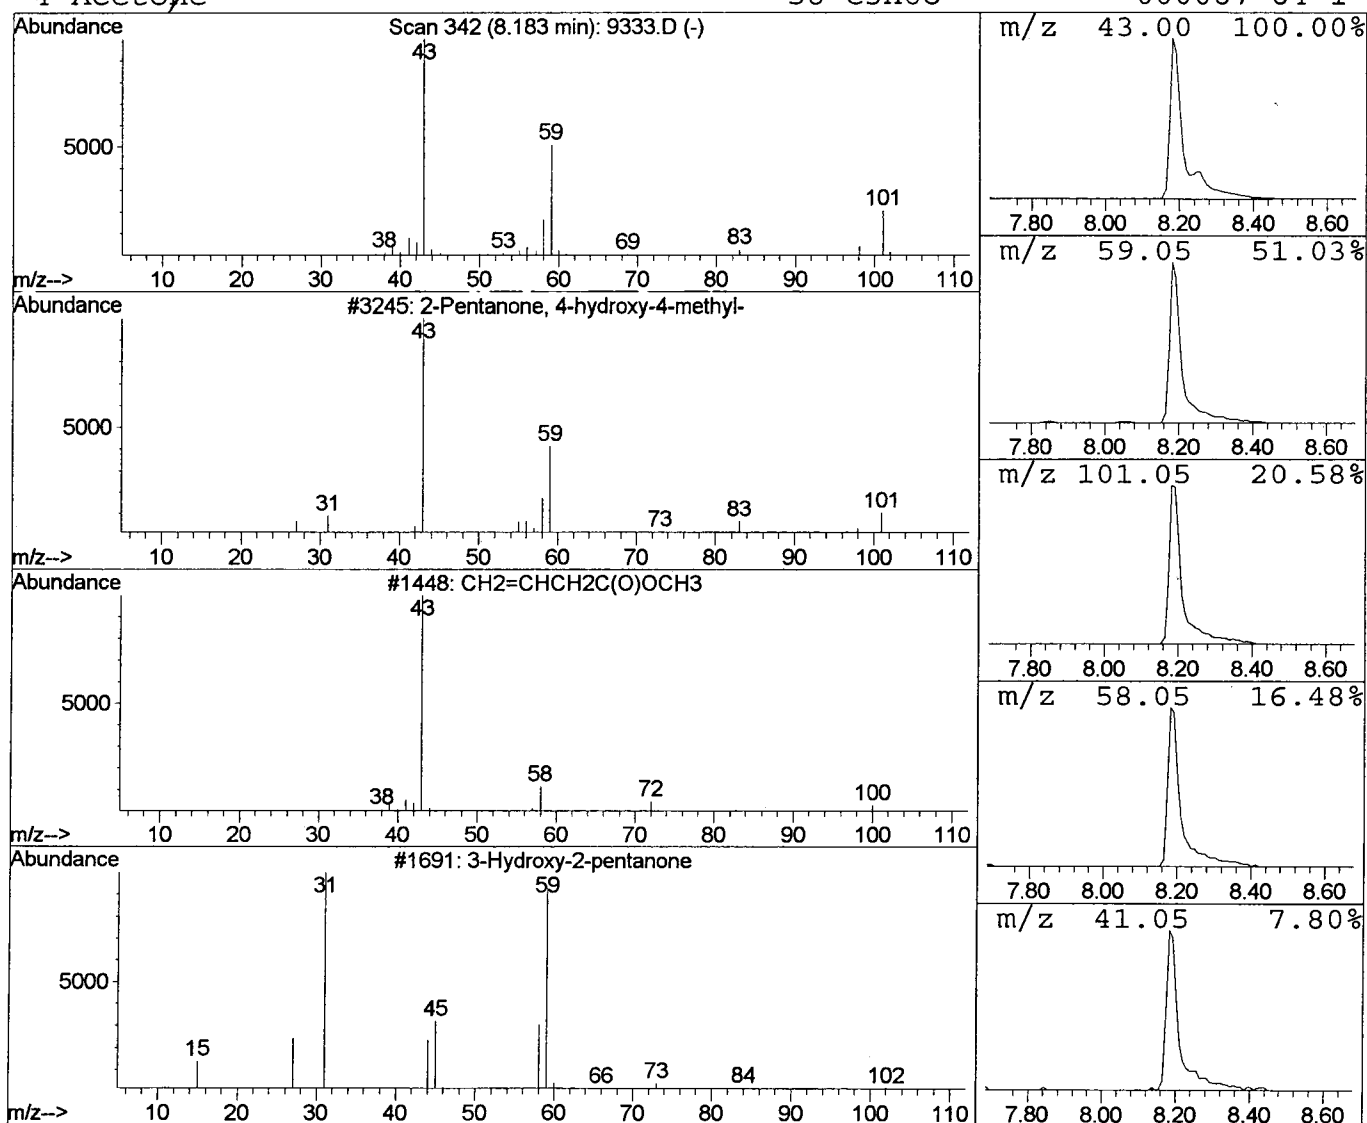

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 25 Apr 2002 9:28 pm
Data File: C:\HPCHEM\1\DATA\APR2502\9333.D
Name: gc/ms scan 4/18
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.18	2.8	ug/l	512834	ISTD01	12.21	3611500	20.0
9333.D GCMS0412.M	Fri Apr 26	08:18:57	2002					