

Page 67

~~#CCMS-19181~~

[illegible]

Analyst K. B.
revision 4/12/01

Verified by My

Reviewed by _____
Date _____

DFTPP

Data File : C:\HPCHEM\1\DATA\APR2502\DFTPP.D

Acq On : 25 Apr 2002 8:35 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : 209

Multiplr: 1.00

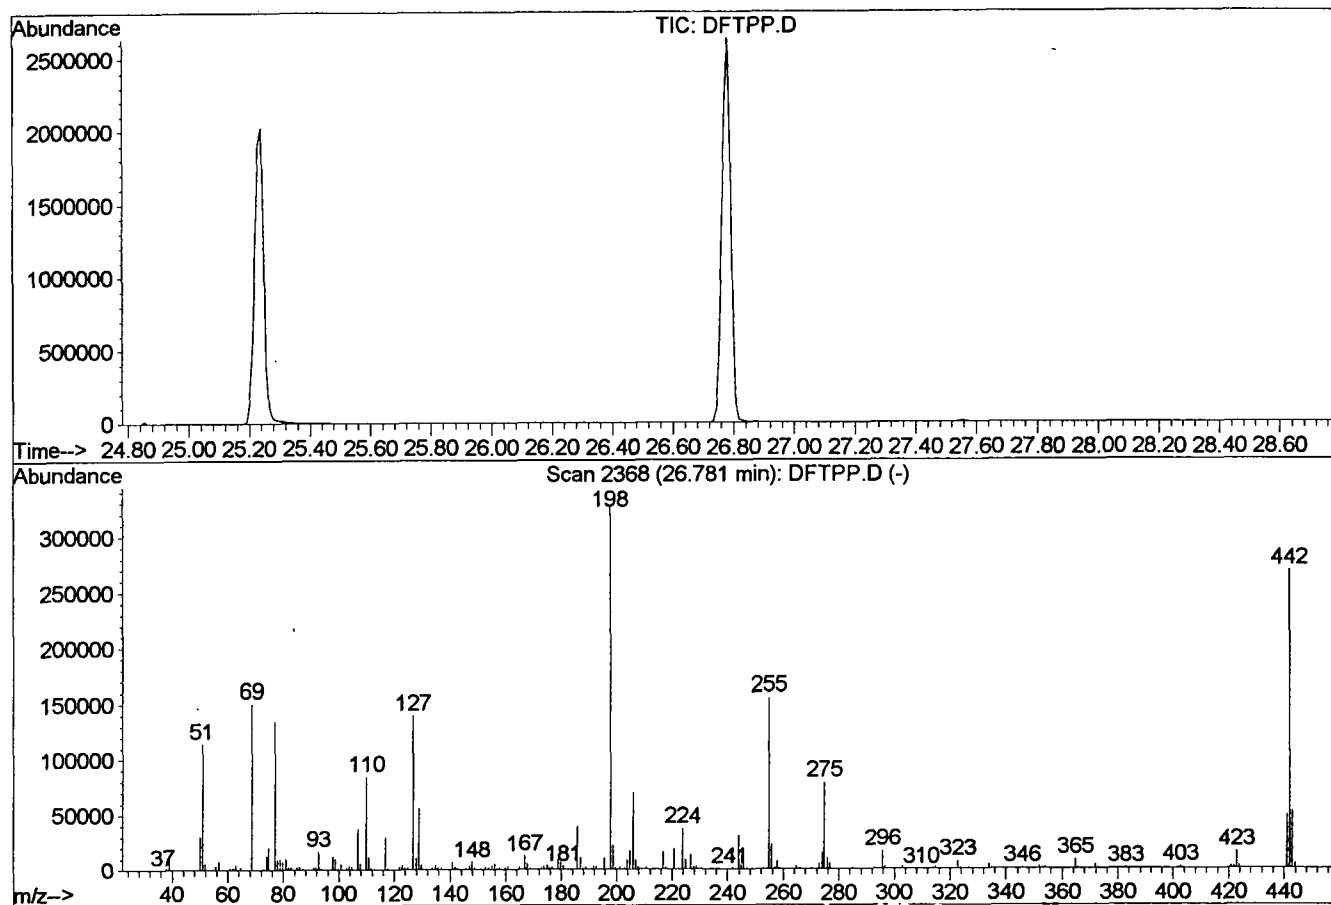

Spectrum Information: Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.9	114528	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.9	150499	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.7	140041	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	328219	PASS
199	198	5	9	6.8	22440	PASS
275	198	10	30	24.1	79007	PASS
365	198	1	100	2.6	8689	PASS
441	443	0.01	100	93.4	48874	PASS
442	198	40	110	81.9	268761	PASS
443	442	17	23	19.5	52341	PASS

DFTPP.D GCMS0412.M

Thu Apr 25 14:44:02 2002