

REF

#GCMs - 18396

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	LAB BLANK	500ml		1ml	1ml		1ml	6A	7			
	REF1				1ML			6B				
	REF2				1ML			7A				
10137								7B				
10159								8A				
10160								8B				
10161								6A				
10162								6B				
10163								7A				
10164								7B				
10165								8A				
10166								8B				
Remarks												
REF1 SEP FUNNEL VERY LEAKY												
Reviewed by, <i>JB 8/21/02</i>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - <i>SEP FUNNEL</i>		Solv. lot# <i>X05E10</i>		NaCl lot# <i>V39614</i>		Na2SO4 lot# <i>V46648</i>						
STANDARD	INT STD LOG#											
CALIBRATION	<i>HP050202</i>											
REF SPIKE	<i>2279E</i>											
MDL/MDRF												
Q. CHECK	<i>15042902</i>											
INT. STD.	<i>050702</i>											
SURROGATE	<i>GCMS</i>											
LPC												
ENDRIN/DDT												

Analyst BN
revision 4/12/01

Verified byReviewed by _____
Date _____

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAY0602.S
 Comment:
 Operator:
 Data Path: C:\HPCHEM\1\DATA\MAY0602\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0501	
2	Sample	2	CAL160	GCMS0501	
3	Sample	3	LB	GCMS0501	GC/MS SCAN 4/24
4	Sample	4	REF1	GCMS0501	GC/MS SCAN 4/24
5	Sample	5	REF2	GCMS0501	GC/MS SCAN 4/24
6	Sample	27	SURR	GCMS0501	
7	Sample	95	CAL10	GCMS0501	
8	Sample	96	CAL20	GCMS0501	
9	Sample	97	CAL40	GCMS0501	
10	Sample	98	CAL80	GCMS0501	
11	Sample	99	CAL160A	GCMS0501	
12	Sample	100	CAL200	GCMS0501	
13	Sample	6	9098	GCMS0501	
14	Sample	7	8936	GCMS0501	GC/MS SCAN 4/24
15	Sample	8	8951	GCMS0501	GC/MS SCAN 4/24
16	Sample	9	8952	GCMS0501	GC/MS SCAN 4/24
17	Sample	10	9652	GCMS0501	GC/MS SCAN 4/24 FB
18	Sample	11	9653	GCMS0501	GC/MS SCAN 4/24
19	Sample	12	9654	GCMS0501	GC/MS SCAN 4/24
20	Sample	13	9673	GCMS0501	GC/MS SCAN 4/24
21	Sample	14	9674	GCMS0501	GC/MS SCAN 4/24 FB
22	Sample	15	9675	GCMS0501	GC/MS SCAN 4/24
23	Sample	16	LBA	GCMS0501	GC/MS SCAN 4/25
24	Sample	17	REFA1	GCMS0501	GC/MS SCAN 4/25
25	Sample	18	REFA2	GCMS0501	GC/MS SCAN 4/25
26	Sample	19	9676	GCMS0501	GC/MS SCAN 4/25 FB
27	Sample	20	9677	GCMS0501	GC/MS SCAN 4/25
28	Sample	21	9678	GCMS0501	GC/MS SCAN 4/25
29	Sample	22	9679	GCMS0501	GC/MS SCAN 4/25
30	Sample	23	9680	GCMS0501	GC/MS SCAN 4/25 FB
31	Sample	24	9681	GCMS0501	GC/MS SCAN 4/25
32	Sample	25	9682	GCMS0501	GC/MS SCAN 4/25
33	Sample	26	8016	GCMS0501	GC/MS SCAN 4/25
34	Sample	1	DFTPP1	GCMS0507	GC/MS SCAN 4/29
35	Sample	2	CAL80A	GCMS0507	GC/MS SCAN 4/29
36	Sample	3	LBB	GCMS0507	GC/MS SCAN 4/29
37	Sample	4	REFB1	GCMS0507	GC/MS SCAN 4/29
38	Sample	5	REFB2	GCMS0507	GC/MS SCAN 4/29
39	Sample	6	10137	GCMS0507	GC/MS SCAN 4/29
40	Sample	7	10159	GCMS0507	GC/MS SCAN 4/29
41	Sample	8	10160	GCMS0507	GC/MS SCAN 4/29
42	Sample	9	10161	GCMS0507	GC/MS SCAN 4/29
43	Sample	10	10162	GCMS0507	GC/MS SCAN 4/29

. Sequence Name: C:\HPCHEM\1\SEQUENCE\MAY0602.S

Line	Type	Vial	DataFile	Method	Sample Name
44	Sample	11 10163	GCMS0507	GC/MS	SCAN 4/29
45	Sample	12 10164	GCMS0507	GC/MS	SCAN 4/29
46	Sample	13 10165	GCMS0507	GC/MS	SCAN 4/29
47	Sample	14 10166	GCMS0507	GC/MS	SCAN 4/29

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY0602\DFTPP1.D

Vial: 1

Acq On : 7 May 2002 5:46 pm

Operator:

Sample : GC/MS SCAN 4/29

Inst : 209


Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)

Title : 209 625/TCLP calibration table

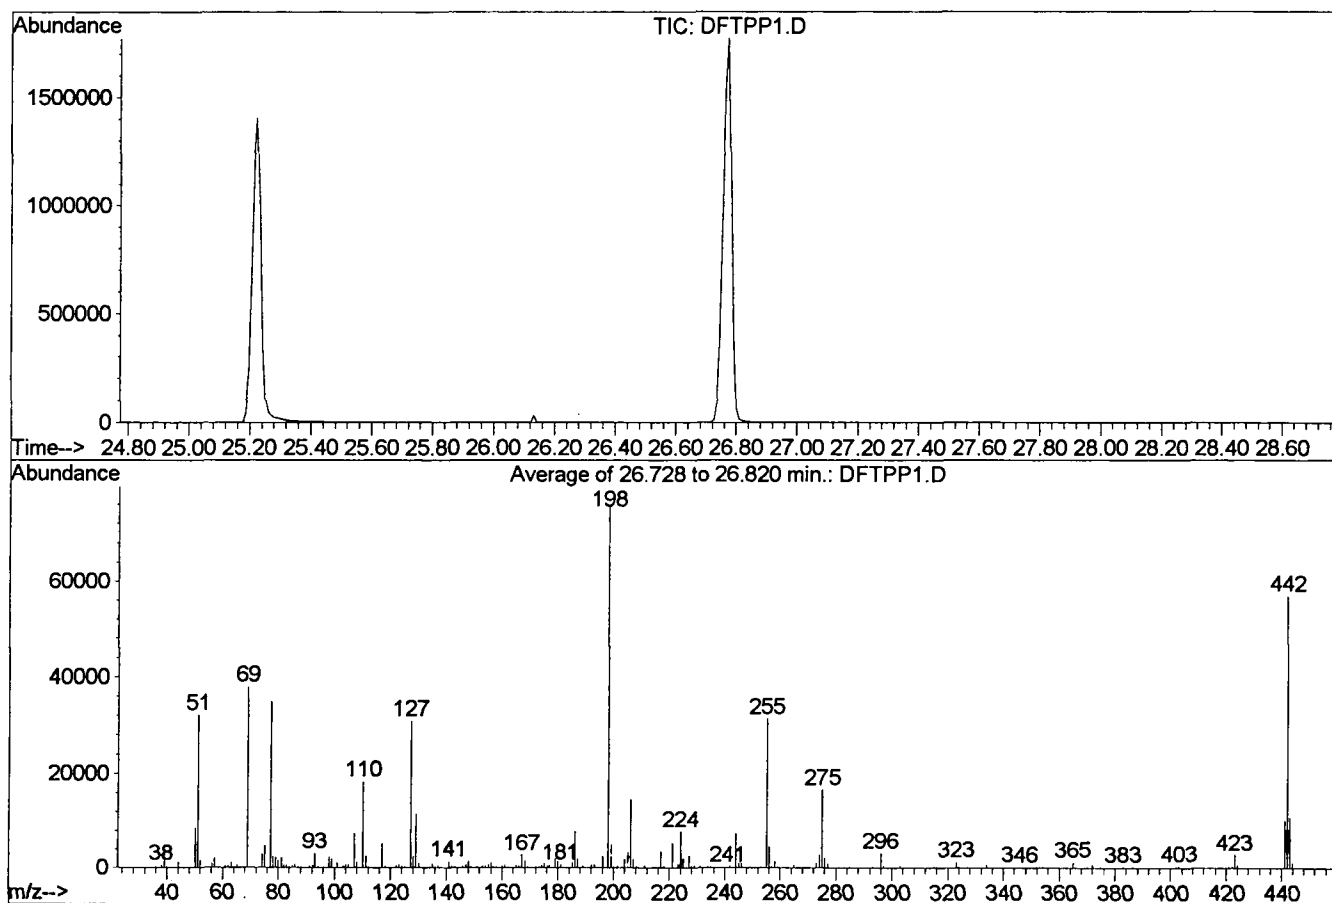

Spectrum Information: Average of 26.728 to 26.820 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.3	32145	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.9	37946	PASS
70	69	0.00	2	0.0	17	PASS
127	198	40	60	40.6	30868	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	75976	PASS
199	198	5	9	6.5	4976	PASS
275	198	10	30	21.9	16611	PASS
365	198	1	100	1.6	1252	PASS
441	443	0.01	100	93.5	10080	PASS
442	198	40	110	74.8	56802	PASS
443	442	17	23	19.0	10780	PASS

DFTPP1.D GCMS0507.M

Thu May 09 09:34:12 2002