

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/10/2002 Time: 14:19:28

Sample: AE10162
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/10/02 14:18 Ended: 5/10/02 14:18 Analyst: DLV
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		81		10.0

Comments for Sample AE10162 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-10-2002 Time: 14:19:31

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\HPCHEM\1\DATA\MAY0602\10162.D
 Acq On : 8 May 2002 2:39 am
 Sample : GC/MS SCAN 4/29
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 9 9:54 2002

Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0507.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue May 07 08:24:38 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0507

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	438120	40.00	ug/l	0.00
10) Naphthalene-d8	15.83	136	1590870	40.00	ug/l	0.00
17) Acenaphthene-d10	21.13	164	874334	40.00	ug/l	0.00
30) Phenanthrene-d10	25.57	188	1233233	40.00	ug/l	0.00
38) Chrysene-d12	33.63	240	749232	40.00	ug/l	0.00
44) Perylene-d12	37.86	264	433359	40.00	ug/l	0.00

System Monitoring Compounds

28) TCMX	23.27	209	35117	8.07	ug/L	0.00
Spiked Amount	10.000		Recovery	=	80.70%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.61	149	315	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.57	178	334	N.D.	

(#) = qualifier out of range (m) = manual integration

10162.D GCMS0507.M Thu May 09 09:54:52 2002

Page 1

Data File : C:\HPCHEM\1\DATA\MAY0602\10162.D

Vial: 10

Acq On : 8 May 2002 2:39 am

Operator:

Sample : GC/MS SCAN 4/29

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 9 9:54 2002

Quant Results File: GCMS0507.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue May 07 08:24:38 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0507

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.57	178	334	N.D.		
36) Di-n-butylphthalate	27.55	149	1356	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.63	228	1500	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.85	149	1553	N.D.		
43) Chrysene	33.63	228	1500	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.87	252	1627	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

10162.D GCMS0507.M Thu May 09 09:54:53 2002


Page 2

Data File : C:\HPCHEM\1\DATA\MAY0602\10162.D
 Acq On : 8 May 2002 2:39 am
 Sample : GC/MS SCAN 4/29
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 9 9:54 2002

Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0507.RES

Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue May 07 08:24:38 2002
 Response via : Initial Calibration

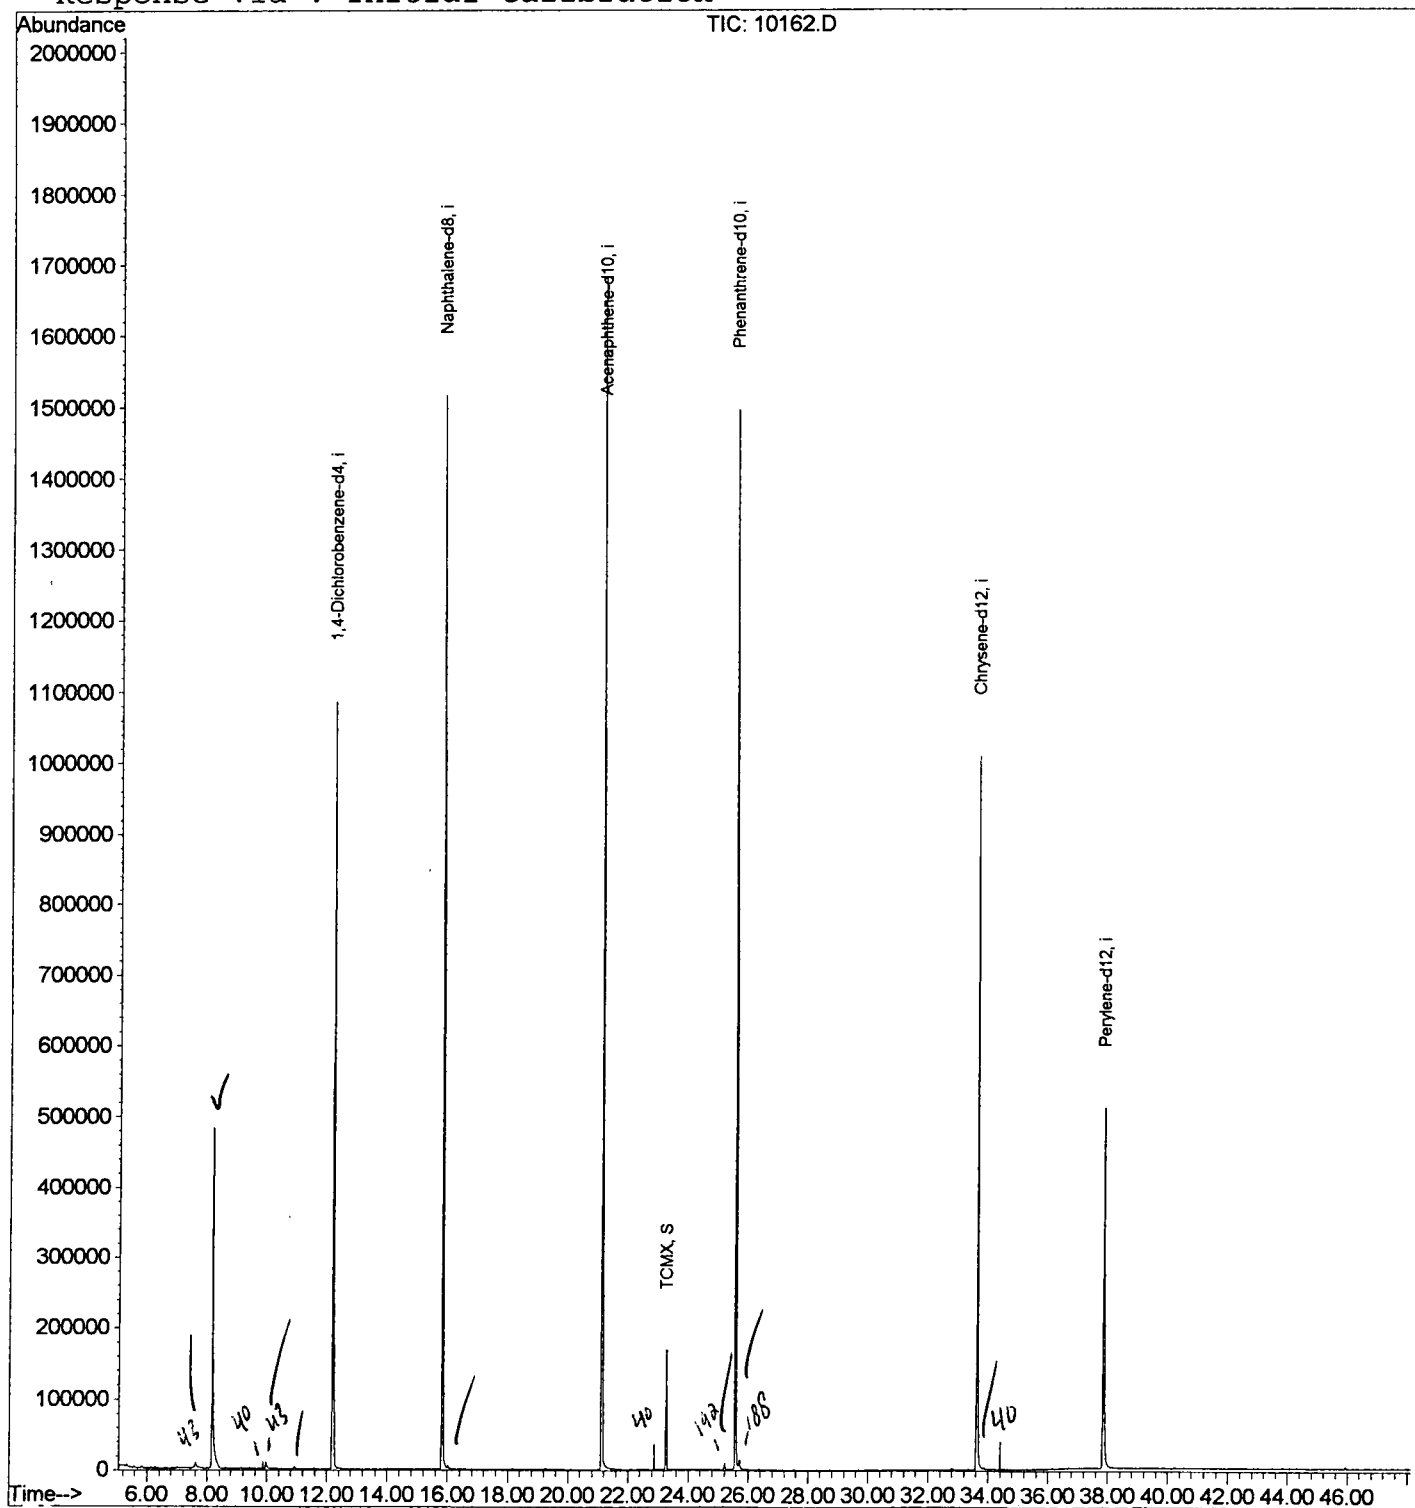

Data File : C:\HPCHEM\1\DATA\MAY0602\10162.D
 Acq On : 8 May 2002 2:39 am
 Sample : GC/MS SCAN 4/29
 Misc :
 MS Integration Params: LSCINT.P

Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.159	336	340	370	rVB	481749	1101006	31.44%	6.268%
2	12.191	775	780	796	rBV	1084942	2492585	71.18%	14.189%
3	15.829	1171	1177	1194	rBV	1516205	3130283	89.39%	17.819%
4	21.134	1749	1756	1776	rBV	1683216	3501979	100.00%	19.935%
5	23.269	1981	1989	1997	rBV	168868	331608	9.47%	1.888%
6	25.569	2234	2240	2250	rBV2	1495870	3269453	93.36%	18.612%
7	33.633	3113	3120	3140	rBV2	1008466	2234611	63.81%	12.721%
8	37.858	3573	3581	3598	rBV2	508404	1505276	42.98%	8.569%

Sum of corrected areas: 17566801

10162.D GCMS0507.M Thu May 09 11:12:56 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0602\10162.D
 Operator :
 Acquired : 8 May 2002 2:39 am using AcqMethod GCMS0507
 Instrument : 209
 Sample Name: GC/MS SCAN 4/29
 Misc Info :
 Vial Number: 10
 Quant File :GCMS0507.RES (RTE Integrator)

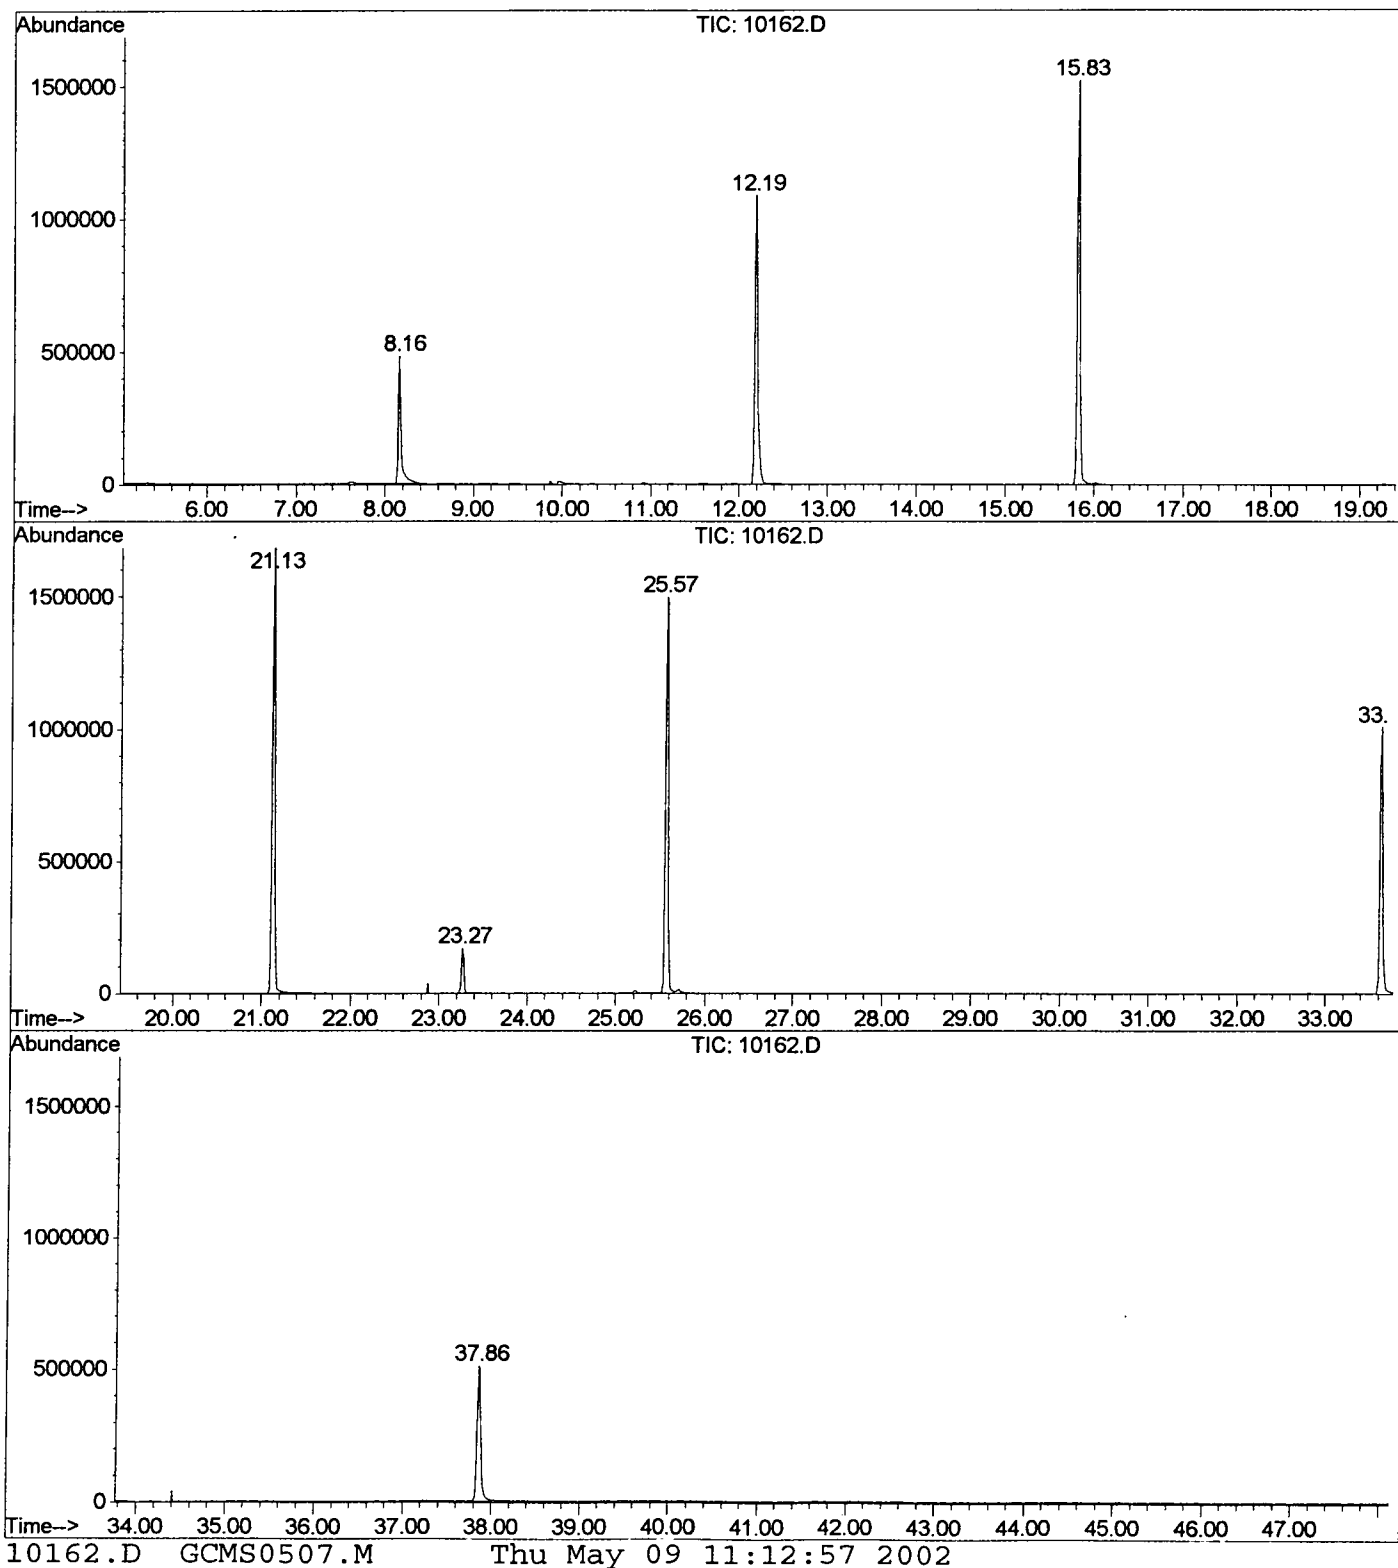

Data File : C:\HPCHEM\1\DATA\MAY0602\10162.D
 Acq On : 8 May 2002 2:39 am
 Sample : GC/MS SCAN 4/29
 Misc :
 MS Integration Params: LSCINT.P


Vial: 10
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	17.67 ug/l	1101010	1,4-Dichlorobenzene-d4	12.19

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2		3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
3		Acetone	58	C3H6O	000067-64-1	7
4		5-Hexen-2-one	98	C6H10O	000109-49-9	7

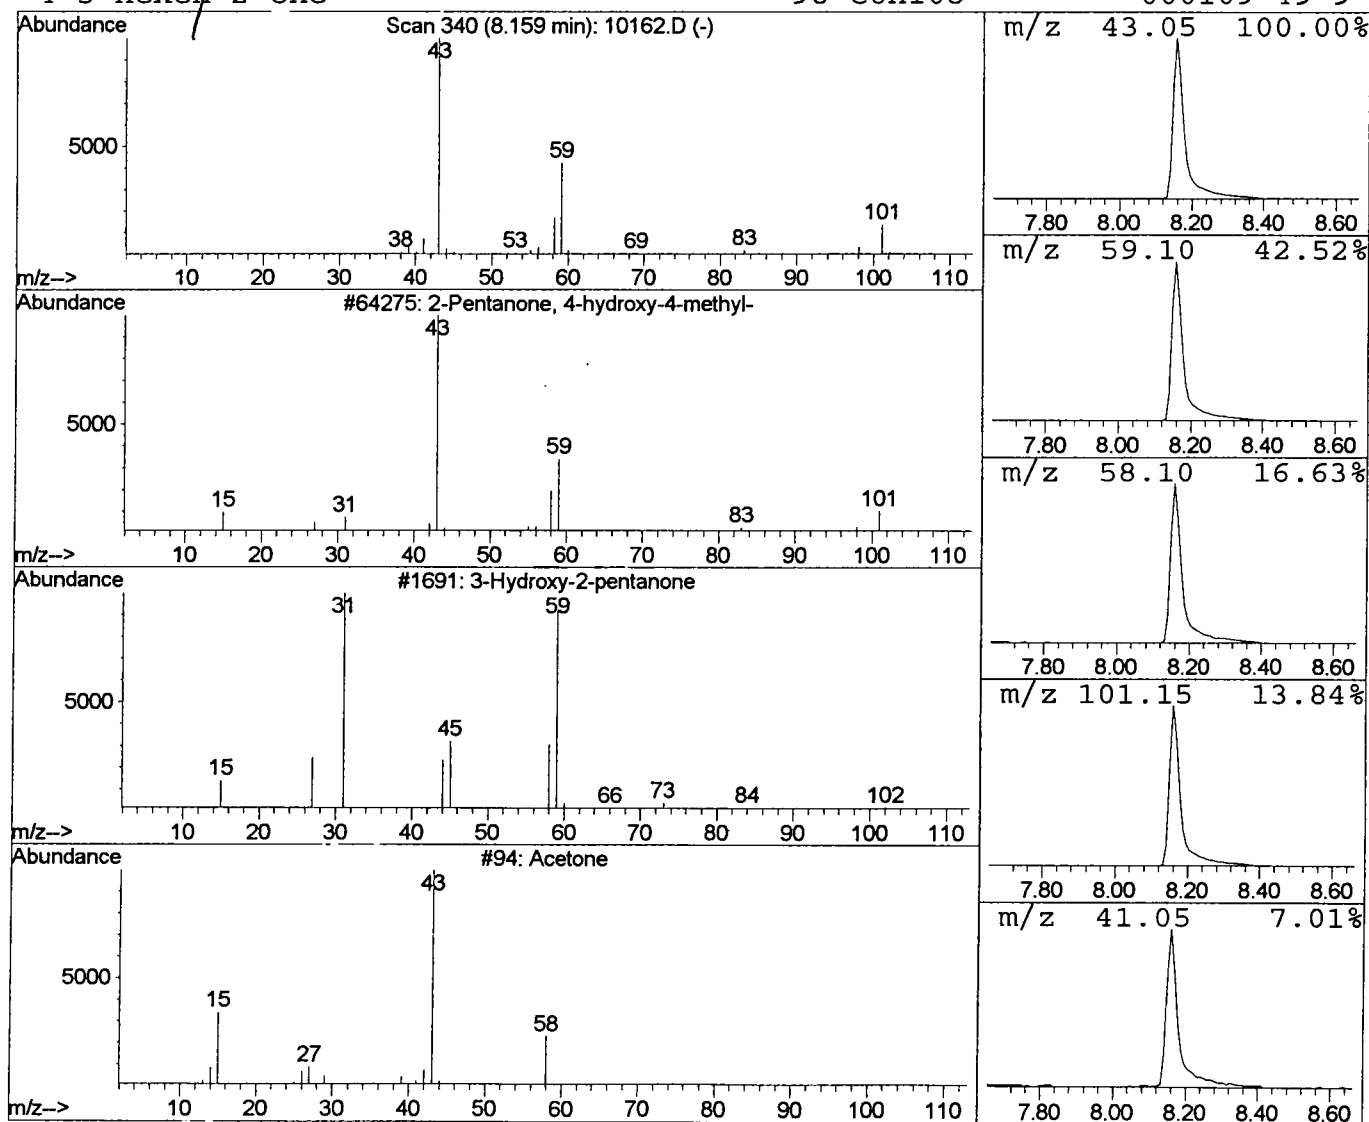

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 8 May 2002 2:39 am
 Data File: C:\HPCHEM\1\DATA\MAY0602\10162.D
 Name: GC/MS SCAN 4/29
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	17.7	ug/l	1101010	ISTD01	12.19	2492590	40.0
10162.D GCMS0507.M	Thu May 09 11:12:58 2002							