

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/21/2002 Time: 12:26:32

Sample: AE10516
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/21/02 12:26 Ended: 5/21/02 12:26 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		75		10.0

Comments for Sample AE10516 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-21-2002 Time: 12:27:36

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\HPCHEM\1\DATA\MAY1002\10516.D

Vial: 39

Acq On : 12 May 2002 3:08 am

Operator:

Sample : gc/ms scan 5/2

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOIFY.P

Quant Time: May 16 14:54 2002

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Thu May 16 09:35:44 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0507

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.16	152	615298	40.00	ug/l	-0.03
10) Naphthalene-d8	15.79	136	2248995	40.00	ug/l	-0.04
17) Acenaphthene-d10	21.10	164	1213387	40.00	ug/l	-0.04
30) Phenanthrene-d10	25.55	188	1678382	40.00	ug/l	-0.02
38) Chrysene-d12	33.62	240	1002470	40.00	ug/l	-0.02
44) Perylene-d12	37.84	264	606848	40.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.24	209	45472	7.53	ug/L	-0.03
Spiked Amount	10.000		Recovery	=	75.30%	

Target Compounds

					Qvalue
2) N-nitrosodimethylamine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.85	128	440	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	21.36	165	357	N.D.	
25) Diethylphthalate	22.59	149	682	N.D.	
26) 4-Chlorophenylphenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene	23.24	77	803	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenylphenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.61	178	352	N.D.	

(#)=qualifier out of range (m)=manual integration

10516.D GCMS0510.M Thu May 16 14:55:32 2002

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY1002\10516.D Vial: 39
Acq On : 12 May 2002 3:08 am Operator:
Sample : gc/ms scan 5/2 Inst : 209
Misc : Multiplr: 1.00
MS Integration Params: GOOFY.P
Quant Time: May 16 14:54 2002 Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu May 16 09:35:44 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0507

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.61	178	352		N.D.	
36) Di-n-butylphthalate	27.52	149	1806		N.D.	
37) Fluoranthene	0.00	202	0		N.D.	
39) Pyrene	0.00	202	0		N.D.	
40) Butylbenzylphthalate	0.00	149	0		N.D.	
41) Benzo(a)anthracene	33.62	228	2330		N.D.	
42) Bis(2-ethylhexyl)phthalate	33.84	149	2839		N.D.	
43) Chrysene	33.69	228	543		N.D.	
45) Di-n-Octylphthalate	0.00	149	0		N.D.	
46) Benzo(b)fluoranthene	36.67	252	440		N.D.	
47) Benzo(k)fluoranthene	36.74	252	396		N.D.	
48) Benzo(a)pyrene	37.85	252	2446		N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

(#) = qualifier out of range (m) = manual integration

10516.D GCMS0510.M Thu May 16 14:55:33 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY1002\10516.D
 Acq On : 12 May 2002 3:08 am
 Sample : gc/ms scan 5/2
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 16 14:54 2002

Vial: 39
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0510.RES

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Thu May 16 09:35:44 2002
 Response via : Initial Calibration

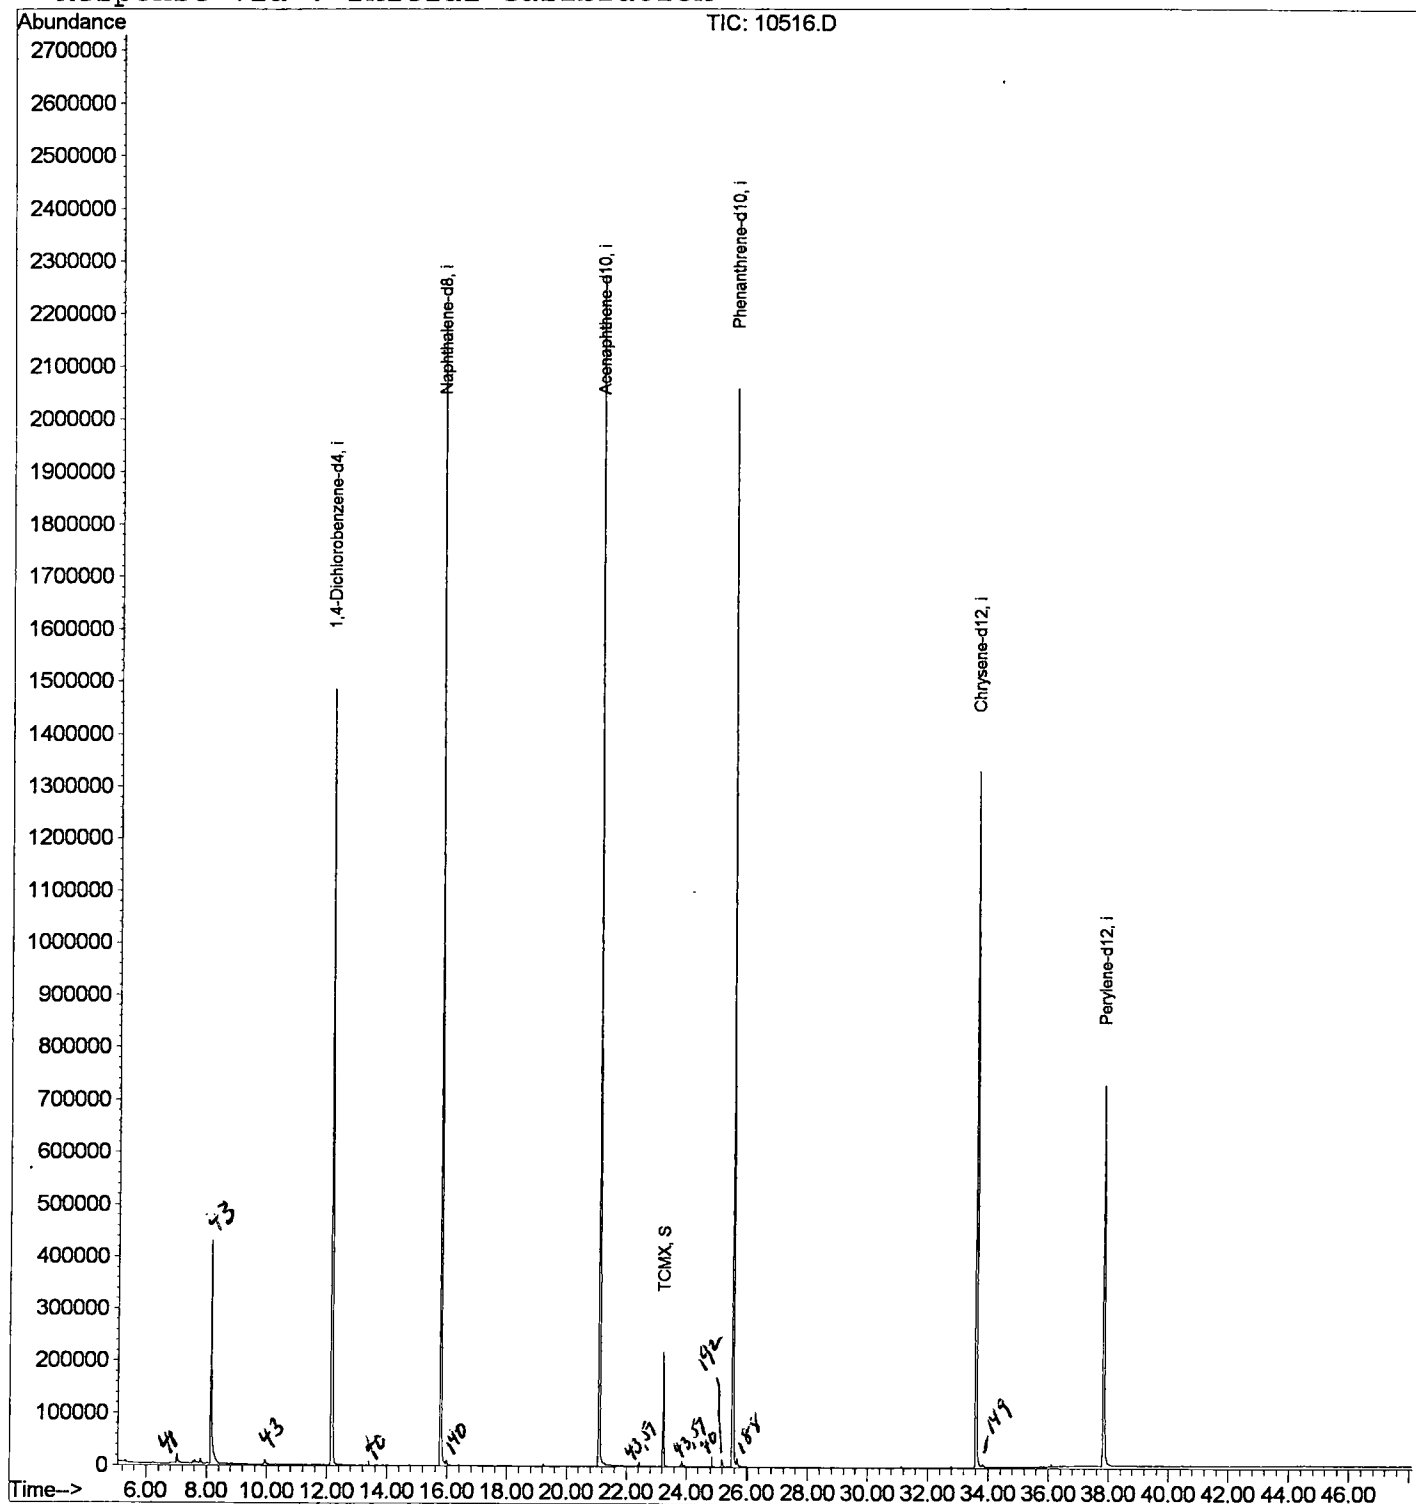

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY1002\10516.D

Vial: 39

Acq On : 12 May 2002 3:08 am

Operator:

Sample : gc/ms scan 5/2

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.141	334	338	366	rBV	426887	1026284	21.01%	4.294%
2	12.164	771	777	794	rBV	1483550	3496951	71.59%	14.632%
3	15.793	1167	1173	1190	rBV	2174513	4410475	90.29%	18.455%
4	21.099	1746	1752	1770	rBV	2272664	4884617	100.00%	20.439%
5	23.243	1978	1986	1993	rVB	219134	437473	8.96%	1.831%
6	25.552	2231	2238	2249	rBV2	2058034	4478704	91.69%	18.740%
7	33.616	3111	3118	3133	rBV2	1327995	3000914	61.44%	12.557%
8	37.840	3571	3579	3602	rBV2	725644	2163583	44.29%	9.053%




Sum of corrected areas: 23899001

10516.D GCMS0510.M

Thu May 16 15:01:49 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY1002\10516.D
 Operator :
 Acquired : 12 May 2002 3:08 am using AcqMethod GCMS0507
 Instrument : 209
 Sample Name: gc/ms scan 5/2
 Misc Info :
 Vial Number: 39
 Quant File : GCMS0510.RES (RTE Integrator)

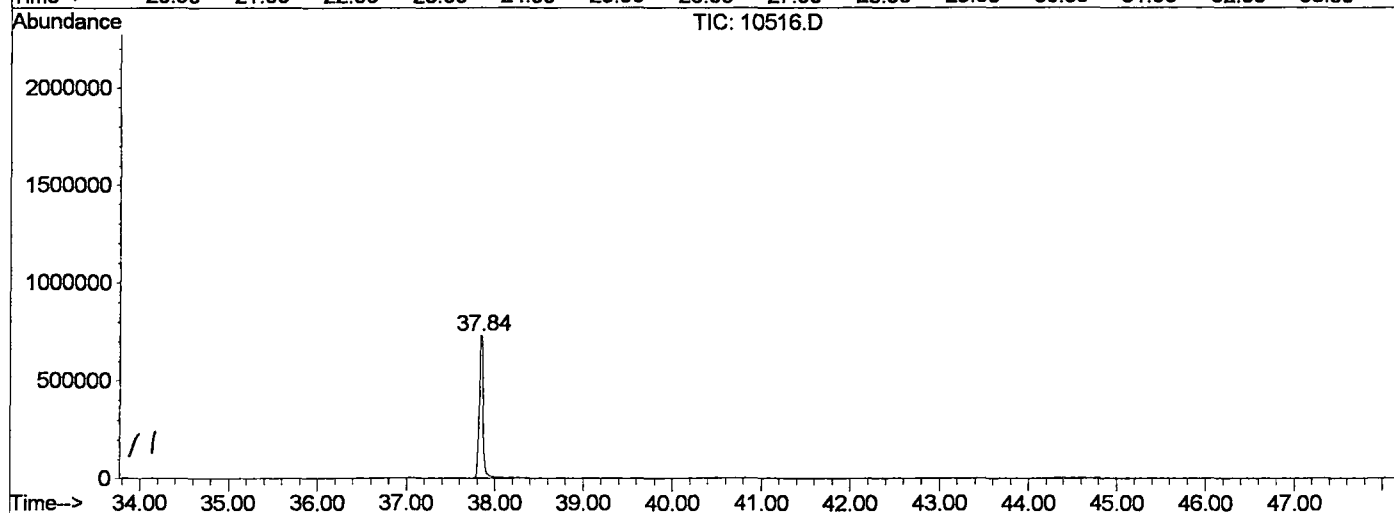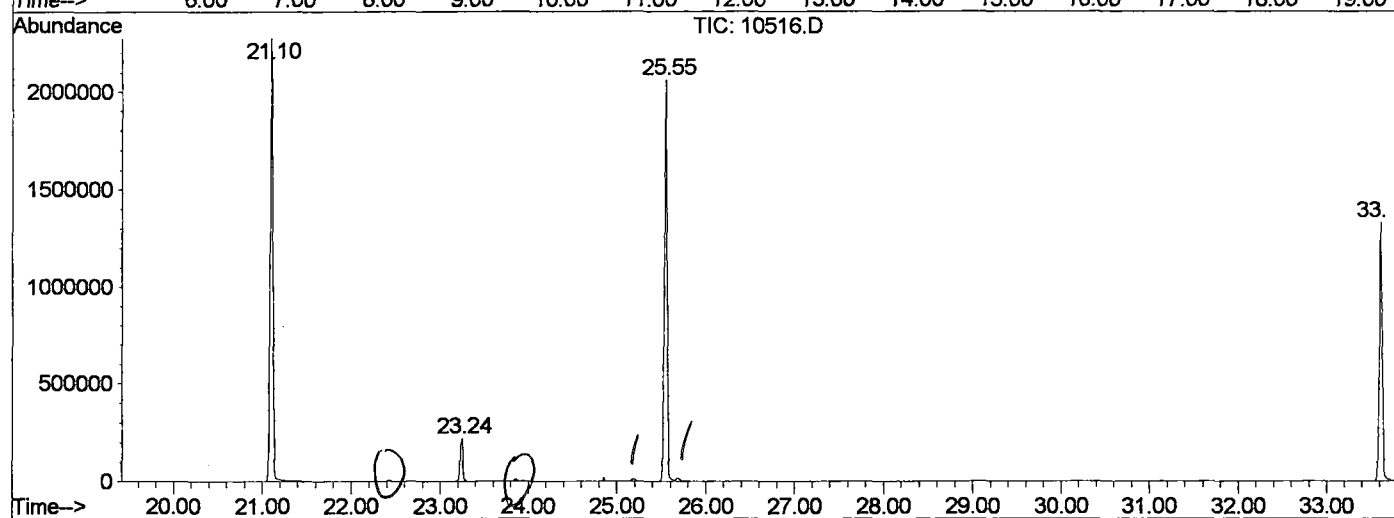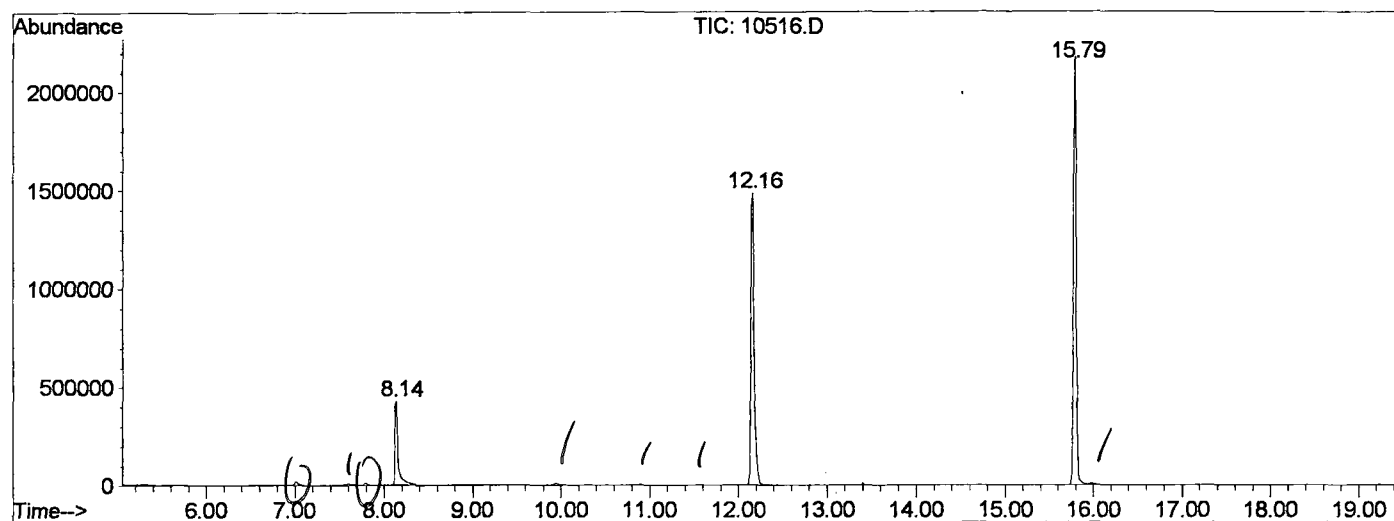

10516.D GCMS0510.M Thu May 16 15:01:50 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY1002\10516.D
 Acq On : 12 May 2002 3:08 am
 Sample : gc/ms scan 5/2
 Misc :
 MS Integration Params: LSCINT.P









Vial: 39
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.14	11.74 ug/l	1026280	1,4-Dichlorobenzene-d4	12.16

Hit# of	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	9
3	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
4	Acetone	58	C3H6O	000067-64-1	7

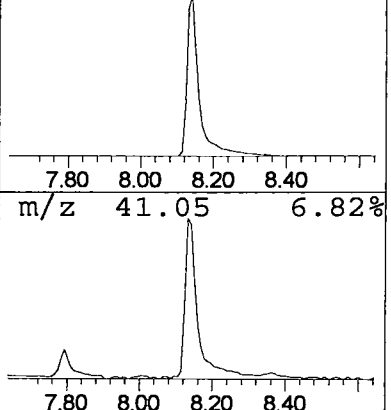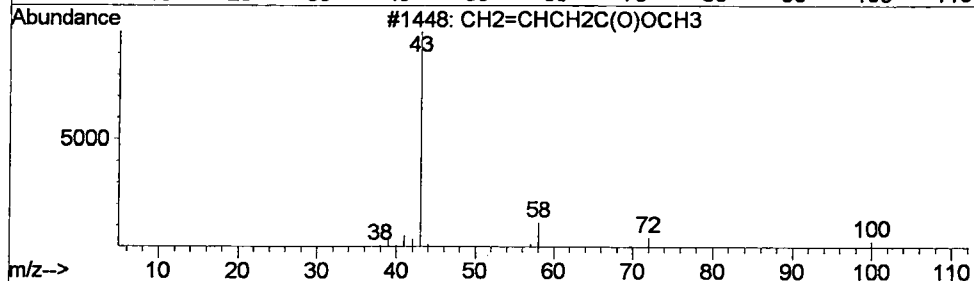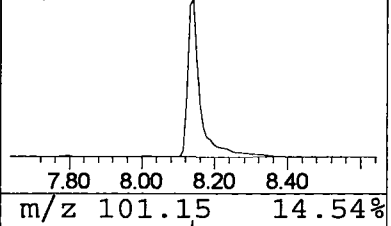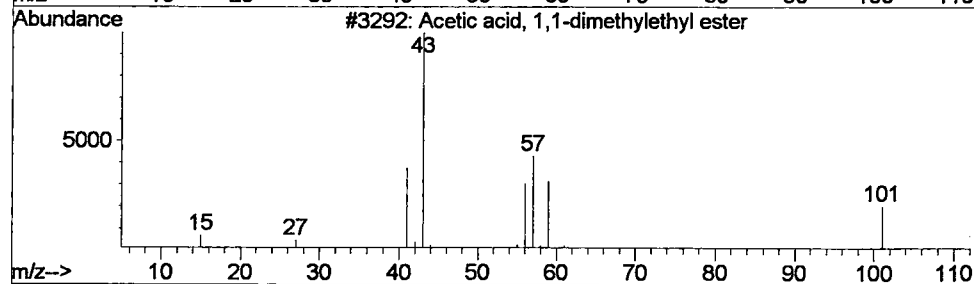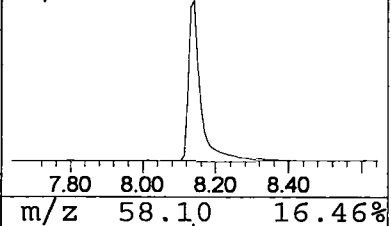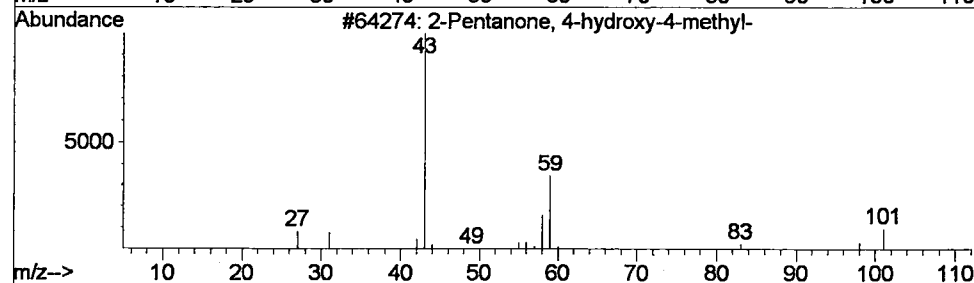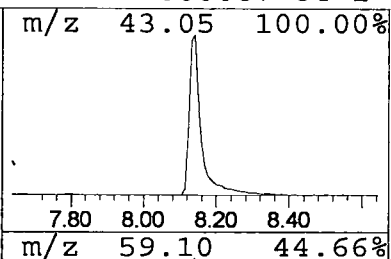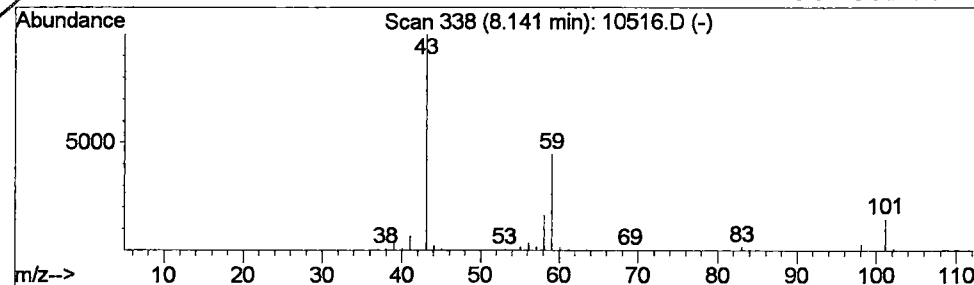

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 12 May 2002 3:08 am
Data File: C:\HPCHEM\1\DATA\MAY1002\10516.D
Name: gc/ms scan 5/2
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top	Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro		8.14	11.7	ug/l	1026280	ISTD01	12.16	3496950	40.0
10516.D	GCMS0510.M			Thu May 16 15:01:51 2002					