

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 05/15/2002 Time: 15:24:25

Sample: AE10608
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 5/15/02 15:24 Ended: 5/15/02 15:24 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifiers	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		83		10.0

Comments for Sample AE10608 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-15-2002 Time: 15:24:50

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0802\10608.D
 Acq On : 8 May 2002 4:26 pm
 Sample : GC/MS SCAN 5/3
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 9 14:35 2002

Vial: 7
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0507.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Thu May 09 14:27:53 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0507

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	461738	40.00	ug/l	0.00
10) Naphthalene-d8	15.83	136	1664054	40.00	ug/l	0.00
17) Acenaphthene-d10	21.13	164	901338m	40.00	ug/l	0.00
30) Phenanthrene-d10	25.58	188	1206987	40.00	ug/l	0.00
38) Chrysene-d12	33.63	240	596118	40.00	ug/l	0.00
44) Perylene-d12	37.86	264	352363	40.00	ug/l	0.00

System Monitoring Compounds

28) TCMX	23.27	209	37308m	8.32	ug/L	0.00
Spiked Amount	10.000		Recovery	=	83.20%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.88	128	755	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.62	149	880	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.63	178	925	N.D.	

(#) = qualifier out of range (m) = manual integration

10608.D GCMS0507.M Thu May 09 14:35:18 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0802\10608.D

Vial: 7

Acq On : 8 May 2002 4:26 pm

Operator:

Sample : GC/MS SCAN 5/3

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: May 9 14:35 2002

Quant Results File: GCMS0507.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Thu May 09 14:27:53 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0507

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.63	178	726	N.D.		
36) Di-n-butylphthalate	27.55	149	3149	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.63	228	1504	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.86	149	3057	N.D.		
43) Chrysene	33.63	228	1504	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	36.70	252	264	N.D.		
47) Benzo(k)fluoranthene	36.76	252	753	N.D.		
48) Benzo(a)pyrene	37.68	252	104	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

10608.D GCMS0507.M Thu May 09 14:35:19 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY0802\10608.D
Acq On : 8 May 2002 4:26 pm
Sample : GC/MS SCAN 5/3
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 9 14:35 2002

Vial: 7
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0507.RES

Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu May 09 14:27:53 2002
Response via : Initial Calibration

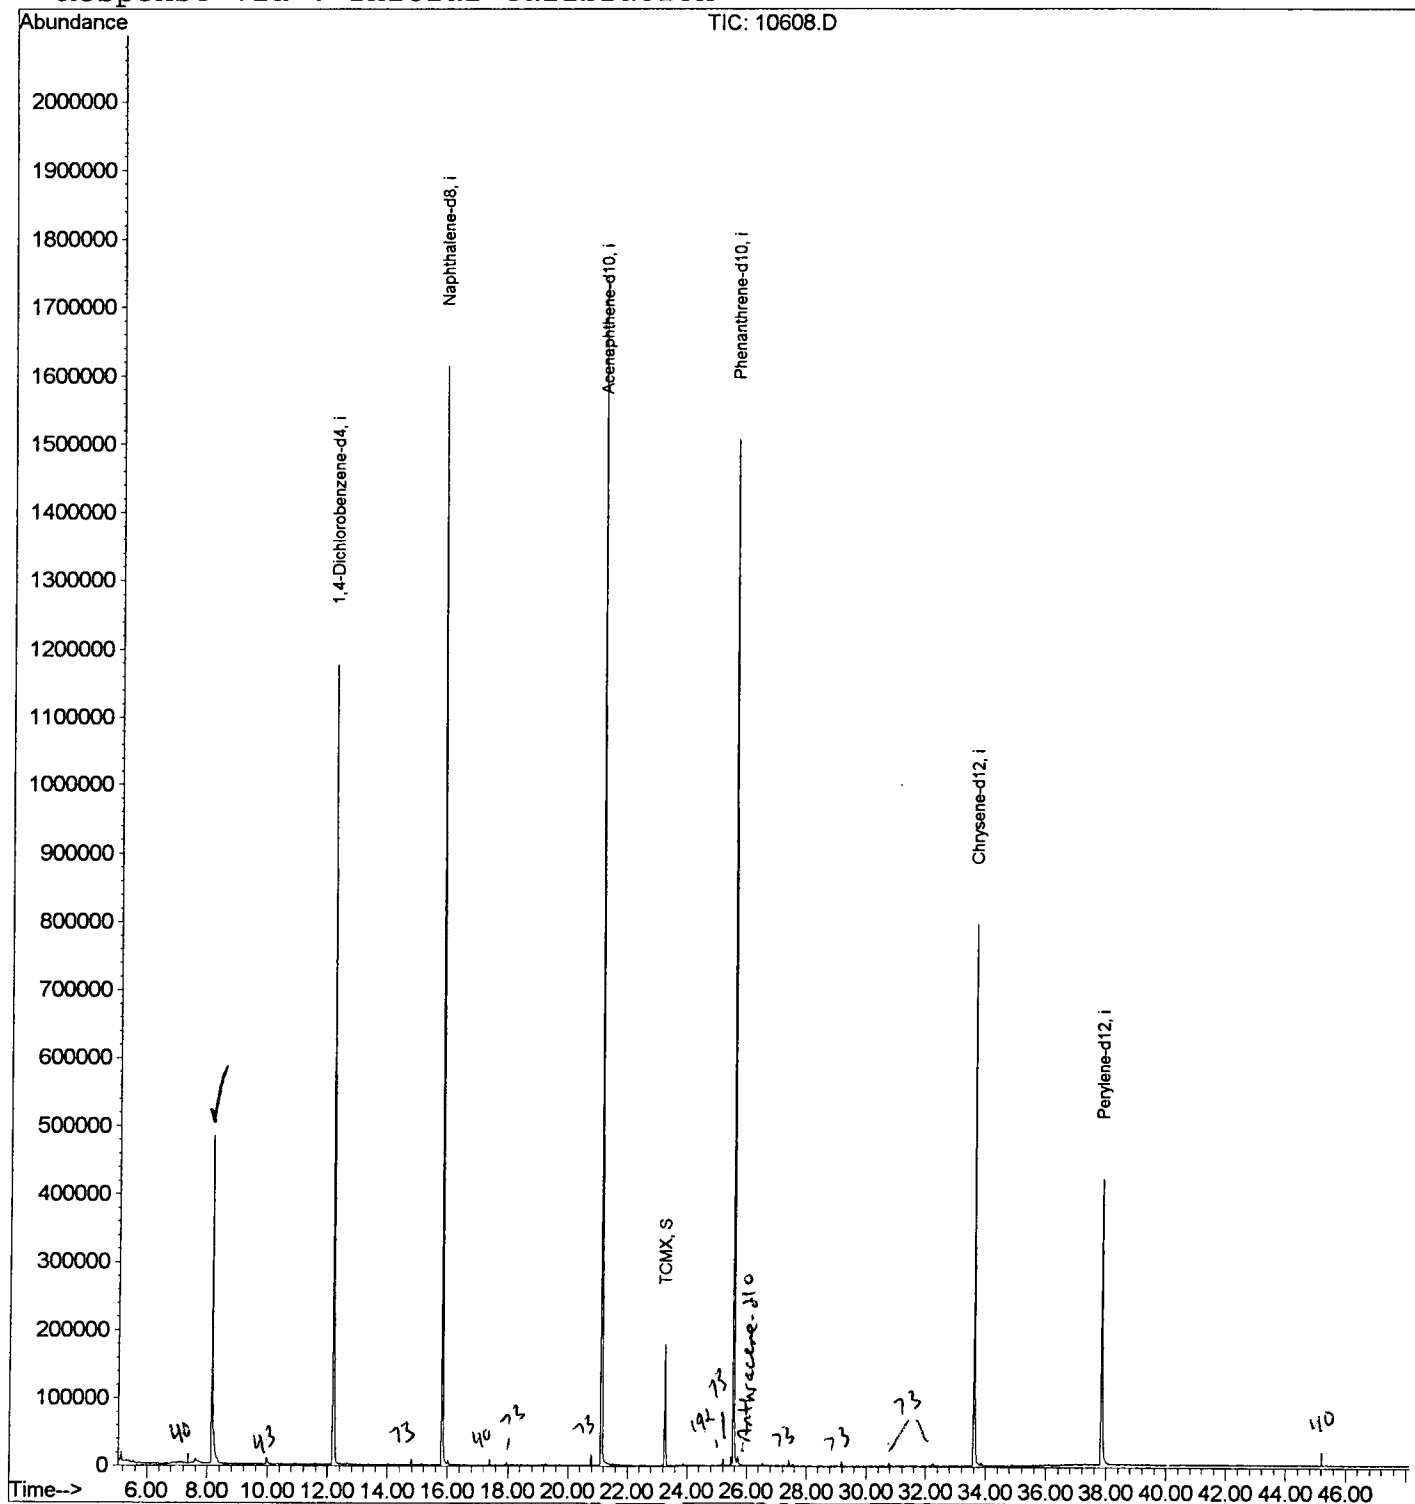

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY0802\10608.D
 Acq On : 8 May 2002 4:26 pm
 Sample : GC/MS SCAN 5/3
 Misc :
 MS Integration Params: LSCINT.P

Vial: 7
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.157	336	340	346	rBV	482291	950349	26.13%	5.560%
2	12.189	775	780	796	rBV	1175313	2620988	72.05%	15.334%
3	15.827	1170	1177	1194	rBV	1612994	3278196	90.12%	19.179%
4	21.133	1749	1756	1771	rBV	1746352	3637679	100.00%	21.282%
5	23.268	1981	1989	1998	rBV2	178619	391848	10.77%	2.292%
6	25.577	2234	2241	2251	rVV2	1505294	3206453	88.15%	18.759%
7	33.632	3113	3120	3134	rBV	796336	1783711	49.03%	10.435%
8	37.856	3573	3581	3601	rBV2	419693	1223646	33.64%	7.159%

Sum of corrected areas: 17092870

10608.D GCMS0507.M Thu May 09 14:42:25 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0802\10608.D
 Operator :
 Acquired : 8 May 2002 4:26 pm using AcqMethod GCMS0507
 Instrument : 209
 Sample Name: GC/MS SCAN 5/3
 Misc Info :
 Vial Number: 7
 Quant File :GCMS0507.RES (RTE Integrator)

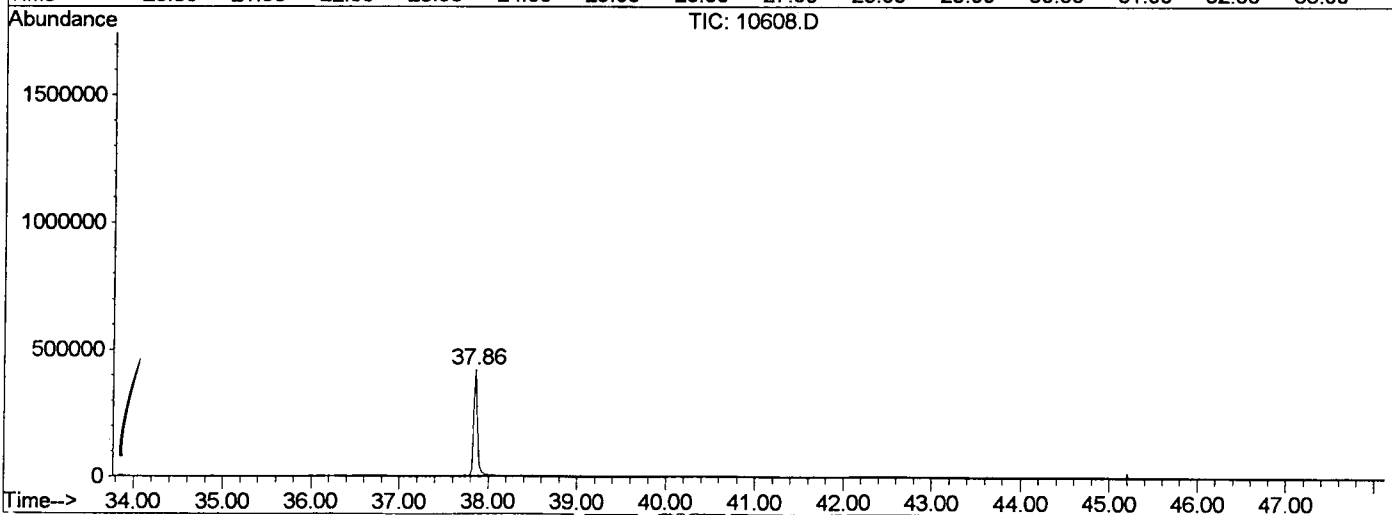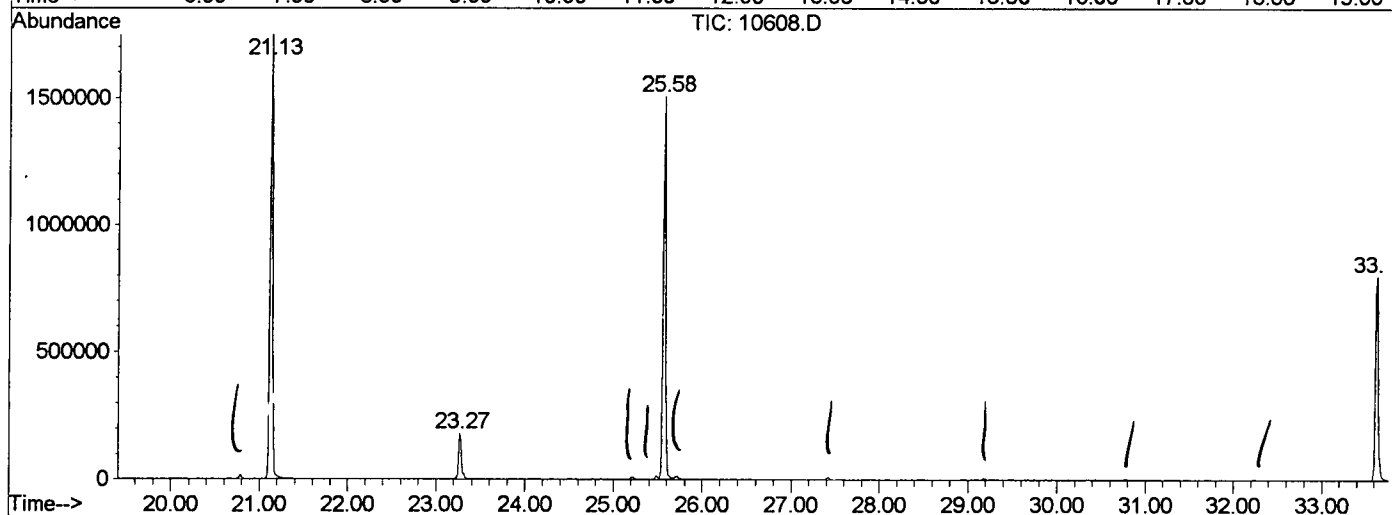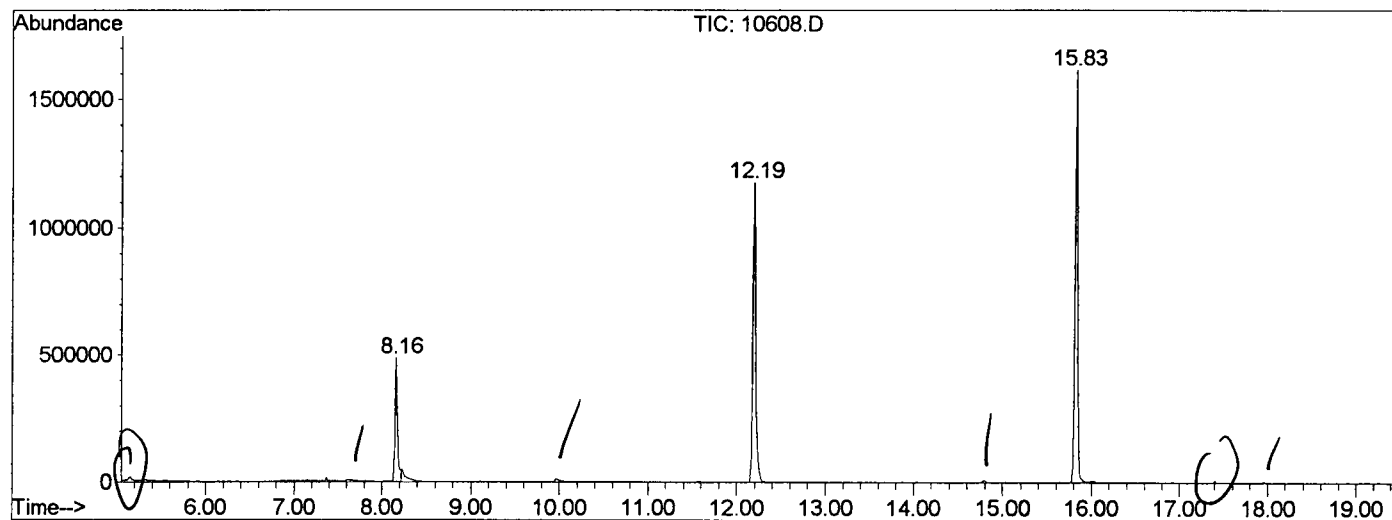

10608.D GCMS0507.M Thu May 09 14:42:26 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0802\10608.D
 Acq On : 8 May 2002 4:26 pm
 Sample : GC/MS SCAN 5/3
 Misc :
 MS Integration Params: LSCINT.P


Vial: 7
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	14.50 ug/l	950349	1,4-Dichlorobenzene-d4	12.19

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
3			CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	9
4			Acetone	58	C3H6O	000067-64-1	7

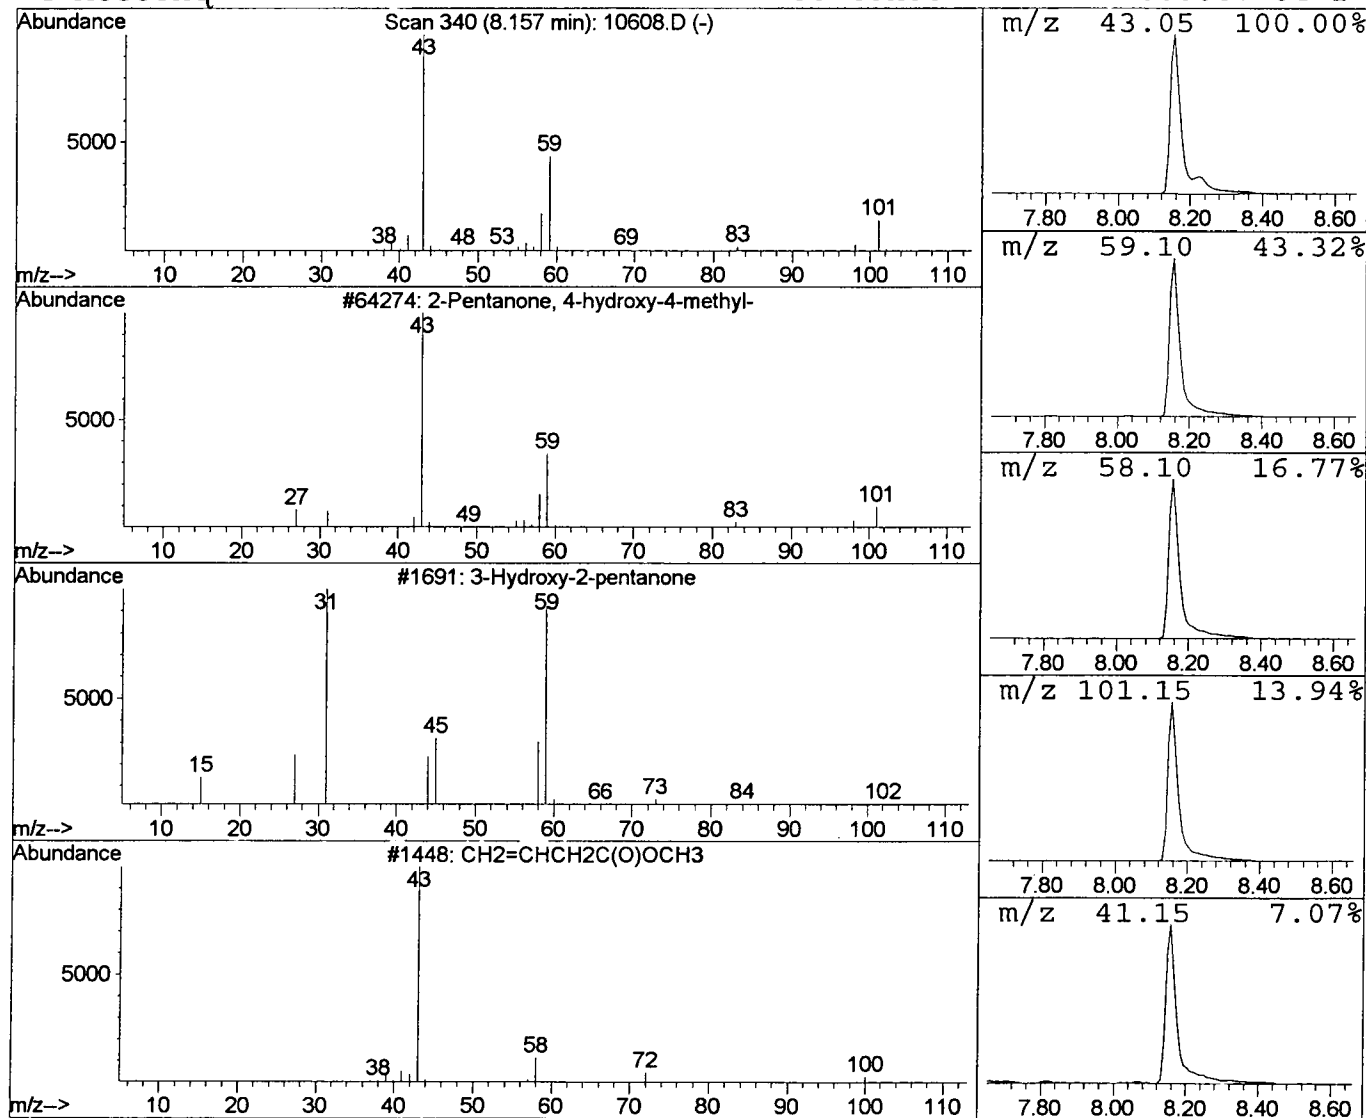

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 8 May 2002 4:26 pm
 Data File: C:\HPCHEM\1\DATA\MAY0802\10608.D
 Name: GC/MS SCAN 5/3
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	14.5	ug/l	950349	ISTD01	12.19	2620990	40.0
10608.D GCMS0507.M	Thu May 09 14:42:27 2002							