

#GEMS-18491 / 05/15/2002

Reviewed by DN
Date 5/20/2

 Comment: GCMS scan
 Operator: Nefliu
 Data Path: C:\MSDchem\1\DATA\020513\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line Type Vial DataFile Method Sample Name

1 Sample	1	DFTPP	508FAST	
2 Sample	2	0513C4	508SCAN1	ccv
3 Sample	3	0506LB	508SCAN1	05/06 lab blk
4 Sample	4	0507LB	508SCAN1	05/07 lab blk
5 Sample	5	0506REF1	508SCAN1	05/06 ref
6 Sample	6	0506REF2	508SCAN1	05/06 ref
7 Sample	7	0507REF1	508SCAN1	05/07 ref
8 Sample	8	0507REF2	508SCAN1	05/07 ref
9 Sample	9	10698	508SCAN1	sample
10 Sample	10	10699	508SCAN1	sample
11 Sample	11	10700	508SCAN1	sample
12 Sample	12	10701	508SCAN1	sample
13 Sample	13	10702	508SCAN1	sample
14 Sample	14	10703	508SCAN1	sample
15 Sample	15	10704	508SCAN1	sample
16 Sample	16	10705	508SCAN1	sample
17 Sample	17	10130	508SCAN1	sample
18 Sample	18	10131	508SCAN1	sample
19 Sample	19	10132	508SCAN1	sample
20 Sample	20	10133	508SCAN1	sample
21 Sample	21	10135	508SCAN1	sample
22 Sample	22	10136	508SCAN1	sample
23 Sample	23	10066	508SCAN1	sample
24 Sample	24	10067	508SCAN1	sample
25 Sample	25	10068	508SCAN1	sample

Method 500 GC MS/Scan
Instrument 214

File Directory 020513

Storage Directory _____

Lab #	Filename	Description	Vial #		Inj. ul	Standards used - Lot #			Int. Std.	Remarks	Initials
			front	rear		Calibration	Reference	Surrogate			
	057304	alt top	1								MN
	057304	alt	2			22873/22847/22860					
	050613	alt bla	3					2285			
	050713		4					2284			
	050601	ref	5					2285			
	↓ J2		6					↓			
	050701		7					2284			
	↓ J2		8					↓			
	10698	sample	9					2285			
	10699		10								
	10700		11								
	10701		12								
	10702		13								
	10703		14								
	10704		15								
	10705		16					↓			
	10130		17					2284			
	10131		18								
	10132		19								
	10133		20								
	10135		21								
	10136		22								
	10066		23								
	10067		24								
	10068		25								

Date 05/13/02


Extraction date 05/06/02/02

Page 8

DFTPP

Data File : C:\MSDCHEM\1\DATA\020513\DFTPP.D
Acq On : 13 May 2002 12:46 pm
Sample :
Misc :
MS Integration Params: rteint.e
Method : C:\MSDCHEM\1\METHODS\SCAN020507.M (RTE Integrator)
Title : Method 508 GC/MS Scan

Vial: 1
Operator: Nefliu
Inst : Instrume
Multiplr: 1.00

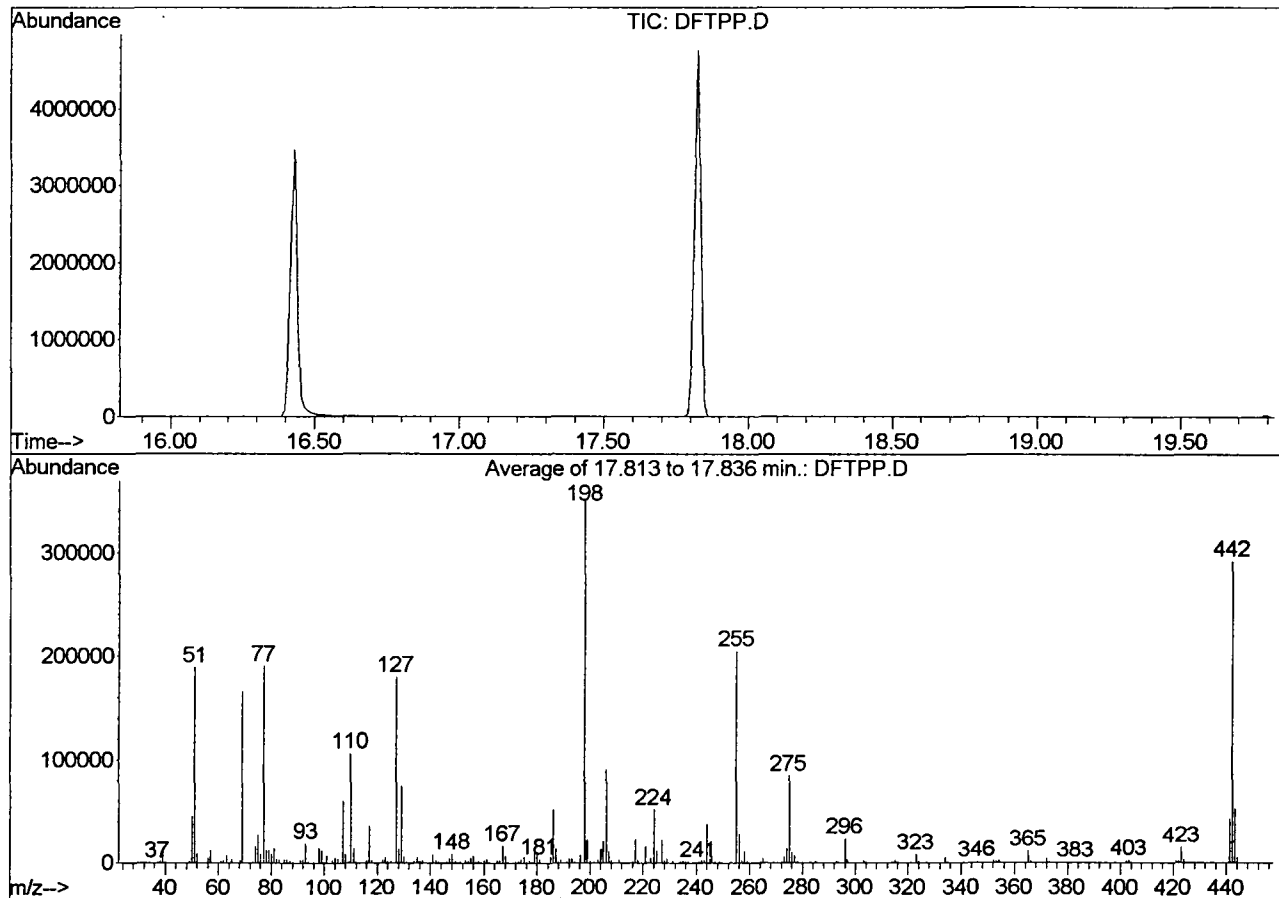

Spectrum Information: Average of 17.813 to 17.836 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	53.7	188848	PASS
68	69	0.00	2	1.7	2830	PASS
69	198	0.00	100	47.1	165781	PASS
70	69	0.00	2	0.4	746	PASS
127	198	40	60	51.0	179557	PASS
197	198	0.00	1	0.3	950	PASS
198	198	100	100	100.0	351893	PASS
199	198	5	9	6.6	23109	PASS
275	198	10	30	24.1	84813	PASS
365	198	1	99	3.3	11715	PASS
441	443	1	100	81.7	43842	PASS
442	198	40	110	83.1	292330	PASS
443	442	17	23	18.4	53664	PASS

DFTPP.D SCAN020507.M

Wed May 15 09:12:08 2002