

User: Galos, Marie  
 Westchester Dept. of Labs & Research  
 Date: 05/15/2002 Time: 09:13:19

Sample: AE10772  
 Analysis: \$B1GCMS Blank for GCMS Scan  
 Units: ug  
 Started: 5/6/02 00:01 Ended: 5/10/02 00:01 Analyst: MG  
 Result source: manual entry  
 Page: 1

|    | Component Name               | Viol | Result | MDL |
|----|------------------------------|------|--------|-----|
| 1  | n-Nitrosodimethylamine       |      | < MRL  | 2.0 |
| 2  | bis(2-Chloroethyl)ether      |      | < MRL  | 2.0 |
| 3  | 1,3-Dichlorobenzene          |      | < MRL  | 2.0 |
| 4  | 1,4-Dichlorobenzene          |      | < MRL  | 2.0 |
| 5  | 1,2-Dichlorobenzene          |      | < MRL  | 2.0 |
| 6  | 2,2'-oxybis(1-Chloropropane) |      | < MRL  | 2.0 |
| 7  | n-Nitrosodi-n-propylamine    |      | < MRL  | 2.0 |
| 8  | Hexachloroethane             |      | < MRL  | 2.0 |
| 9  | Nitrobenzene                 |      | < MRL  | 2.0 |
| 10 | Isophorone                   |      | < MRL  | 2.0 |
| 11 | bis(2-Chloroethoxy)methane   |      | < MRL  | 2.0 |
| 12 | 1,2,4-Trichlorobenzene       |      | < MRL  | 2.0 |
| 13 | Naphthalene                  |      | < MRL  | 2.0 |
| 14 | Hexachlorobutadiene          |      | < MRL  | 2.0 |
| 15 | 2-Chloronaphthalene          |      | < MRL  | 2.0 |
| 16 | Dimethylphthalate            |      | < MRL  | 2.0 |
| 17 | 2,6-Dinitrotoluene           |      | < MRL  | 2.0 |
| 18 | Acenaphthylene               |      | < MRL  | 2.0 |
| 19 | Acenaphthene                 |      | < MRL  | 2.0 |
| 20 | 2,4-Dinitrotoluene           |      | < MRL  | 2.0 |
| 21 | Diethylphthalate             |      | < MRL  | 2.0 |
| 22 | 4-Chlorophenylphenylether    |      | < MRL  | 2.0 |
| 23 | Fluorene                     |      | < MRL  | 2.0 |
| 24 | Azobenzene                   |      | < MRL  | 2.0 |
| 25 | n-Nitrosodiphenylamine       |      | < MRL  | 2.0 |
| 26 | 4-Bromophenylphenylether     |      | < MRL  | 2.0 |
| 27 | Hexachlorobenzene            |      | < MRL  | 2.0 |
| 28 | Phenanthrene                 |      | < MRL  | 2.0 |
| 29 | Anthracene                   |      | < MRL  | 2.0 |
| 30 | Di-n-butylphthalate          |      | < MRL  | 2.0 |
| 31 | Fluoranthene                 |      | < MRL  | 2.0 |
| 32 | Pyrene                       |      | < MRL  | 2.0 |
| 33 | Butylbenzylphthalate         |      | < MRL  | 2.0 |
| 34 | Benzo(a)anthracene           |      | < MRL  | 2.0 |
| 35 | bis(2-Ethylhexyl)phthalate   |      | < MRL  | 2.0 |
| 36 | Chrysene                     |      | < MRL  | 2.0 |
| 37 | Di-n-octylphthalate          |      | < MRL  | 2.0 |
| 38 | Benzo(b)fluoranthene         |      | < MRL  | 2.0 |
| 39 | Benzo(k)fluoranthene         |      | < MRL  | 2.0 |
| 40 | Benzo(a)pyrene               |      | < MRL  | 2.0 |
| 41 | Indeno(1,2,3-cd)pyrene       |      | < MRL  | 2.0 |
| 42 | Dibenz(a,h)anthracene        |      | < MRL  | 2.0 |
| 43 | Benzo(g,h,i)perylene         |      | < MRL  | 2.0 |

## Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY1002\LBA.D  
 Acq On : 11 May 2002 12:46 am  
 Sample : GC/MS SCAN 5/6  
 Misc :  
 MS Integration Params: GOOFY.P  
 Quant Time: May 13 12:39 2002

Vial: 13  
 Operator:  
 Inst : 209  
 Multiplr: 1.00

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)  
 Title : 209 625/TCLP calibration table  
 Last Update : Mon May 13 12:35:42 2002  
 Response via : Initial Calibration  
 DataAcq Meth : GCMS0507

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev (Min) |
|---------------------------|-------|------|----------|-------|-------|-----------|
| 1) 1,4-Dichlorobenzene-d4 | 12.16 | 152  | 572175   | 40.00 | ug/l  | -0.04     |
| 10) Naphthalene-d8        | 15.80 | 136  | 2056919  | 40.00 | ug/l  | -0.04     |
| 17) Acenaphthene-d10      | 21.10 | 164  | 1131008  | 40.00 | ug/l  | -0.04     |
| 30) Phenanthrene-d10      | 25.55 | 188  | 1536487  | 40.00 | ug/l  | -0.03     |
| 38) Chrysene-d12          | 33.62 | 240  | 974481   | 40.00 | ug/l  | -0.02     |
| 44) Perylene-d12          | 37.84 | 264  | 649798   | 40.00 | ug/l  | -0.02     |

## System Monitoring Compounds

|               |        |     |          |      |        |       |
|---------------|--------|-----|----------|------|--------|-------|
| 28) TCMX      | 23.25  | 209 | 37974    | 6.75 | ug/L   | -0.03 |
| Spiked Amount | 10.000 |     | Recovery | =    | 67.50% |       |

## Target Compounds

|                                 |       |     |      |      |  |  |
|---------------------------------|-------|-----|------|------|--|--|
| 2) N-nitrosodimethylamine       | 5.32  | 74  | 950  | N.D. |  |  |
| 3) bis(2-Chloroethyl) ether     | 0.00  | 93  | 0    | N.D. |  |  |
| 4) 1,3-Dichlorobenzene          | 0.00  | 146 | 0    | N.D. |  |  |
| 5) 1,4-Dichlorobenzene          | 0.00  | 146 | 0    | N.D. |  |  |
| 6) 1,2-Dichlorobenzene          | 0.00  | 146 | 0    | N.D. |  |  |
| 7) 2,2'-oxybis(1-Chloropropan   | 0.00  | 45  | 0    | N.D. |  |  |
| 8) N-Nitrosodi-n-propylamine    | 0.00  | 70  | 0    | N.D. |  |  |
| 9) Hexachloroethane             | 0.00  | 117 | 0    | N.D. |  |  |
| 11) Nitrobenzene                | 13.39 | 77  | 787  | N.D. |  |  |
| 12) Isophorone                  | 0.00  | 82  | 0    | N.D. |  |  |
| 13) bis(2-Chloroethoxy) methane | 0.00  | 93  | 0    | N.D. |  |  |
| 14) 1,2,4-Trichlorobenzene      | 0.00  | 180 | 0    | N.D. |  |  |
| 15) Naphthalene                 | 15.85 | 128 | 189  | N.D. |  |  |
| 16) Hexachlorobutadiene         | 0.00  | 225 | 0    | N.D. |  |  |
| 18) Hexachlorocyclopentadiene   | 0.00  | 237 | 0    | N.D. |  |  |
| 19) 2-Chloronaphthalene         | 0.00  | 162 | 0    | N.D. |  |  |
| 20) Dimethylphthalate           | 0.00  | 163 | 0    | N.D. |  |  |
| 21) 2,6-Dinitrotoluene          | 0.00  | 165 | 0    | N.D. |  |  |
| 22) Acenaphthylene              | 0.00  | 152 | 0    | N.D. |  |  |
| 23) Acenaphthene                | 0.00  | 153 | 0    | N.D. |  |  |
| 24) 2,4-Dinitrotoluene          | 21.35 | 165 | 178  | N.D. |  |  |
| 25) Diethylphthalate            | 22.59 | 149 | 1610 | N.D. |  |  |
| 26) 4-Chlorophenylphenylether   | 0.00  | 204 | 0    | N.D. |  |  |
| 27) Fluorene                    | 0.00  | 166 | 0    | N.D. |  |  |
| 29) Azobenzene                  | 0.00  | 77  | 0    | N.D. |  |  |
| 31) N-Nitrosodiphenylamine      | 0.00  | 168 | 0    | N.D. |  |  |
| 32) 4-Bromophenylphenylether    | 0.00  | 248 | 0    | N.D. |  |  |
| 33) Hexachlorobenzene           | 0.00  | 284 | 0    | N.D. |  |  |
| 34) Phenanthrene                | 25.56 | 178 | 496  | N.D. |  |  |

Qvalue

(# ) = qualifier out of range (m) = manual integration

LBA.D GCMS0510.M Mon May 13 12:42:27 2002

Page 1

## Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY1002\LBA.D  
Acq On : 11 May 2002 12:46 am  
Sample : GC/MS SCAN 5/6  
Misc :  
MS Integration Params: GOOFY.P  
Quant Time: May 13 12:39 2002

Vial: 13  
Operator:  
Inst : 209  
Multiplr: 1.00

Quant Results File: GCMS0510.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)  
Title : 209 625/TCLP calibration table  
Last Update : Mon May 13 12:35:42 2002  
Response via : Initial Calibration  
DataAcq Meth : GCMS0507

| Compound                       | R.T.  | QIon | Response | Conc Unit | Qvalue |
|--------------------------------|-------|------|----------|-----------|--------|
| 35) Anthracene                 | 25.56 | 178  | 496      | N.D.      |        |
| 36) Di-n-butylphthalate        | 27.53 | 149  | 6967     | N.D.      |        |
| 37) Fluoranthene               | 0.00  | 202  | 0        | N.D.      |        |
| 39) Pyrene                     | 0.00  | 202  | 0        | N.D.      |        |
| 40) Butylbenzylphthalate       | 0.00  | 149  | 0        | N.D.      |        |
| 41) Benzo(a)anthracene         | 33.62 | 228  | 2171     | N.D.      |        |
| 42) Bis(2-ethylhexyl)phthalate | 33.84 | 149  | 3700     | N.D.      |        |
| 43) Chrysene                   | 33.62 | 228  | 2171     | N.D.      |        |
| 45) Di-n-Octylphthalate        | 0.00  | 149  | 0        | N.D.      |        |
| 46) Benzo(b)fluoranthene       | 0.00  | 252  | 0        | N.D.      |        |
| 47) Benzo(k)fluoranthene       | 0.00  | 252  | 0        | N.D.      |        |
| 48) Benzo(a)pyrene             | 37.84 | 252  | 2487     | N.D.      |        |
| 49) Indeno(1,2,3-cd)pyrene     | 0.00  | 276  | 0        | N.D.      |        |
| 50) Dibenz(a,h)anthracene      | 0.00  | 278  | 0        | N.D.      |        |
| 51) Benzo(g,h,i)perylene       | 0.00  | 276  | 0        | N.D.      |        |

-----  
(#) = qualifier out of range (m) = manual integration  
LBA.D GCMS0510.M Mon May 13 12:42:28 2002


## Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY1002\LBA.D  
Acq On : 11 May 2002 12:46 am  
Sample : GC/MS SCAN 5/6  
Misc :  
MS Integration Params: GOOFY.P  
Quant Time: May 13 12:39 2002

Vial: 13  
Operator:  
Inst : 209  
Multiplr: 1.00

Quant Results File: GCMS0510.RES

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)  
Title : 209 625/TCLP calibration table  
Last Update : Mon May 13 12:35:42 2002  
Response via : Initial Calibration

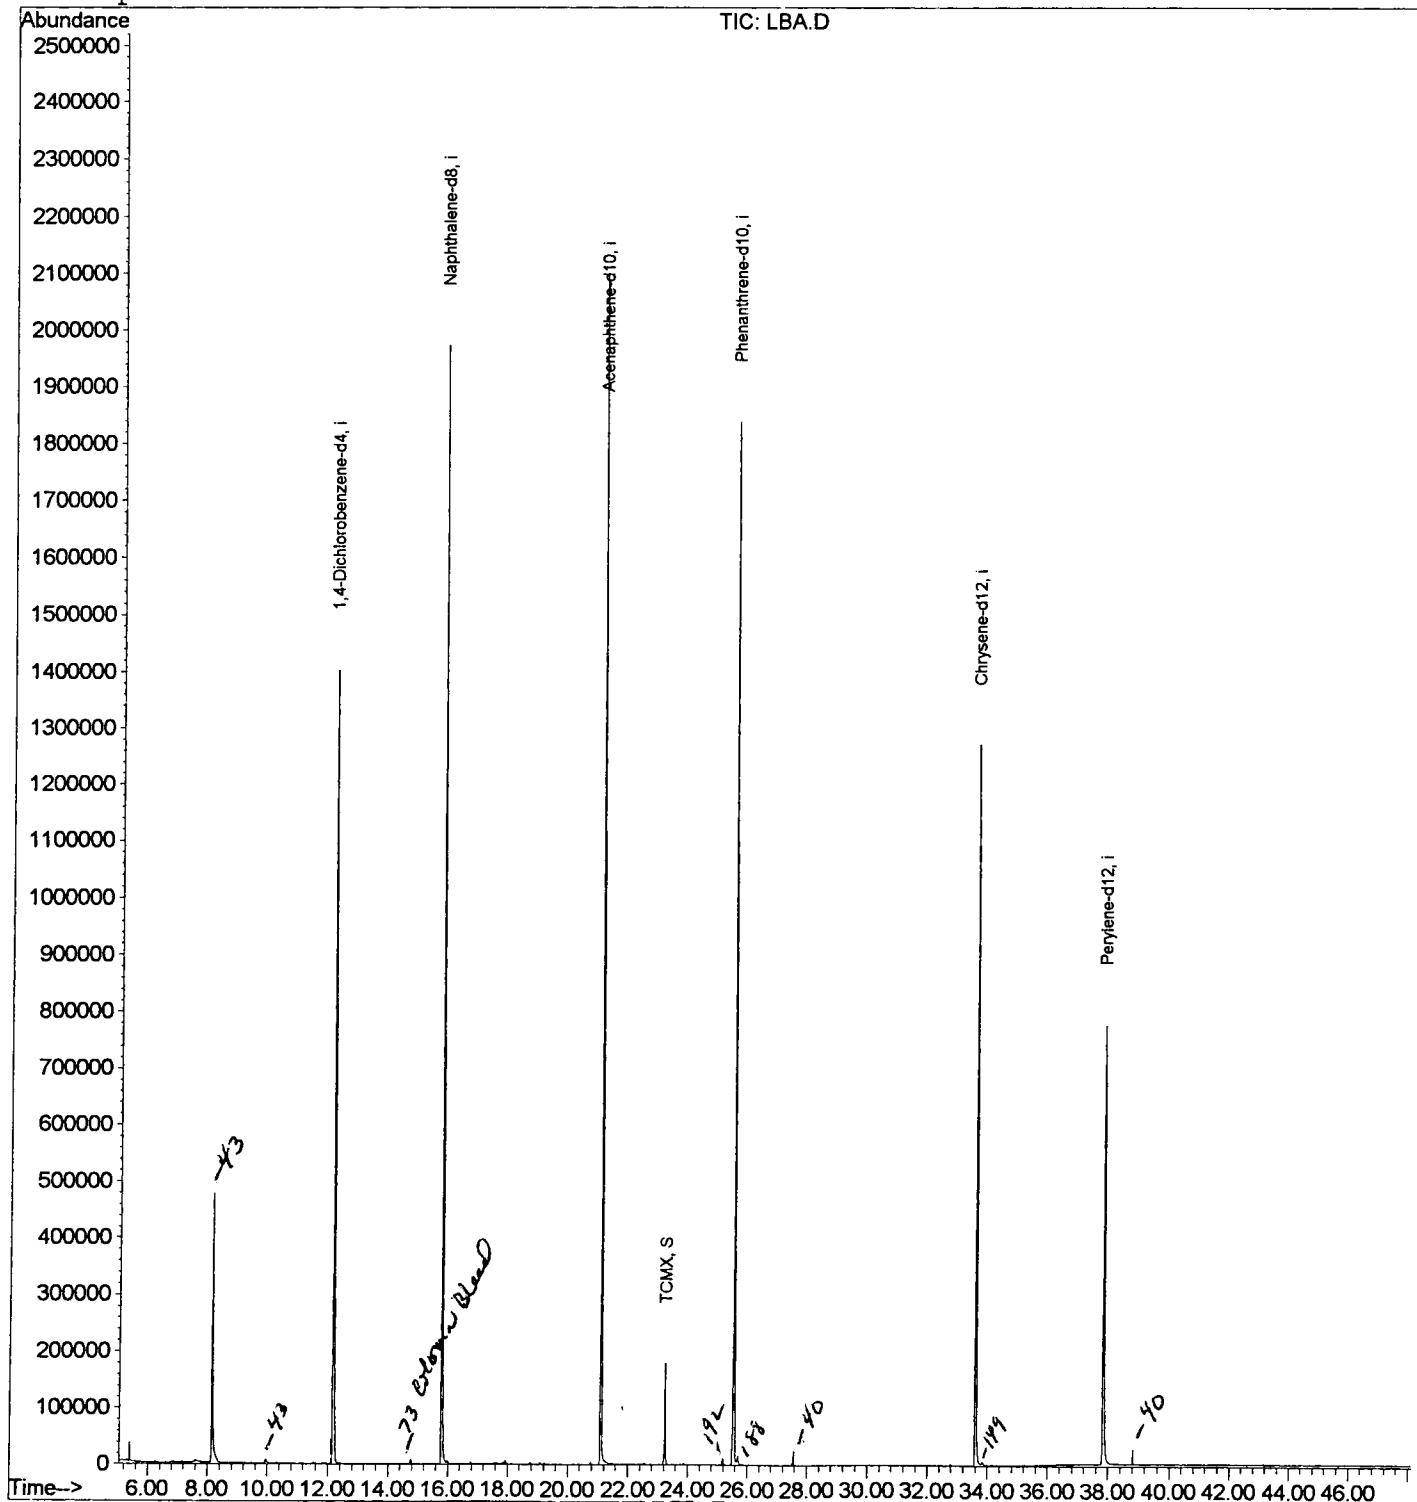

# LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY1002\LBA.D  
 Acq On : 11 May 2002 12:46 am  
 Sample : GC/MS SCAN 5/6  
 Misc :  
 MS Integration Params: LSCINT.P

Vial: 13  
 Operator:  
 Inst : 209  
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)  
 Title : 209 625/TCLP calibration table  
 Smoothing : OFF  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 1 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Signal : TIC


| peak # | R.T. min | first scan | max scan | last scan | PK TY | peak height | peak area | peak % max. | % of total |
|--------|----------|------------|----------|-----------|-------|-------------|-----------|-------------|------------|
| 1      | 8.144    | 335        | 339      | 367       | rVB   | 475747      | 1072258   | 23.77%      | 4.750%     |
| 2      | 12.158   | 772        | 777      | 794       | rVB   | 1400175     | 3248282   | 72.00%      | 14.390%    |
| 3      | 15.796   | 1168       | 1174     | 1190      | rBV   | 1971589     | 4046044   | 89.69%      | 17.924%    |
| 4      | 21.102   | 1747       | 1753     | 1767      | rBV   | 2100012     | 4511335   | 100.00%     | 19.985%    |
| 5      | 23.246   | 1977       | 1987     | 1996      | rBV   | 179855      | 373052    | 8.27%       | 1.653%     |
| 6      | 25.546   | 2232       | 2238     | 2250      | rBV2  | 1837118     | 4104533   | 90.98%      | 18.183%    |
| 7      | 33.619   | 3111       | 3119     | 3138      | rBV   | 1271484     | 2931248   | 64.98%      | 12.985%    |
| 8      | 37.844   | 3571       | 3580     | 3595      | rBV2  | 774330      | 2286940   | 50.69%      | 10.131%    |

Sum of corrected areas: 22573692

LBA.D GCMS0510.M Mon May 13 12:47:35 2002

# LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY1002\LBA.D  
 Operator :  
 Acquired : 11 May 2002 12:46 am using AcqMethod GCMS0507  
 Instrument : 209  
 Sample Name: GC/MS SCAN 5/6  
 Misc Info :  
 Vial Number: 13  
 Quant File :GCMS0510.RES (RTE Integrator)

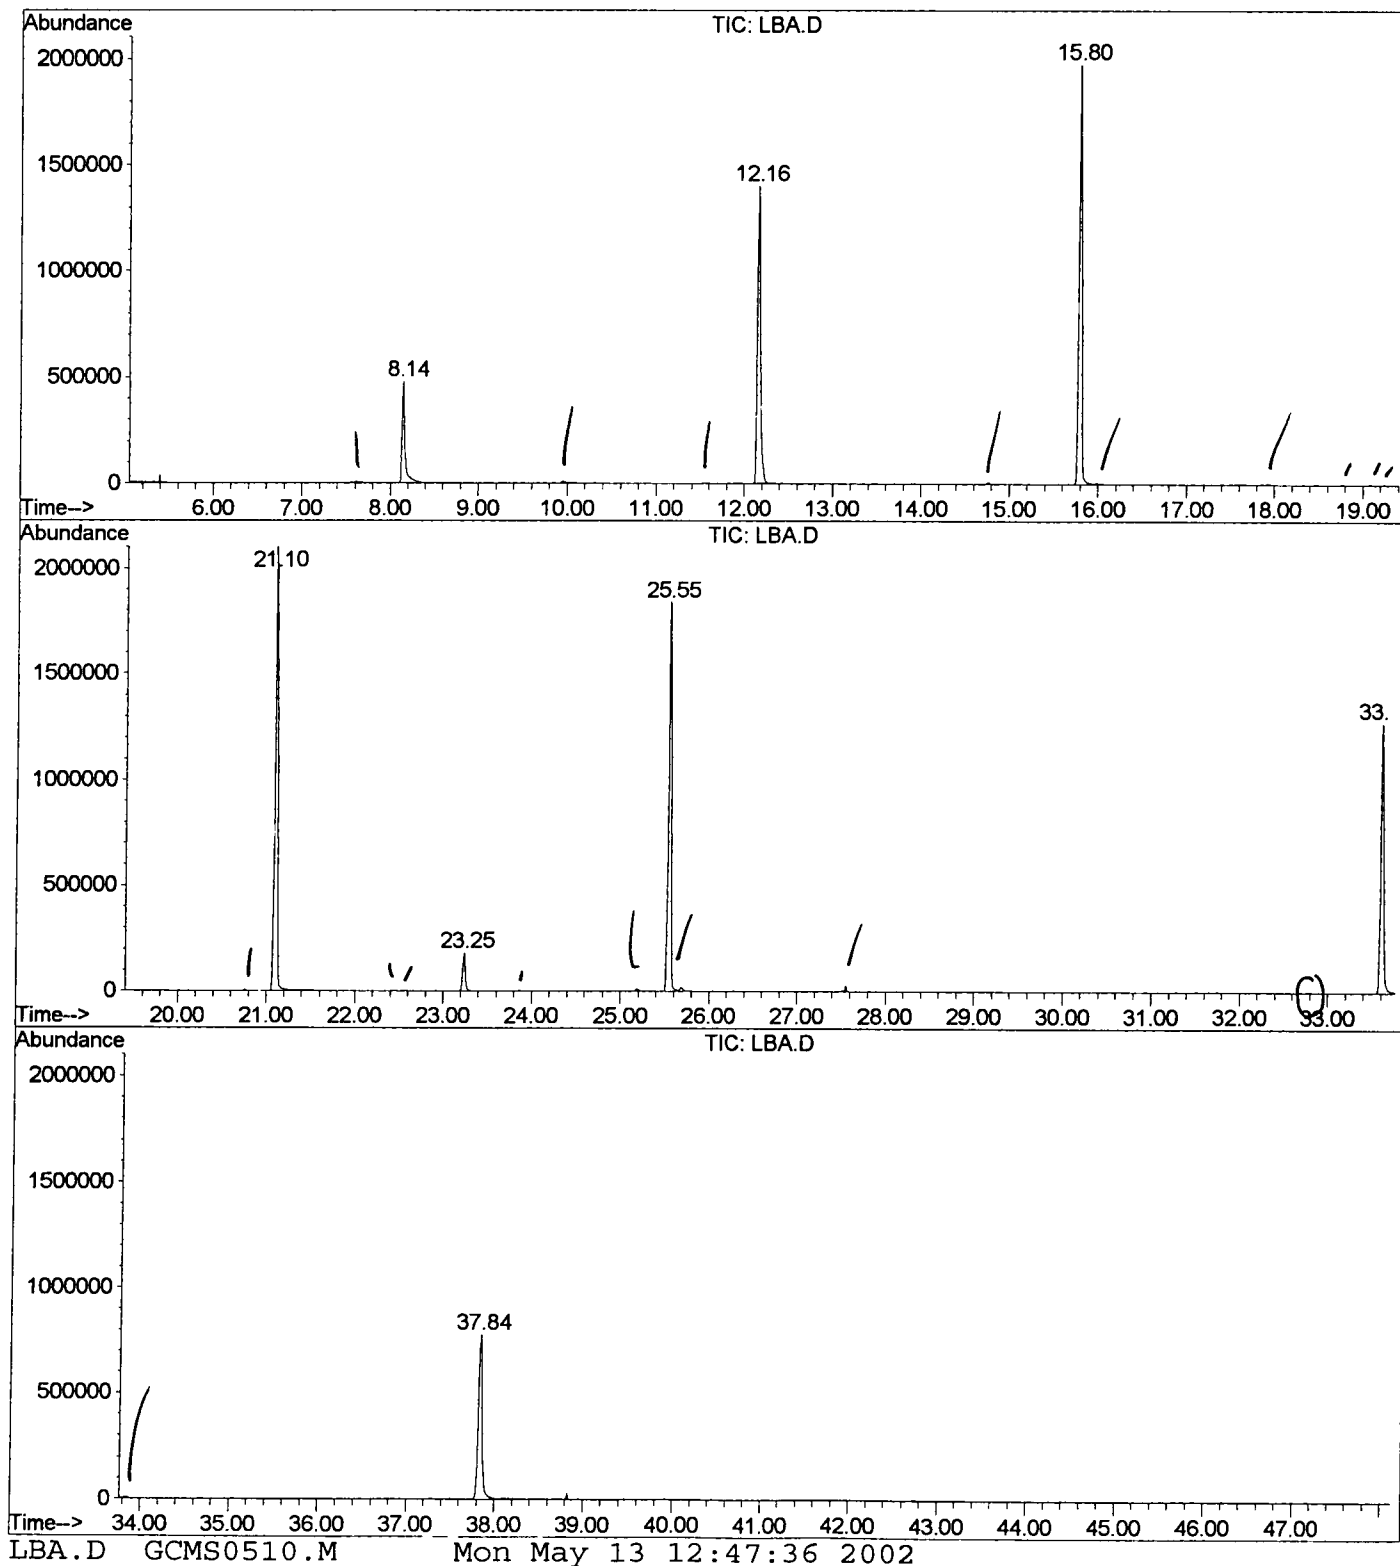

# Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY1002\LBA.D  
 Acq On : 11 May 2002 12:46 am  
 Sample : GC/MS SCAN 5/6  
 Misc :  
 MS Integration Params: LSCINT.P


Vial: 13  
 Operator:  
 Inst : 209  
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)  
 Title : 209 625/TCLP calibration table  
 Library : C:\DATABASE\NBS75K.L

\*\*\*\*\*  
 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

| R.T. | EstConc    | Area    | Relative to ISTD       | R.T.  |
|------|------------|---------|------------------------|-------|
| 8.14 | 13.20 ug/l | 1072260 | 1,4-Dichlorobenzene-d4 | 12.16 |

| Hit# | of | 5 | Tentative ID                        | MW  | MolForm | CAS#        | Qual |
|------|----|---|-------------------------------------|-----|---------|-------------|------|
| 1    |    |   | 2-Pentanone, 4-hydroxy-4-methyl-    | 116 | C6H12O2 | 000123-42-2 | 64   |
| 2    |    |   | CH2=CHCH2C(O)OCH3                   | 100 | C5H8O2  | 003724-55-8 | 9    |
| 3    |    |   | Acetic acid, 1,1-dimethylethyl este | 116 | C6H12O2 | 000540-88-5 | 9    |
| 4    |    |   | Acetone                             | 58  | C3H6O   | 000067-64-1 | 7    |

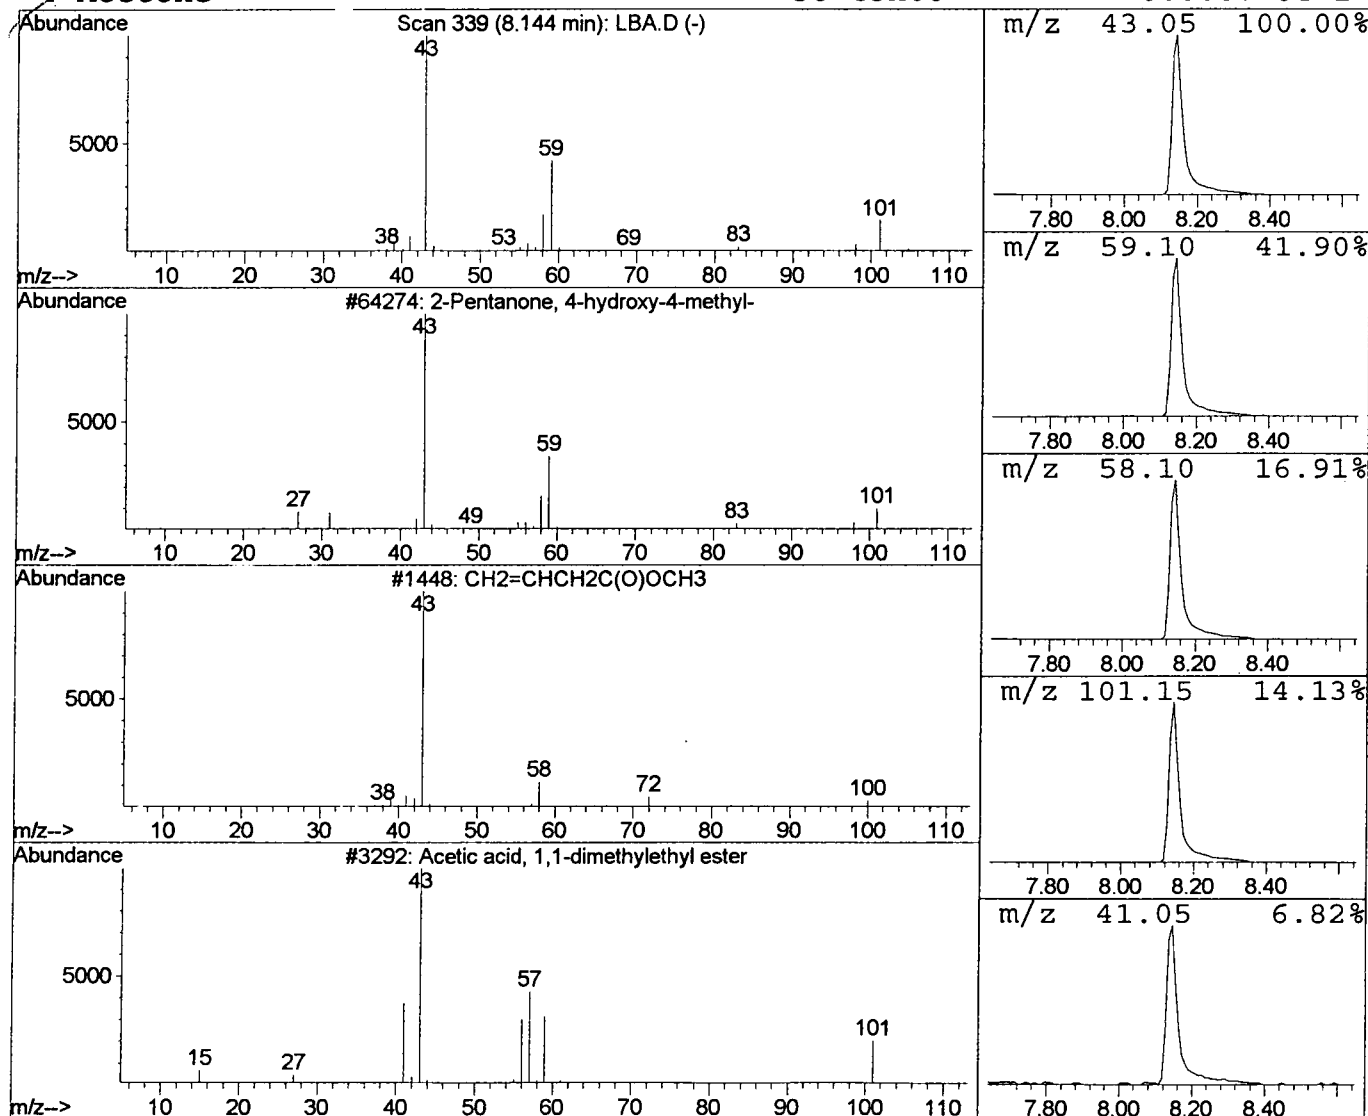

Tentatively Identified Compound (LSC) summary

Operator ID:            Date Acquired: 11 May 2002 12:46 am  
 Data File: C:\HPCHEM\1\DATA\MAY1002\LBA.D  
 Name: GC/MS SCAN 5/6  
 Misc:  
 Method: C:\HPCHEM\1\METHODS\GCMS0510.M (RTE Integrator)  
 Title: 209 625/TCLP calibration table  
 Library Searched: C:\DATABASE\NBS75K.L

| TIC Top Hit name                | RT   | EstConc | Units | Area    | IntStd | ISRT  | ISArea  | ISConc |
|---------------------------------|------|---------|-------|---------|--------|-------|---------|--------|
| <del>2-Pentanone, 4-hydro</del> | 8.14 | 13.2    | ug/l  | 1072260 | ISTD01 | 12.16 | 3248280 | 40.0   |

LBA.D GCMS0510.M Mon May 13 12:47:37 2002