

Method 508 MOD.

Date Extracted 5/7/02

Page 104

Ref

HGCMs - 18428

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500ml		1ml			1ml	3A	7			
Ref 1					1ml			4A				
Ref 2					1ml			3B				
9579								2A				
9580								2B				
9585								9B				
9586								9A				
9587	Q, FB							1A				
9334	Q 2-Indifferent batch							10A				
10807	Q							1B				
10808								10B				
Remarks ① Na OH WAS ADDED TO ALL Q-SAMPLES TO bring THEIR PH TO SEVEN ② (ALL) RE EXTRACTS Reviewed by, <u>C/B 8/22/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type - <u>SEP. Fun.</u> Solv.lot# <u>X05E10</u> NaCl lot# <u>1/39614</u> Na2SO4 lot# <u>1/46648</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>HP050602</u>											
(REF) SPIKE	<u>2279E</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>050708</u>											
SURROGATE	<u>IST 440</u>											
LPC												
ENDRIN/DDT												

Analyst A.D.
Revision 4/12/01

Verified by my

Reviewed by DP
Date 5/17/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAY0802.S
 Comment:
 Operator:
 Data Path: C:\HPCHEM\1\DATA\MAY0802\
 Pre-Seq Cmd:
 Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0507	
2	Sample	2	CAL80	GCMS0507	
3	Sample	3	LB	GCMS0507	GC/MS SCAN 5/3
4	Sample	100	SURR	GCMS0507	
5	Sample	4	REF1	GCMS0507	GC/MS SCAN 5/3
6	Sample	5	REF2	GCMS0507	GC/MS SCAN 5/3
7	Sample	6	10607	GCMS0507	GC/MS SCAN 5/3
8	Sample	7	10608	GCMS0507	GC/MS SCAN 5/3
9	Sample	8	9391	GCMS0507	RE-EXT.
10	Sample	9	9448	GCMS0507	RE-EXT.
11	Sample	10	9449	GCMS0507	RE-EXT.
12	Sample	11	9451	GCMS0507	RE-EXT.
13	Sample	12	9447	GCMS0507	RE-EXT.
14	Sample	13	LBA	GCMS0507	GC/MS SCAN 5/7
15	Sample	14	REFA1	GCMS0507	GC/MS SCAN 5/7
16	Sample	15	REFA2	GCMS0507	GC/MS SCAN 5/7
17	Sample	16	9579	GCMS0507	RE-EXT.
18	Sample	17	9580	GCMS0507	RE-EXT.
19	Sample	18	9585	GCMS0507	RE-EXT.
20	Sample	19	9586	GCMS0507	RE-EXT.
21	Sample	20	9587	GCMS0507	RE-EXT.
22	Sample	21	9334	GCMS0507	RE-EXT.
23	Sample	22	10807	GCMS0507	GC/MS SCAN 5/7
24	Sample	23	10808	GCMS0507	GC/MS SCAN 5/7

DFTPP

Data File : C:\HPCHEM\1\DATA\MAY0802\DFTPP.D
 Acq On : 8 May 2002 9:36 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0507.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

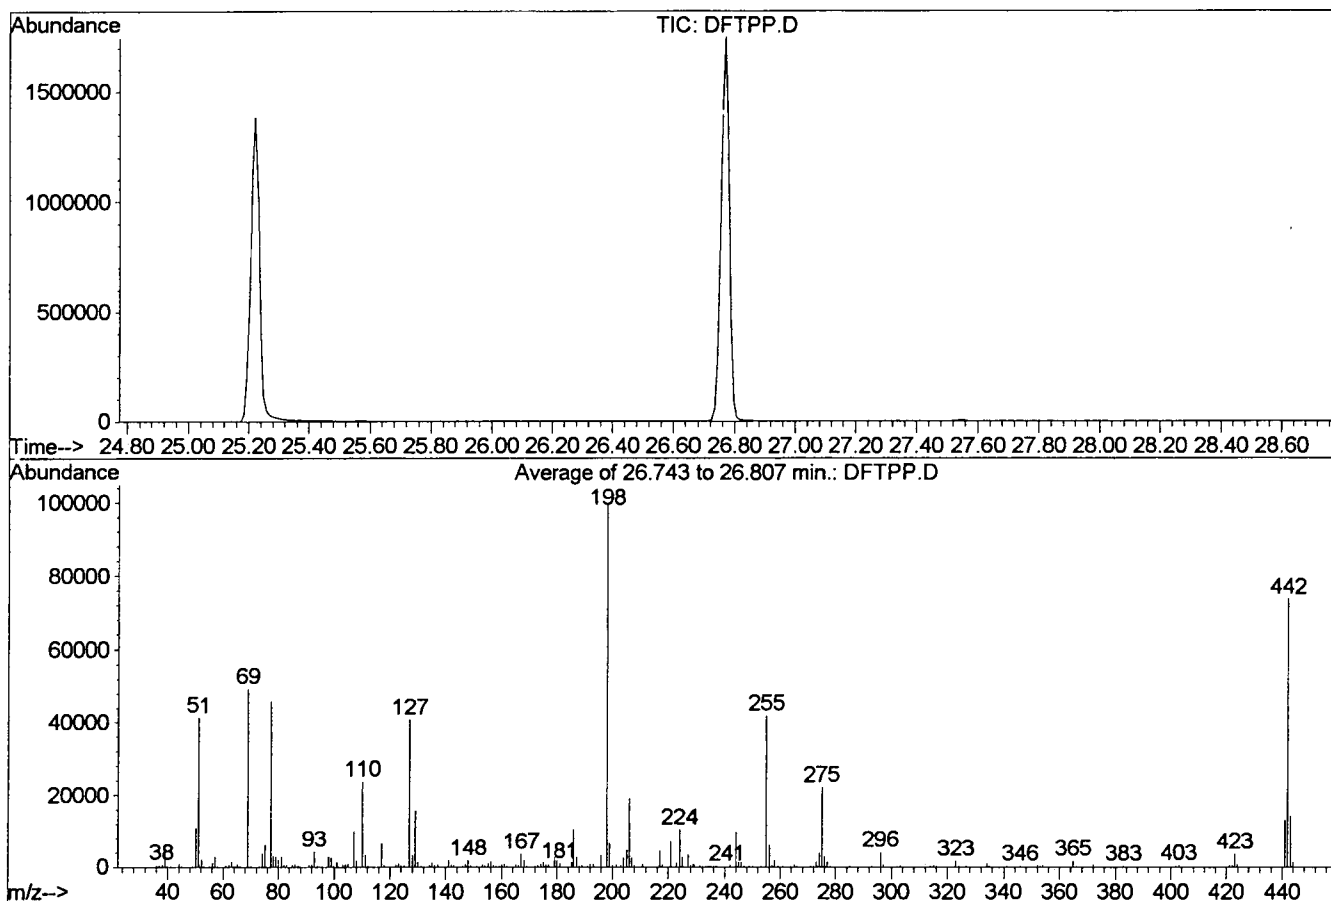

Spectrum Information: Average of 26.743 to 26.807 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.4	41348	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.5	49407	PASS
70	69	0.00	2	0.1	42	PASS
127	198	40	60	40.9	40836	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	99832	PASS
199	198	5	9	6.6	6572	PASS
275	198	10	30	22.1	22107	PASS
365	198	1	100	1.6	1636	PASS
441	443	0.01	100	92.3	13033	PASS
442	198	40	110	73.8	73725	PASS
443	442	17	23	19.2	14124	PASS