

Method 508mod.

Date Extracted 4-17-02

Page 64

Ref

#6CMS-18166

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
<u>LB</u>		<u>500ml</u>		<u>1ml</u>			<u>1ml</u>	<u>1B</u>	<u>7</u>			
<u>Ref.</u>					<u>1ml</u>			<u>1A</u>				
<u>Ref.</u>					<u>↓</u>			<u>4A</u>				
<u>58415</u>	<u>Re-ext.</u>							<u>7A</u>				
<u>9095</u>								<u>7B</u>				
<u>9096</u>	<u>FB</u>							<u>4B</u>				
<u>9097</u>								<u>2B</u>				
<u>9098</u>	<u>see 4/24</u>							<u>8A</u>				
<u>9099</u>								<u>8B</u>				
<u>9100</u>	<u>FB</u>							<u>6A</u>				
<u>9150</u>		<u>↓</u>		<u>↓</u>			<u>↓</u>	<u>2A</u>	<u>↓</u>			
Remarks												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - <u>Self Fun</u> Solv. lot# <u>41470</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V46648</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>12041002</u>											
REF/SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>041902</u>											
SURROGATE	<u>TCM X</u>											
LPC												
ENDRN/DDT												

Reviewed by SPB 8/16/02

Analyst E.H.
revision 4/12/01

Verified by hzy

Reviewed by DR
Date 4/26/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\APR2302.S
Comment:
Operator:
Data Path: C:\HPCHEM\1\DATA\APR2302\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0412	
2	Sample	2	CAL80	GCMS0412	
3	Sample	3	LB	GCMS0412	gc/ms scan 4/15
4	Sample	4	REF1	GCMS0412	gc/ms scan 4/15
5	Sample	5	REF2	GCMS0412	gc/ms scan 4/15
6	Sample	6	8837	GCMS0412	gc/ms scan 4/15
7	Sample	7	8838	GCMS0412	gc/ms scan 4/15
8	Sample	8	8839	GCMS0412	gc/ms scan 4/15
9	Sample	9	8840	GCMS0412	gc/ms scan 4/15 fb
10	Sample	10	8930	GCMS0412	gc/ms scan 4/15
11	Sample	11	8931	GCMS0412	gc/ms scan 4/15
12	Sample	12	8932	GCMS0412	gc/ms scan 4/15
13	Sample	13	8933	GCMS0412	gc/ms scan 4/15
14	Sample	14	8934	GCMS0412	gc/ms scan 4/15
15	Sample	15	8935	GCMS0412	gc/ms scan 4/15
16	Sample	16	LBA	GCMS0412	gc/ms scan 4/17
17	Sample	17	REFA1	GCMS0412	gc/ms scan 4/17
18	Sample	18	REFA2	GCMS0412	gc/ms scan 4/17
19	Sample	19	5845	GCMS0412	gc/ms scan 4/17
20	Sample	20	9095	GCMS0412	gc/ms scan 4/17
21	Sample	21	9096	GCMS0412	gc/ms scan 4/17 fb
22	Sample	22	9097	GCMS0412	gc/ms scan 4/17
23	Sample	23	9099	GCMS0412	gc/ms scan 4/17
24	Sample	24	9100	GCMS0412	gc/ms scan 4/17 fb
25	Sample	25	9150	GCMS0412	gc/ms scan 4/17

DFTPP

Data File : C:\HPCHEM\1\DATA\APR2302\DFTPP.D

Vial: 1

Acq On : 23 Apr 2002 2:17 pm

Operator:

Sample :

Inst : 209


Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

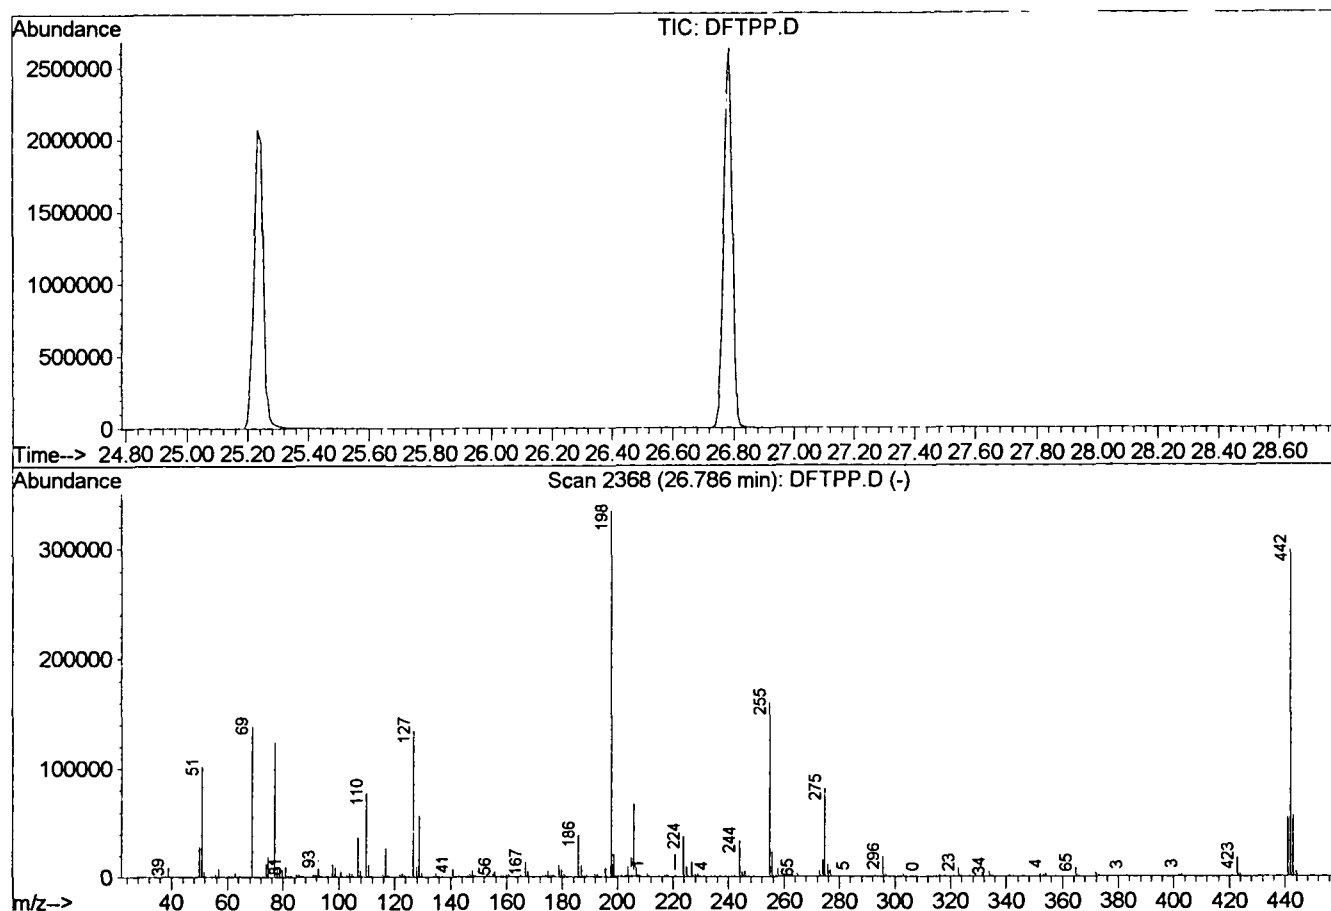

Spectrum Information: Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	30.4	101808	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.5	138944	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	40.3	134656	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	334464	PASS
199	198	5	9	6.4	21360	PASS
275	198	10	30	24.4	81456	PASS
365	198	1	100	2.4	8170	PASS
441	443	0.01	100	95.2	53704	PASS
442	198	40	110	89.1	297984	PASS
443	442	17	23	18.9	56424	PASS