

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/26/2002 Time: 14:09:06

Sample: AE09099
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/26/02 14:08 Ended: 4/26/02 14:08 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Quantity	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		90		10.0

Comments for Sample AE09099 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-26-2002 Time: 14:09:30

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2302\9099.D
 Acq On : 24 Apr 2002 12:53 pm
 Sample : gc/ms scan 4/17
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 24 14:17 2002

Vial: 23
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 17 11:48:30 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	473995	20.00	ug/l	-0.03
10) Naphthalene-d8	15.84	136	1743144	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.15	164	985829	20.00	ug/l	-0.02
30) Phenanthrene-d10	25.58	188	1437463	20.00	ug/l	-0.03
39) Chrysene-d12	33.64	240	912134	20.00	ug/l	-0.03
45) Perylene-d12	37.88	264	546257	20.00	ug/l	-0.04

System Monitoring Compounds

28) TCMX	23.28	209	44331	8.97	ug/L	-0.05
Spiked Amount	10.000		Recovery	=	89.70%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.90	128	272	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.63	149	485	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

9099.D GCMS0412.M Wed Apr 24 14:18:37 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR2302\9099.D

Vial: 23

Acq On : 24 Apr 2002 12:53 pm

Operator:

Sample : gc/ms scan 4/17

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 24 14:17 2002

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Apr 17 11:48:30 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.58	178	545	N.D.		
35) Anthracene	25.58	178	442	N.D.		
36) Di-n-butylphthalate	27.56	149	2409	N.D.		
37) Fluoranthene	29.27	202	1068	N.D.		
40) Pyrene	29.95	202	801	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.65	228	2868	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.87	149	41975	1.83 ug/l	#	99
44) Chrysene	33.71	228	505	N.D.		
46) Di-n-Octylphthalate	35.60	149	197	N.D.		
47) Benzo(b)fluoranthene	0.00	252	0	N.D.		
48) Benzo(k)fluoranthene	0.00	252	0	N.D.		
49) Benzo(a)pyrene	37.88	252	2059	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

9099.D GCMS0412.M Wed Apr 24 14:18:38 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR2302\9099.D
 Acq On : 24 Apr 2002 12:53 pm
 Sample : gc/ms scan 4/17
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 24 14:17 2002

Vial: 23
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 17 11:48:30 2002
 Response via : Initial Calibration

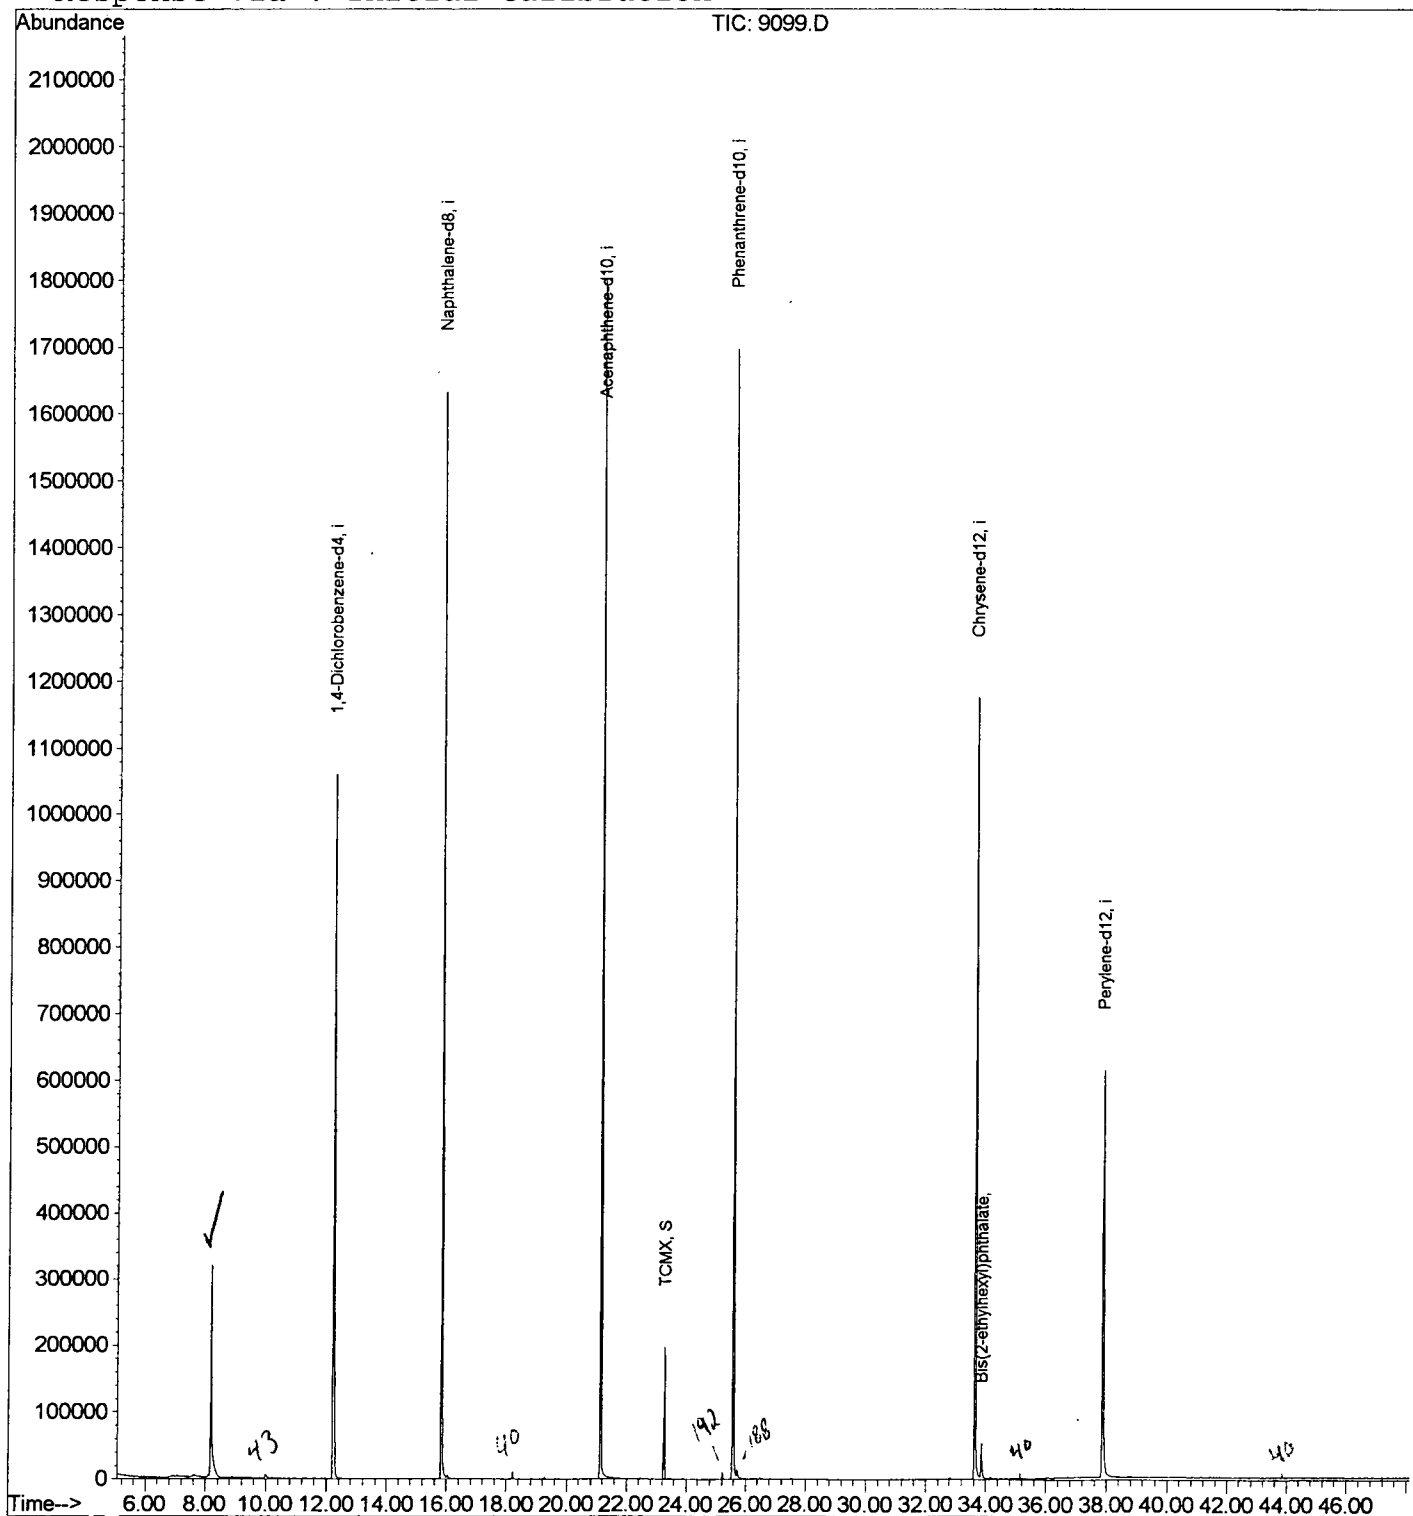

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR2302\9099.D
Acq On : 24 Apr 2002 12:53 pm
Sample : gc/ms scan 4/17
Misc :
MS Integration Params: LSCINT.P

Vial: 23
Operator:
Inst : 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.188	338	342	371	rVB	318965	784796	20.93%	4.130%
2	12.209	775	780	794	rBV	1059953	2551048	68.04%	13.426%
3	15.844	1170	1176	1193	rBV	1632347	3288719	87.71%	17.308%
4	21.150	1747	1754	1769	rBV	1803864	3749474	100.00%	19.733%
5	23.280	1978	1986	1993	rBV	198463	396572	10.58%	2.087%
6	25.584	2231	2237	2249	rBV2	1697246	3613061	96.36%	19.015%
7	33.645	3108	3115	3134	rBV	1176380	2629875	70.14%	13.841%
8	33.865	3134	3139	3151	rVB	52896	133950	3.57%	0.705%
9	37.877	3567	3576	3593	rBV	612936	1853544	49.43%	9.755%

Sum of corrected areas: 19001039

9099.D GCMS0412.M Wed Apr 24 14:19:07 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR2302\9099.D
 Operator :
 Acquired : 24 Apr 2002 12:53 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: gc/ms scan 4/17
 Misc Info :
 Vial Number: 23
 Quant File :GCMS0412.RES (RTE Integrator)

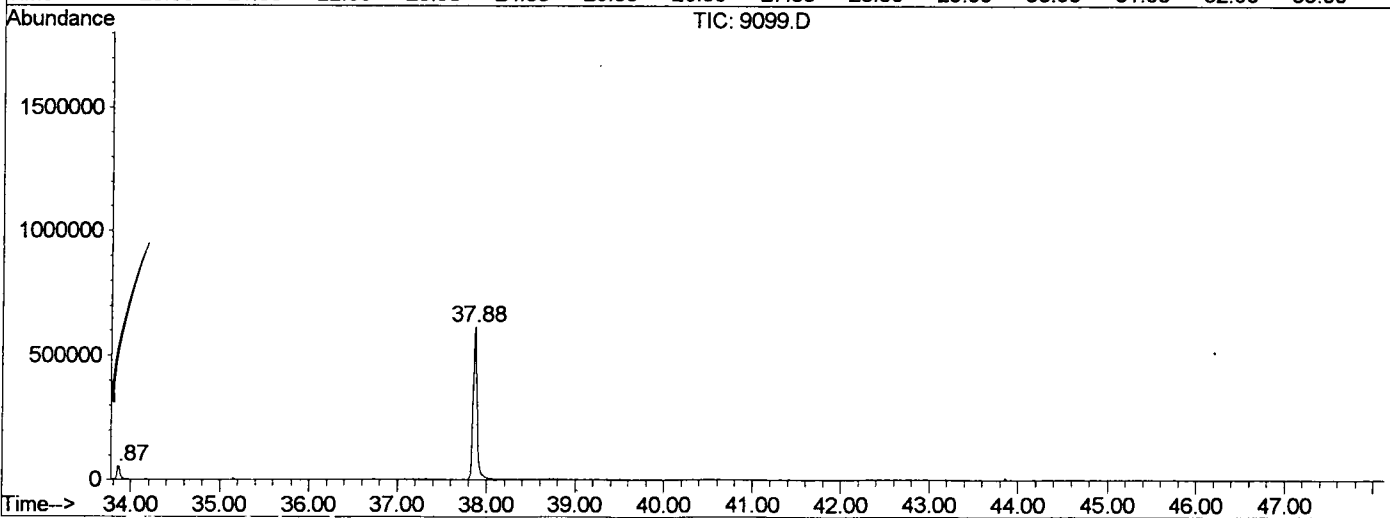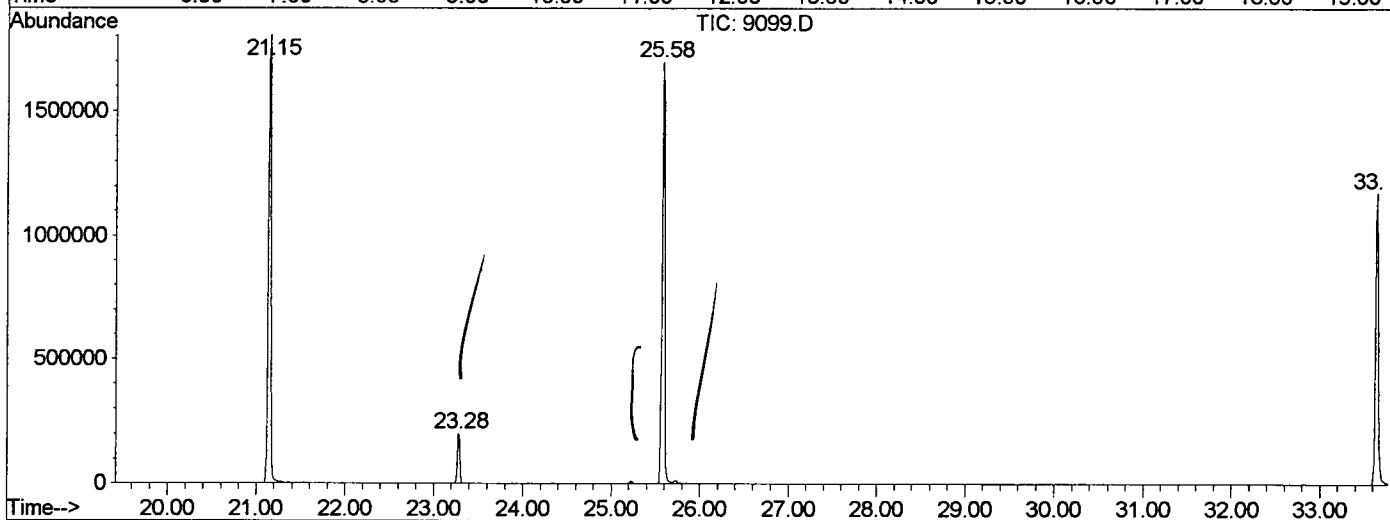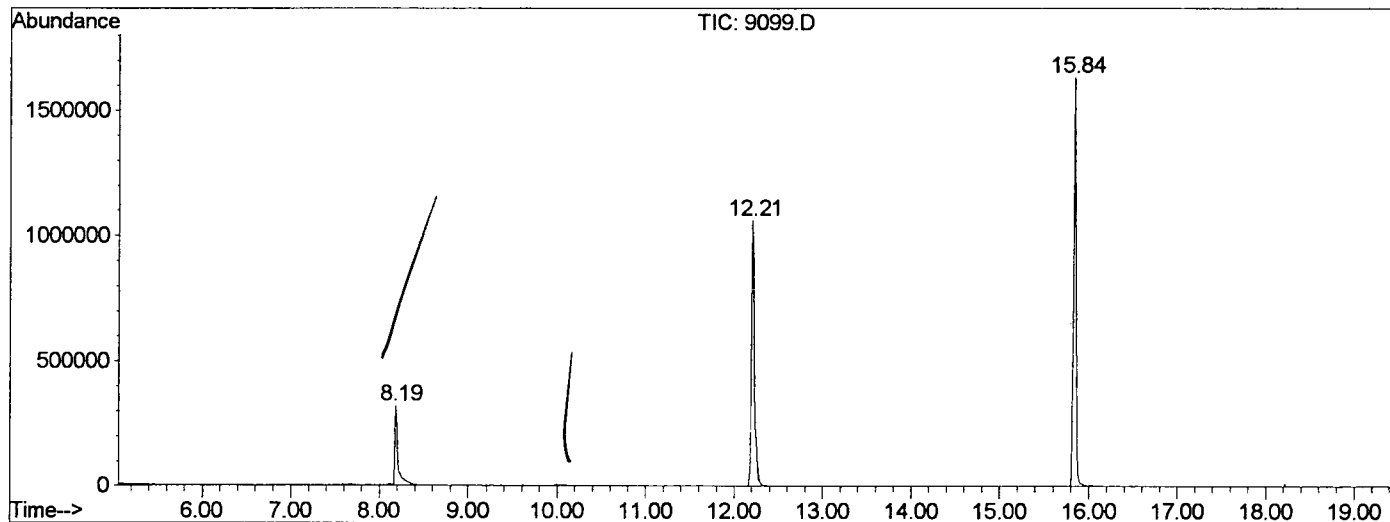

9099.D GCMS0412.M Wed Apr 24 14:19:08 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR2302\9099.D
 Acq On : 24 Apr 2002 12:53 pm
 Sample : gc/ms scan 4/17
 Misc :
 MS Integration Params: LSCINT.P


Vial: 23
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.19	6.15 ug/l	784796	1,4-Dichlorobenzene-d4	12.21

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33	
3	Acetic acid, cyano-, 1,1-dimethylet	141	C7H11NO2	001116-98-9	17	
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9	

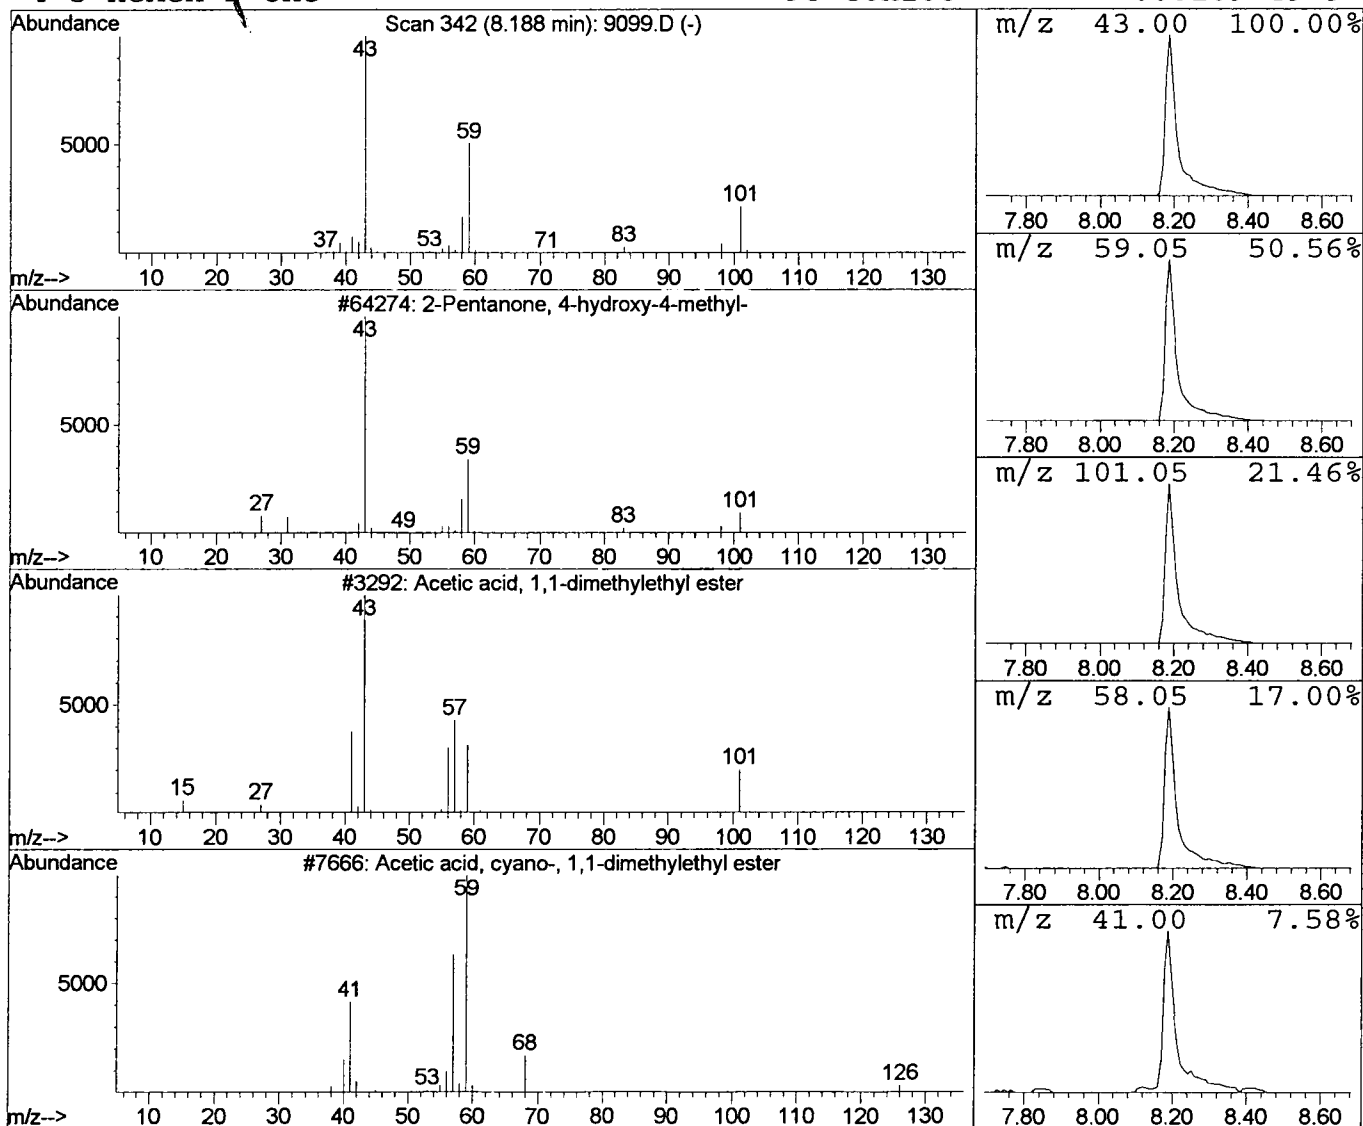

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 24 Apr 2002 12:53 pm
 Data File: C:\HPCHEM\1\DATA\APR2302\9099.D
 Name: gc/ms scan 4/17
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.19	6.2	ug/l	784796	ISTD01	12.21	2551050	20.0

9099.D GCMS0412.M Wed Apr 24 14:19:09 2002