

DFTPP

Data File : C:\HPCHEM\1\DATA\APR0302\DFTPP.D

Acq On : 3 Apr 2002 11:40 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

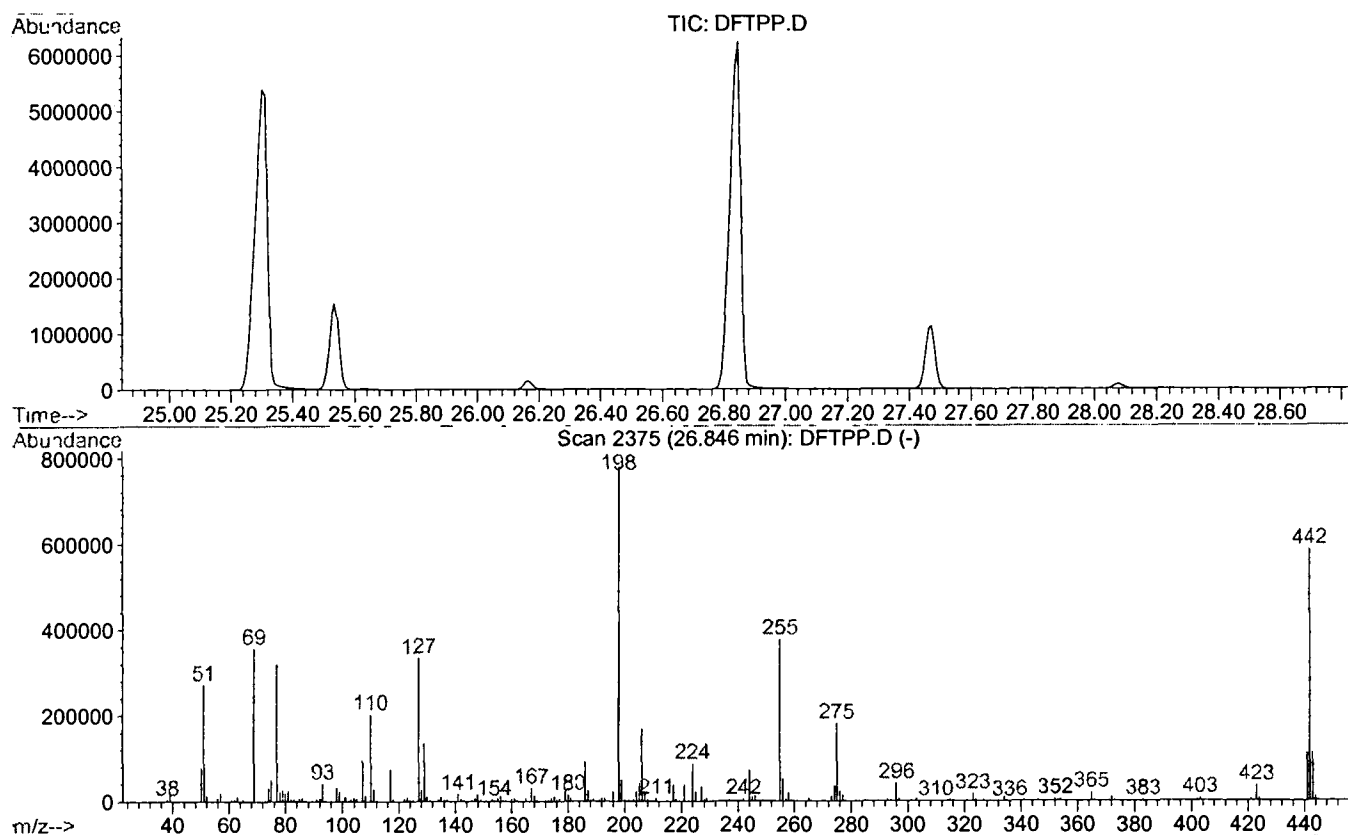

Spectrum Information: Scan 2375

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.9	271588	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.9	356985	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	43.0	334372	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	778102	PASS
199	198	5	9	6.4	49824	PASS
275	198	10	30	23.4	182123	PASS
365	198	1	100	2.6	20256	PASS
441	443	0.01	100	99.8	112656	PASS
442	198	40	110	75.2	584862	PASS
443	442	17	23	19.3	112919	PASS