

Method 508 mod.Date Extracted 4-5-02Page 46

BGCUS-18032/04/17/02

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
LB		500ml		1ml			1ml	1A	7	
Ref.					1ml			2A		
Ref.								1B		
7978								4B		
7979								4A		
8063								2B		
8064								1B		
8065								10A		
8066								4A		
8067								9B		
8068								1A		
8069								4B		
8070								10B		
7766	Re-Ext.	425						9A		
Remarks										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type <u>Sep Fun.</u>		Solv. lot# <u>V41470</u>		NaCl lot# <u>V39614</u>		Na2SO4 lot# <u>V46623</u>				
STANDARD	INT STD LOG#									
CALIBRATION										
REF SPIKE	2193									
MDL/MORF										
Q. CHECK										
INT. STD.										
SURROGATE	New Surrogate									
SP. LPC										
ENDRIN/DDT										

Analyst BH.
Revision 4/12/01

Verified by _____

Reviewed by DN
Date 4/18/02

Sequence Name: C:\MSDchem\1\sequence\020415.S
 Comment:
 Operator: GALOS
 Data Path: C:\MSDCHEM\1\DATA\MAR2102\
 Pre-Seq Cmd:
 Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP1	508FAST	
2	Sample	2	0415C3	508SCAN	ccv
3	Sample	3	TCMX	508SCAN	tcmx
4	Sample	4	0404REF1	508SCAN	04/04 ref
5	Sample	5	0404REF2	508SCAN	04/04 ref
6	Sample	6	0405REF1	508SCAN	04/05 ref
7	Sample	7	0405REF2	508SCAN	04/05 ref
8	Sample	8	0404LB	508SCAN	04/04 lab blk
9	Sample	9	0405LB	508SCAN	04/05 lab blk
10	Sample	10	07631	508SCAN	sample
11	Sample	11	07632	508SCAN	sample
12	Sample	12	07972	508SCAN	sample
13	Sample	13	07973	508SCAN	sample
14	Sample	14	07974	508SCAN	sample
15	Sample	15	07975	508SCAN	sample
16	Sample	16	07976	508SCAN	sample
17	Sample	17	07977	508SCAN	sample
18	Sample	18	07978	508SCAN	sample
19	Sample	19	07979	508SCAN	sample
20	Sample	20	08063	508SCAN	sample
21	Sample	21	08064	508SCAN	sample
22	Sample	22	08065	508SCAN	sample
23	Sample	23	08066	508SCAN	sample
24	Sample	24	08067	508SCAN	sample
25	Sample	25	08068	508SCAN	sample
26	Sample	26	08069	508SCAN	sample
27	Sample	27	08070	508SCAN	sample
28	Sample	28	07766	508SCAN	sample

DFTPP

Data File : C:\MSDCHEM\1\DATA\020415\DFTPP1.D
Acq On : 15 Apr 2002 10:43 am
Sample :
Misc :
MS Integration Params: EVENTS.E
Method : C:\MSDCHEM\1\METHODS\041202SCAN.M (Chemstation Integrator)
Title : 508 Modified GC/MS scan

Vial: 1
Operator: Nefliu
Inst : Instrume
Multiplr: 1.00

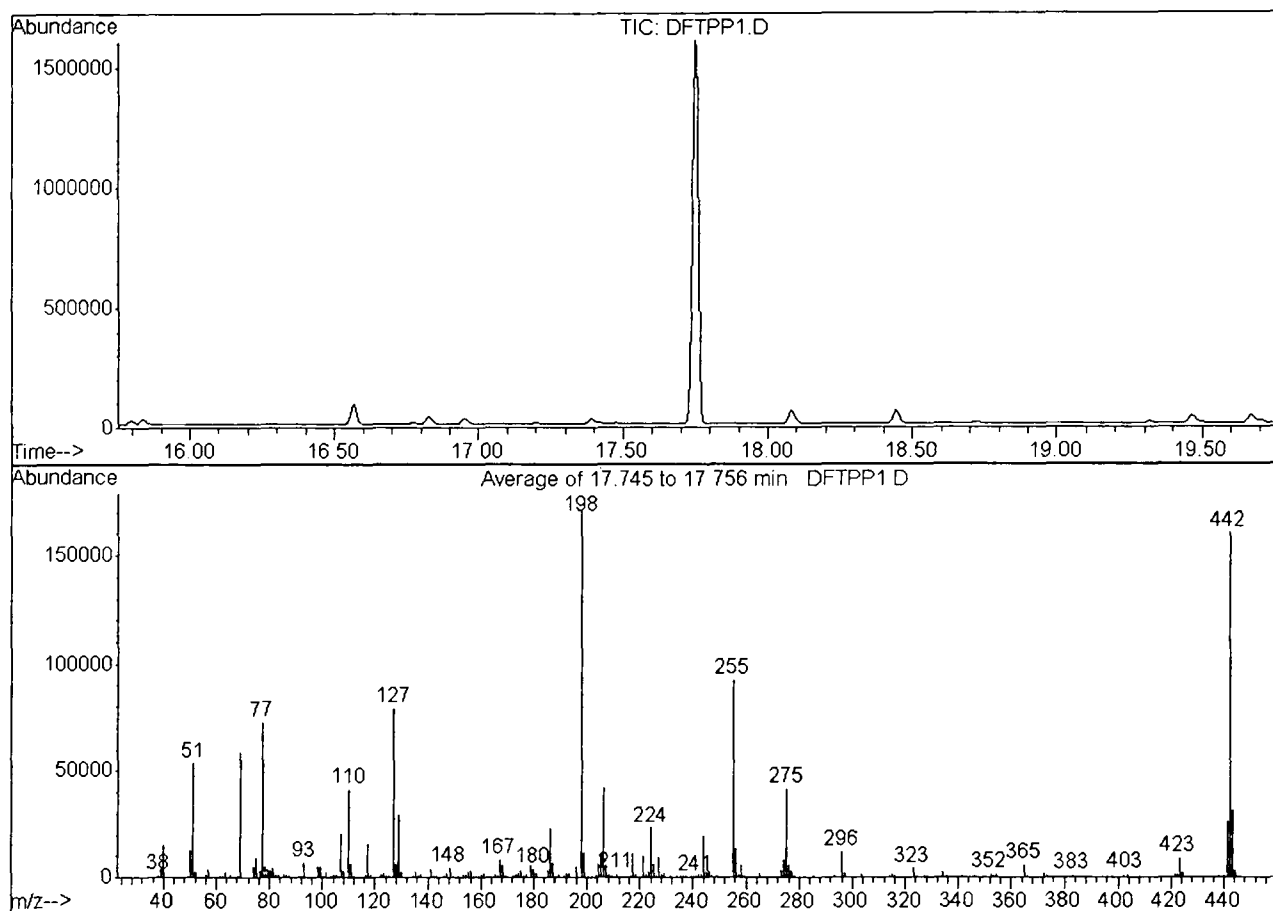

Spectrum Information: Average of 17.745 to 17.756 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	31.4	53720	PASS
68	69	0.00	2	1.4	822	PASS
69	198	0.00	100	34.1	58328	PASS
70	69	0.00	2	0.5	268	PASS
127	198	40	60	46.5	79440	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	170858	PASS
199	198	5	9	6.8	11595	PASS
275	198	10	30	24.3	41549	PASS
365	198	1	99	3.4	5765	PASS
441	443	1	100	83.6	26066	PASS
442	198	40	110	93.7	160074	PASS
443	442	17	23	19.5	31173	PASS