

Method 508 mod

Date Extracted 4-1-02

Page 36

Ref

AGCMS-18118

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spt add	IS add	Final vol.	T.V. pos.	pH	Count		
1B		500ml		1ml	1ml		1ml	1A	7			
201					↓			4A				
202								10A				
7493								2B				
7499								4B				
7500								9A				
7501	FB							6A				
7502								2A				
7503								1B				
7504								10B				
7505	FB	↓		↓			↓	9B	↓			
Remarks												
Reviewed by, <u>CB</u> 8/14/02												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type <u>Sep fun</u> Solv. lot# <u>V41470</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V4602</u>												
STANDARD INT STD LOG# GENERATION <u>170041002</u> REF SPIKE <u>2193</u> MDL/MDF Q CHECK INT. STD. <u>15041002</u> SURROGATE <u>New Surrogate</u> LPC END RUN/DOY												

Analyst EA
Revision 4/12/01

Verified by ms

Reviewed by DW
Date 4/23/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\APR1902.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\apr1802\

Pre-Seq Cmd:

Post-Seq Cmd:


Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0412	
2	Sample	2	CAL20	GCMS0412	
3	Sample	3	8269	GCMS0412	
4	Sample	4	8270	GCMS0412	
5	Sample	5	LB	GCMS0412	GC/MS SCAN 3/25
6	Sample	6	REF1	GCMS0412	GC/MS SCAN 3/25
7	Sample	7	REF2	GCMS0412	GC/MS SCAN 3/25
8	Sample	8	6981	GCMS0412	GC/MS SCAN 3/25
9	Sample	9	6982	GCMS0412	GC/MS SCAN 3/25
10	Sample	10	6983	GCMS0412	GC/MS SCAN 3/25
11	Sample	11	6984	GCMS0412	GC/MS SCAN 3/25 FB
12	Sample	12	6985	GCMS0412	GC/MS SCAN 3/25
13	Sample	13	6986	GCMS0412	GC/MS SCAN 3/25
14	Sample	14	6987	GCMS0412	GC/MS SCAN 3/25
15	Sample	15	6988	GCMS0412	GC/MS SCAN 3/25 FB
16	Sample	16	LBA	GCMS0412	GC/MS SCAN 3/26
17	Sample	17	REFA1	GCMS0412	GC/MS SCAN 3/26
18	Sample	18	REFA2	GCMS0412	GC/MS SCAN 3/26
19	Sample	19	7001	GCMS0412	GC/MS SCAN 3/26
20	Sample	20	7002	GCMS0412	GC/MS SCAN 3/26 FB
21	Sample	21	7066	GCMS0412	GC/MS SCAN 3/26
22	Sample	22	7067	GCMS0412	GC/MS SCAN 3/26
23	Sample	23	7068	GCMS0412	GC/MS SCAN 3/26 FB
24	Sample	24	7105	GCMS0412	GC/MS SCAN 3/26
25	Sample	25	7106	GCMS0412	GC/MS SCAN 3/26
26	Sample	1	DFTPP2	GCMS0412	
27	Sample	2	CAL20A	GCMS0412	
28	Sample	26	7107	GCMS0412	GC/MS SCAN 3/26
29	Sample	27	7108	GCMS0412	GC/MS SCAN 3/26 FB
30	Sample	28	7109	GCMS0412	GC/MS SCAN 3/26
31	Sample	1	DFTPP3	GCMS0412	
32	Sample	2	CAL10	GCMS0412	
33	Sample	3	LBC	GCMS0412	gc/ms scan 4/1
34	Sample	4	REFB1	GCMS0412	gc/ms scan 4/1
35	Sample	5	REFB2	GCMS0412	gc/ms scan 4/1
36	Sample	6	7498	GCMS0412	gc/ms scan 4/1
37	Sample	7	7499	GCMS0412	gc/ms scan 4/1
38	Sample	8	7500	GCMS0412	gc/ms scan 4/1
39	Sample	9	7501	GCMS0412	gc/ms scan 4/1 fb
40	Sample	10	7502	GCMS0412	gc/ms scan 4/1
41	Sample	11	7503	GCMS0412	gc/ms scan 4/1
42	Sample	12	7504	GCMS0412	gc/ms scan 4/1
43	Sample	13	7505	GCMS0412	gc/ms scan 4/1 fb

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1802\DFTPP3.D
 Acq On : 19 Apr 2002 5:35 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

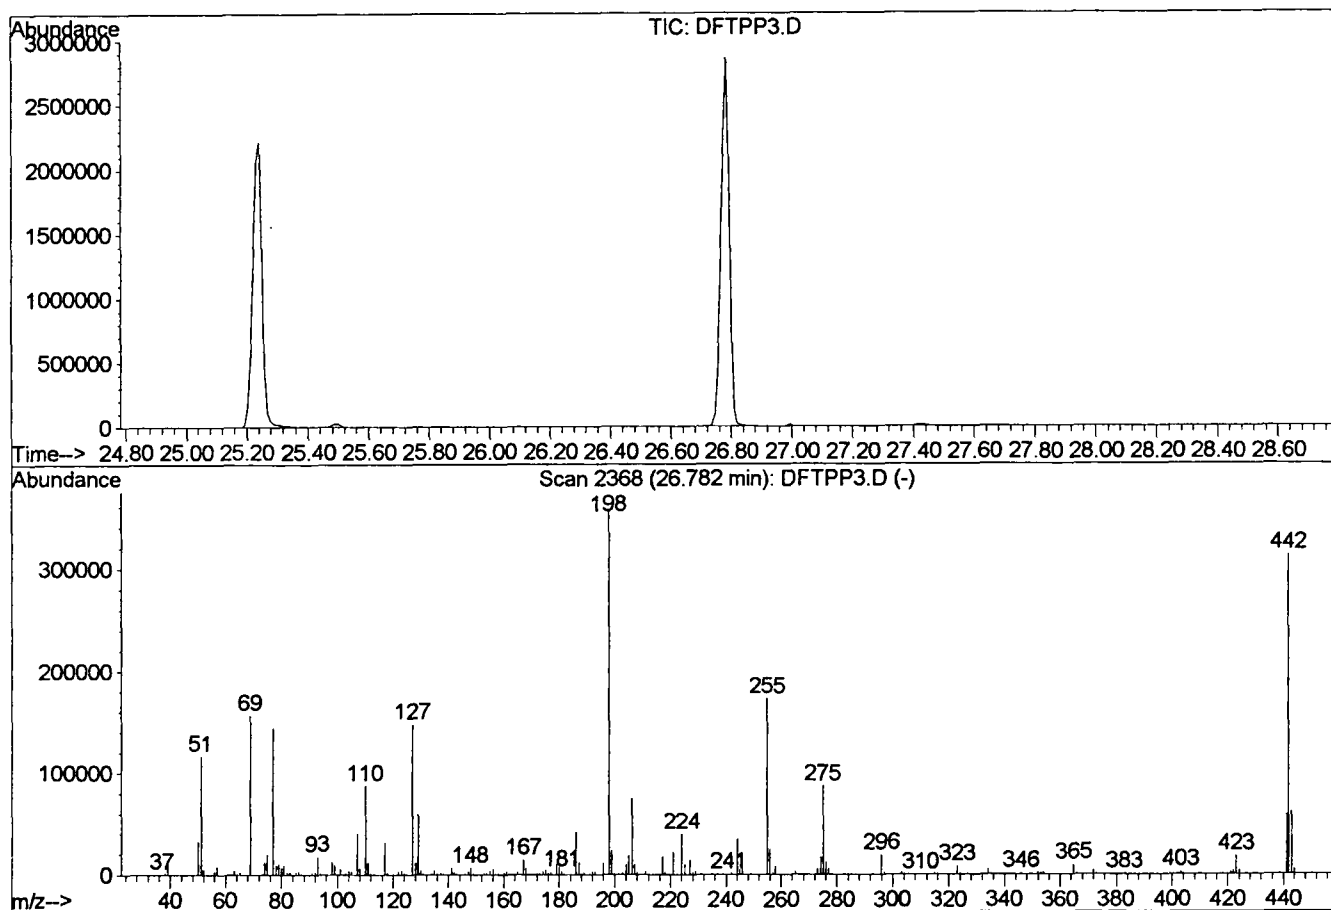

Spectrum Information: Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.8	117024	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.0	157120	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.5	148224	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	356864	PASS
199	198	5	9	6.5	23336	PASS
275	198	10	30	24.5	87312	PASS
365	198	1	100	2.7	9716	PASS
441	443	0.01	100	94.7	56936	PASS
442	198	40	110	87.6	312512	PASS
443	442	17	23	19.2	60104	PASS