

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 04/22/2002 Time: 11:58:20

Sample: AE07498
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 4/19/20 00:06 Ended: 4/19/20 00:06 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	MDL
1	n-Nitrosodimethylamine		< MDL	2.0
2	bis(2-Chloroethyl)ether		< MDL	2.0
3	1,3-Dichlorobenzene		< MDL	2.0
4	1,4-Dichlorobenzene		< MDL	2.0
5	1,2-Dichlorobenzene		< MDL	2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL	2.0
7	n-Nitrosodi-n-propylamine		< MDL	2.0
8	Hexachloroethane		< MDL	2.0
9	Nitrobenzene		< MDL	2.0
10	Isophorone		< MDL	2.0
11	bis(2-Chloroethoxy)methane		< MDL	2.0
12	1,2,4-Trichlorobenzene		< MDL	2.0
13	Naphthalene		< MDL	2.0
14	Hexachlorobutadiene		< MDL	2.0
15	2-Chloronaphthalene		< MDL	2.0
16	Dimethylphthalate		< MDL	2.0
17	2,6-Dinitrotoluene		< MDL	2.0
18	Acenaphthylene		< MDL	2.0
19	Acenaphthene		< MDL	2.0
20	2,4-Dinitrotoluene		< MDL	2.0
21	Diethylphthalate		< MDL	2.0
22	4-Chlorophenylphenylether		< MDL	2.0
23	Fluorene		< MDL	2.0
24	Azobenzene		< MDL	2.0
25	n-Nitrosodiphenylamine		< MDL	2.0
26	4-Bromophenylphenylether		< MDL	2.0
27	Hexachlorobenzene		< MDL	2.0
28	Phenanthrene		< MDL	2.0
29	Anthracene		< MDL	2.0
30	Di-n-butylphthalate		< MDL	2.0
31	Fluoranthene		< MDL	2.0
32	Pyrene		< MDL	2.0
33	Butylbenzylphthalate		< MDL	2.0
34	Benzo(a)anthracene		< MDL	2.0
35	bis(2-Ethylhexyl)phthalate		< MDL	2.0
36	Chrysene		< MDL	2.0
37	Di-n-octylphthalate		< MDL	2.0
38	Benzo(b)fluoranthene		< MDL	2.0
39	Benzo(k)fluoranthene		< MDL	2.0
40	Benzo(a)pyrene		< MDL	2.0
41	Indeno(1,2,3-cd)pyrene		< MDL	2.0
42	Dibenz(a,h)anthracene		< MDL	2.0
43	Benzo(g,h,i)perylene		< MDL	2.0

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1802\LBC.D
 Acq On : 19 Apr 2002 7:32 pm
 Sample : gc/ms scan 4/1
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 22 10:27 2002

Vial: 3
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0419.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Apr 19 14:51:24 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	414293	20.00	ug/l	-0.03
10) Naphthalene-d8	15.84	136	1513467	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.15	164	863129	20.00	ug/l	-0.02
30) Phenanthrene-d10	25.58	188	1272127	20.00	ug/l	-0.03
39) Chrysene-d12	33.64	240	842788	20.00	ug/l	-0.03
45) Perylene-d12	37.87	264	556277	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	23.29	209	34706	4.82	ug/L	-0.04
Spiked Amount	4.000		Recovery	=	120.50%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.90	128	443	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.63	149	427	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

LBC.D GCMS0419.M Mon Apr 22 10:28:36 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1802\LBC.D
 Acq On : 19 Apr 2002 7:32 pm
 Sample : gc/ms scan 4/1
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 22 10:27 2002

Vial: 3
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0419.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Apr 19 14:51:24 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.58	178	435	N.D.		
35) Anthracene	25.65	178	102	N.D.		
36) Di-n-butylphthalate	27.55	149	1147	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.64	228	2340	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.86	149	1028	N.D.		
44) Chrysene	33.71	228	560	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	36.70	252	281	N.D.		
48) Benzo(k)fluoranthene	36.76	252	314	N.D.		
49) Benzo(a)pyrene	37.88	252	2082	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration
 LBC.D GCMS0419.M Mon Apr 22 10:28:37 2002


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR1802\LBC.D
Acq On : 19 Apr 2002 7:32 pm
Sample : gc/ms scan 4/1
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 22 10:27 2002

Vial: 3
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0419.RES

Method : C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Apr 19 14:51:24 2002
Response via : Initial Calibration

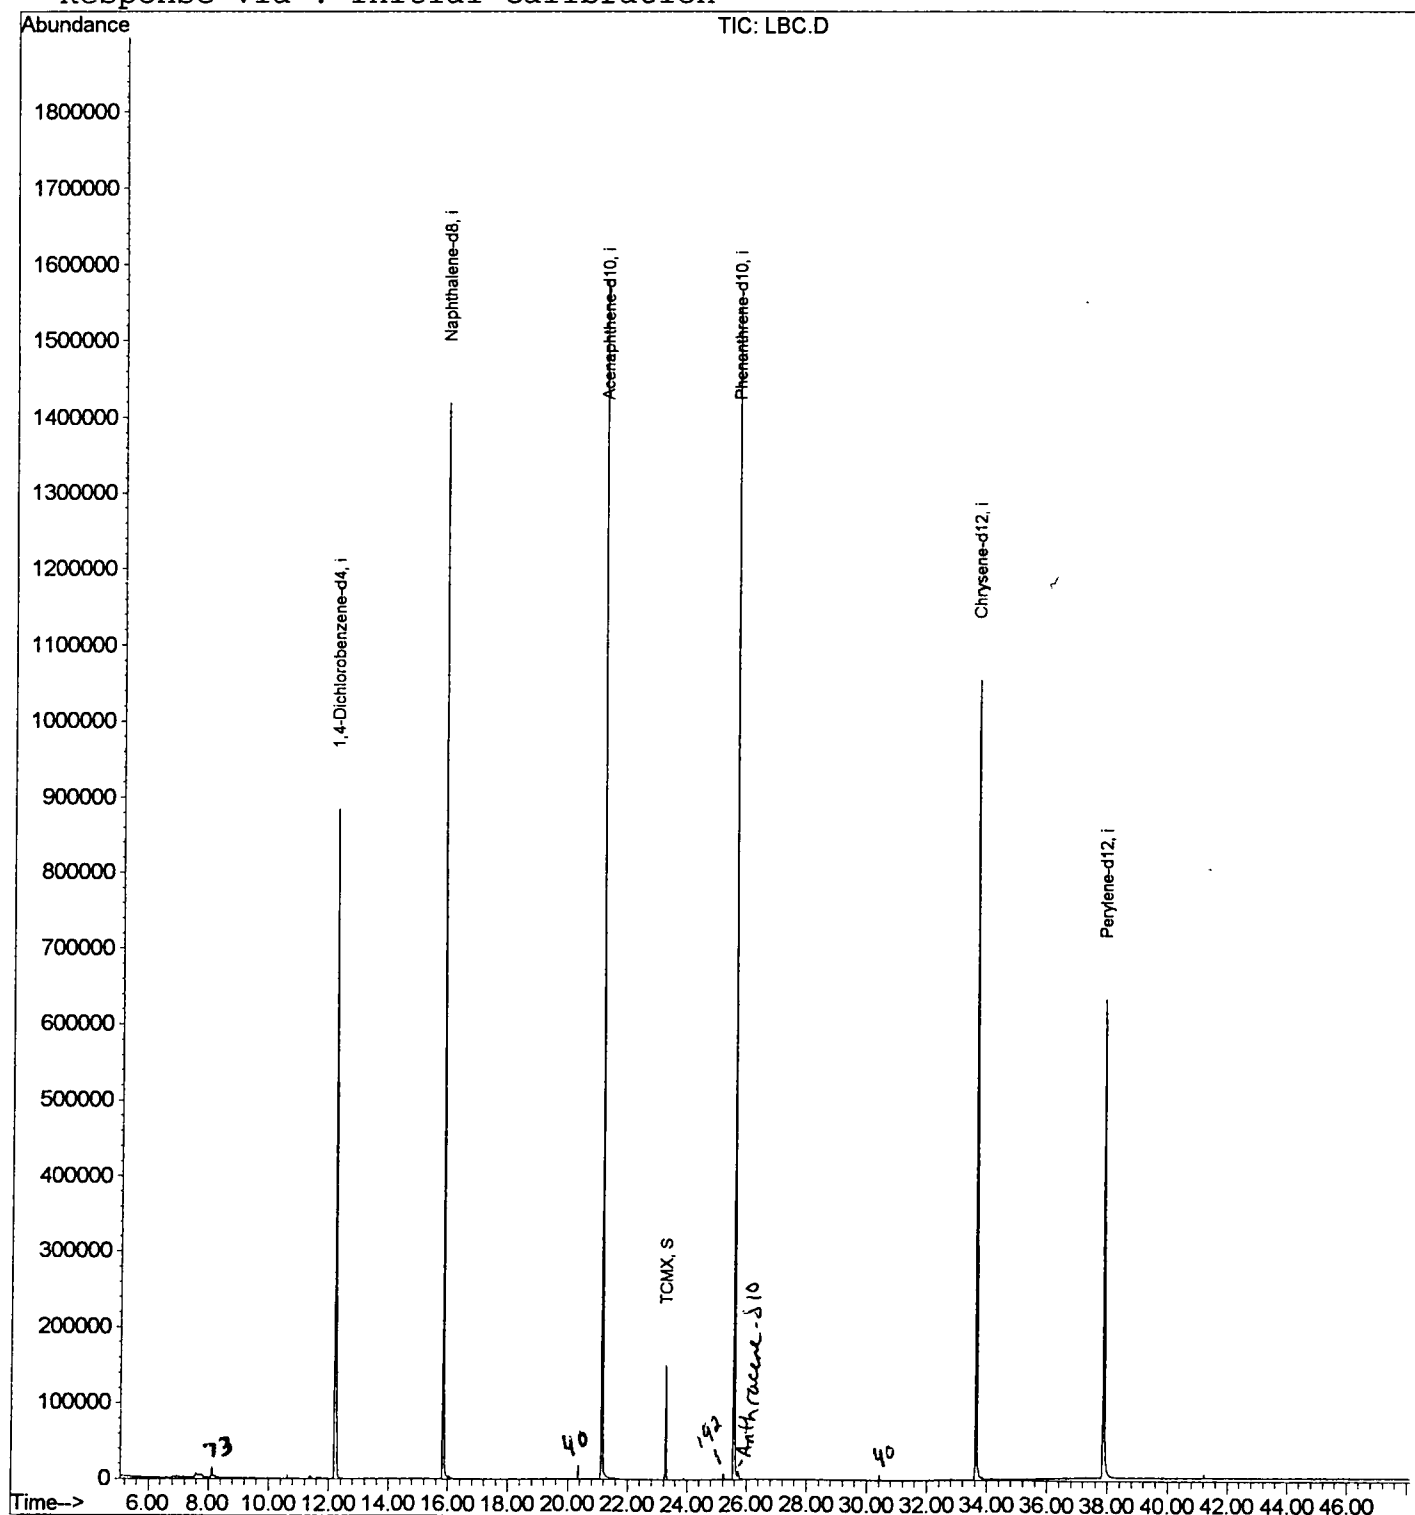

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR1802\LBC.D
 Acq On : 19 Apr 2002 7:32 pm
 Sample : gc/ms scan 4/1
 Misc :
 MS Integration Params: LSCINT.P

Vial: 3
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.209	775	780	797	rVB	883745	2209536	67.61%	13.720%
2	15.844	1170	1176	1193	rBV	1419208	2851572	87.26%	17.706%
3	21.150	1747	1754	1771	rBV	1580882	3268085	100.00%	20.292%
4	23.280	1979	1986	1994	rBV	150641	305355	9.34%	1.896%
5	25.584	2230	2237	2249	rBV2	1544935	3185744	97.48%	19.781%
6	33.645	3108	3115	3131	rBV2	1056294	2423000	74.14%	15.045%
7	37.868	3567	3575	3593	rBV2	630771	1861704	56.97%	11.560%

Sum of corrected areas: 16104996

LBC.D GCMS0419.M Mon Apr 22 10:44:33 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR1802\LBC.D
 Operator :
 Acquired : 19 Apr 2002 7:32 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: gc/ms scan 4/1
 Misc Info :
 Vial Number: 3
 Quant File :GCMS0419.RES (RTE Integrator)

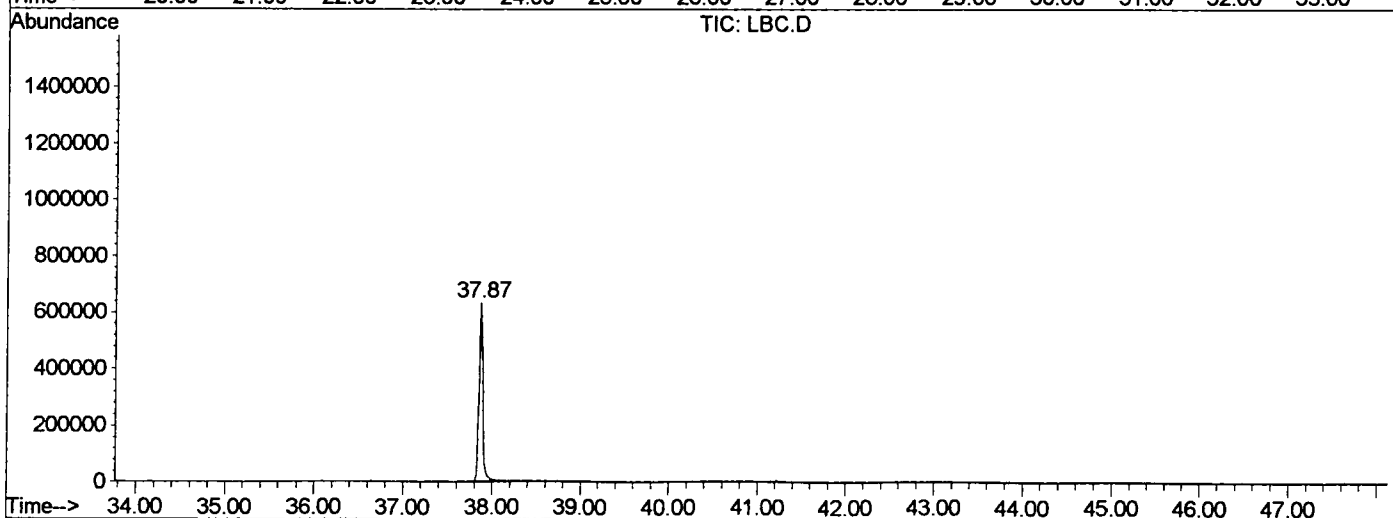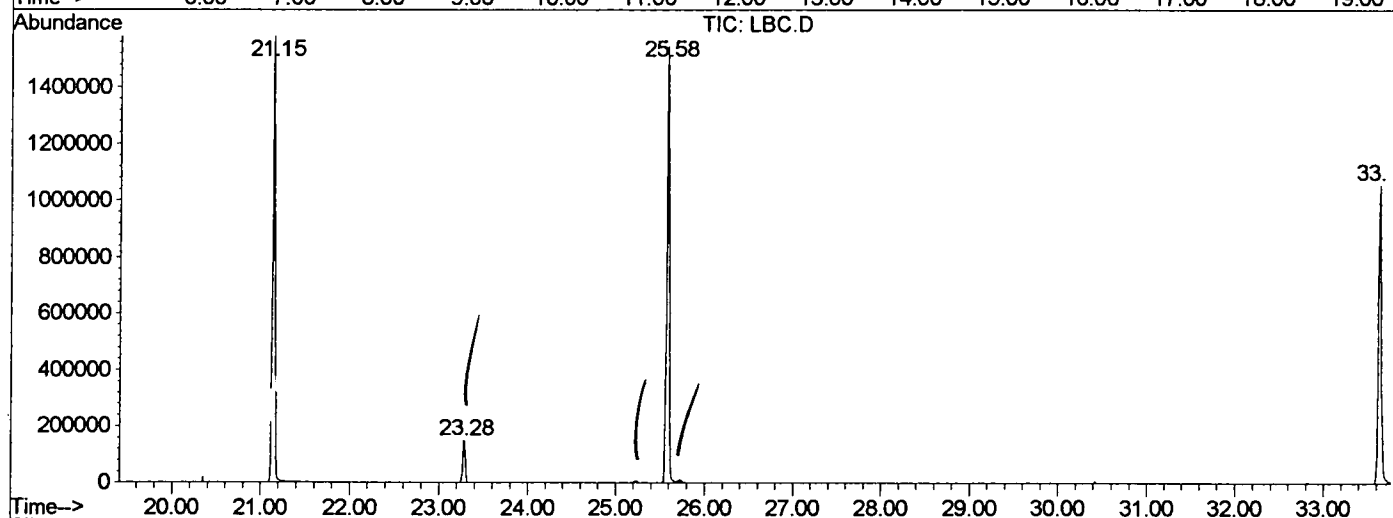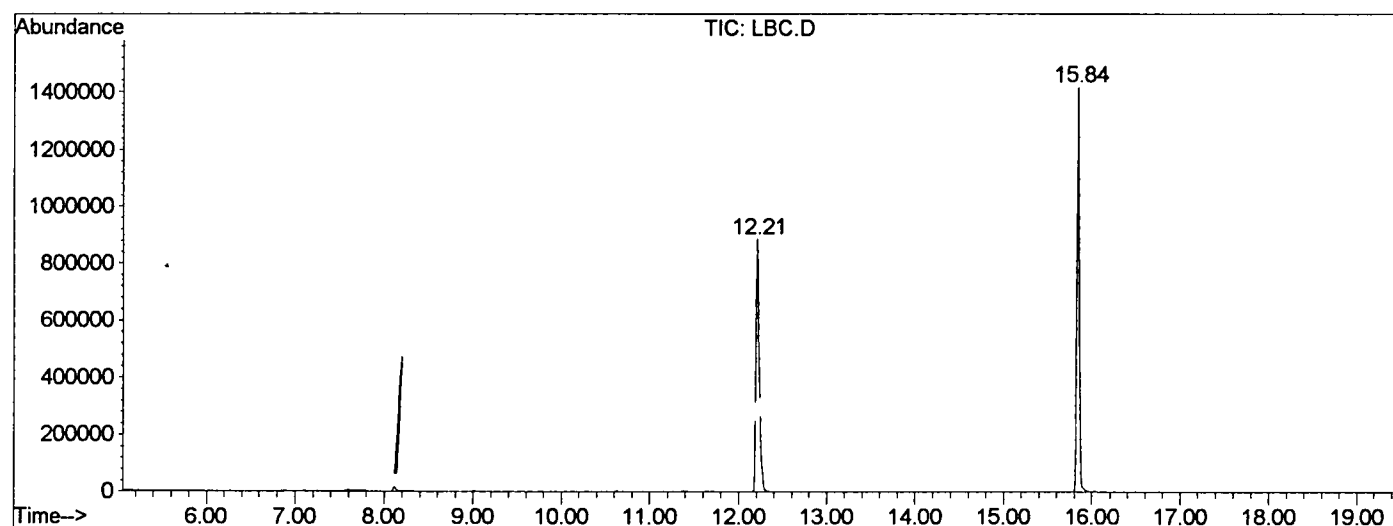

LBC.D GCMS0419.M Mon Apr 22 10:44:34 2002

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 19 Apr 2002 7:32 pm
 Data File: C:\HPCHEM\1\DATA\APR1802\LBC.D
 Name: gc/ms scan 4/1
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

LBC.D GCMS0419.M	Mon Apr 22	10:44:35	2002					