

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1802\DFTPP3.D

Vial: 1

Acq On : 19 Apr 2002 5:35 pm

Operator:

Sample :

Inst : 209


Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0419.M (RTE Integrator)

Title : 209 625/TCLP calibration table

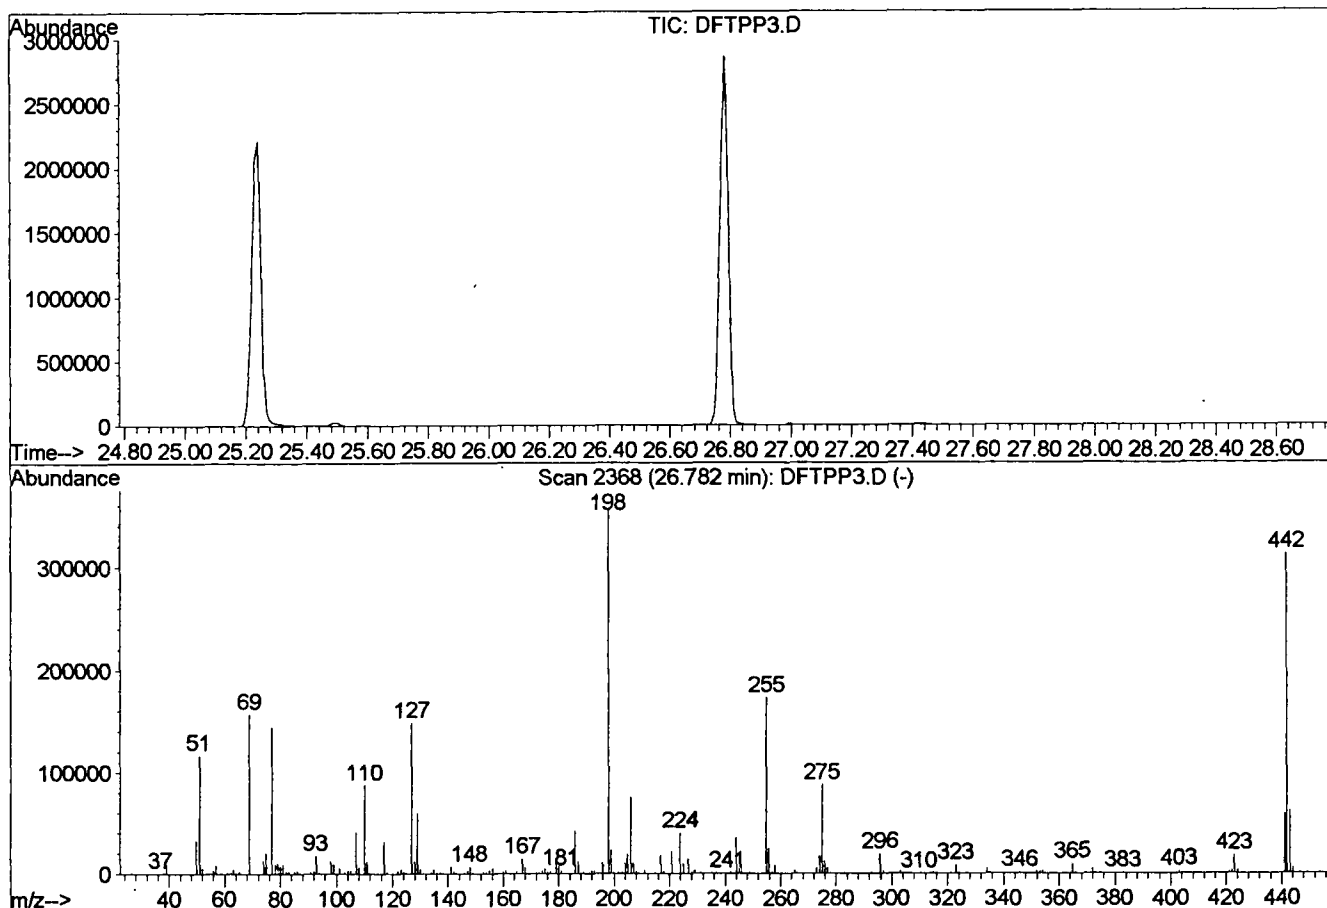

Spectrum Information: Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.8	117024	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.0	157120	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.5	148224	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	356864	PASS
199	198	5	9	6.5	23336	PASS
275	198	10	30	24.5	87312	PASS
365	198	1	100	2.7	9716	PASS
441	443	0.01	100	94.7	56936	PASS
442	198	40	110	87.6	312512	PASS
443	442	17	23	19.2	60104	PASS

DFTPP3.D GCMS0419.M

Mon Apr 22 12:08:27 2002