

Method 508 mod. Date Extracted 4-2-02

Page 39

\$GCMS-17892/p4/10/02

Ref

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ul		1ml			1ml	4B	7			
Ref.					1ml			6A				
Ref.					↓			2B				
7510								4A				
7511								2A				
7512								1A				
7513								4B				
7514								1B				
7515								1A				
7516								1B				
7517	FB							2A				
7518								2B				
7519								4A				
Remarks												
Reviewed by, <u>CB 8/14/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type <u>sep fun</u> Solv. lot# <u>X01E19/41470</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V46623</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>New Surrogate GCMS Scan</u>											
LPC												
ENDRN/DDT												

Analyst EAH

Verified by

Reviewed by DN

Date 4/11/02

Sequence Name: C:\MSDchem\1\sequence\020404.S
 Comment: GCMS scan
 Operator: Nefliu
 Data Path: C:\MSDchem\1\DATA\020404\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
☒ (X) Full Method ☒ (X) Inject Anyway
☐ () Reprocessing Only ☐ () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP1	508FAST	dftpp
2	Sample	2	0404C2	508SCAN1	ccv1
3	Sample	3	0402LB	508SCAN1	04/02 lab blk
4	Sample	4	0402REF1	508SCAN1	04/02 ref
5	Sample	5	0402REF2	508SCAN1	04/02 ref
6	Sample	6	07510	508SCAN1	sample
7	Sample	7	07511	508SCAN1	sample
8	Sample	8	07512	508SCAN1	sample
9	Sample	9	07513	508SCAN1	sample
10	Sample	10	07514	508SCAN1	sample
11	Sample	11	07515	508SCAN1	sample
12	Sample	12	07516	508SCAN1	sample
13	Sample	13	07517	508SCAN1	sample
14	Sample	14	07518	508SCAN1	sample
15	Sample	15	07519	508SCAN1	sample
16	Sample	16	0403LB	508SCAN1	04/03 lab blk
17	Sample	17	0403REF1	508SCAN1	04/03 ref
18	Sample	18	0403REF2	508SCAN1	04/03 ref
19	Sample	19	03257	508SCAN1	sample
20	Sample	20	07766	508SCAN1	sample
21	Sample	21	07767	508SCAN1	sample
22	Sample	22	07768	508SCAN1	sample
23	Sample	23	07769	508SCAN1	sample
24	Sample	24	07770	508SCAN1	sample
25	Sample	25	07771	508SCAN1	sample
26	Sample	26	07772	508SCAN1	sample
27	Sample	5	0402REF	508SCAN1	04/02ref

Method GC/MS Scan
Instrument 214

File Directory 020404

Storage Directory _____

Lab #	Filename	Description	Vial #		Inj. ul	Standards used - Lot #			Int. Std.	Remarks	Initials
			front	rear		Calibration	Reference	Surrogate			
	AFTPP1	offtop	1								MN
	040402	cal	2			2121 C/2196			2203d		
	040266	lab blk	3						2286K		
	040261	ref	4				2193.				
	040262	↓	5				↓				
	07570	sample	6								
	07571		7								
	07572		8								
	07573		9								
	07574		10								
	07575		11								
	07576		12								
	07577		13								
	07578		14								
	07579	↓	15								
	040368	lab blk	16								
	040369	ref	17				2193				
	040372	↓	18				↓				
	03257	sample	19								
	02266		20								
	02267		21								
	02268		22								
	02269		23								
	02270										
	02271										
	02272										
	040264	ref					2193				

Date 04/04/02

Extraction date 04/02, 05/02

Page 2

DFTPP

Data File : C:\MSDCHEM\1\DATA\020404\DFTPP1.D

Acq On : 4 Apr 2002 8:00 am

Sample : dftpp

Misc :

MS Integration Params: EVENTS.E

Method : C:\MSDCHEM\1\METHODS\SCANAPR0902.M (Chemstation Integrator)


Title : Method 508 GC/MS Scan

Vial: 1

Operator: Nefliu

Inst : Instrume

Multiplr: 1.00

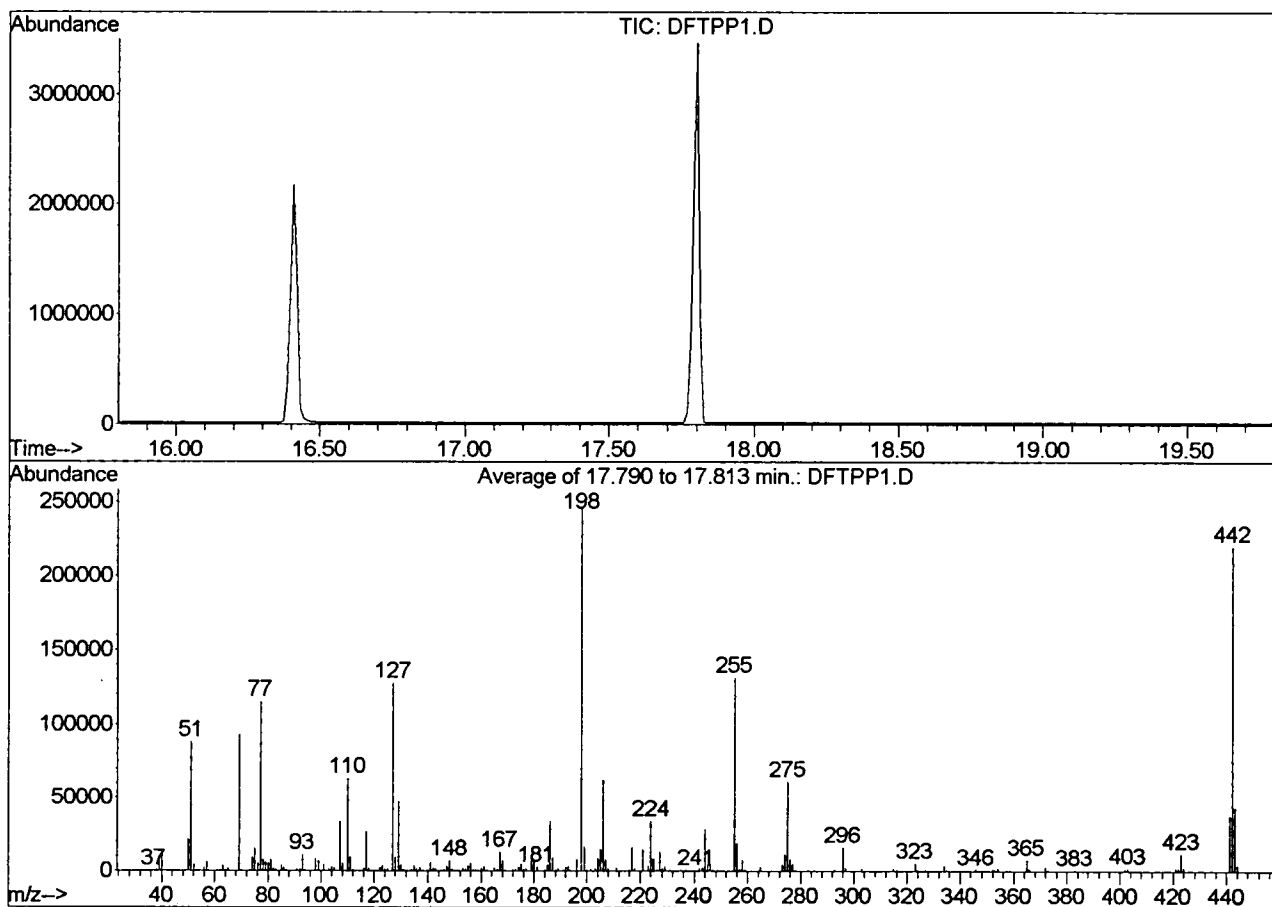

Spectrum Information: Average of 17.790 to 17.813 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.5	87752	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.8	93240	PASS
70	69	0.00	2	0.5	451	PASS
127	198	40	60	51.7	127568	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	246941	PASS
199	198	5	9	6.7	16510	PASS
275	198	10	30	24.5	60506	PASS
365	198	1	99	3.1	7546	PASS
441	443	1	100	87.6	37741	PASS
442	198	40	110	89.3	220432	PASS
443	442	17	23	19.6	43101	PASS