

Date _____

Sequence Name: C:\MSDchem\1\sequence\020415.S

Comment:

Operator: GALOS

Data Path: C:\MSDCHEM\1\DATA\MAR2102\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP1	508FAST	
2	Sample	2	0415C3	508SCAN	ccv
3	Sample	3	TCMX	508SCAN	tcmx
4	Sample	4	0404REF1	508SCAN	04/04 ref
5	Sample	5	0404REF2	508SCAN	04/04 ref
6	Sample	6	0405REF1	508SCAN	04/05 ref
7	Sample	7	0405REF2	508SCAN	04/05 ref
8	Sample	8	0404LB	508SCAN	04/04 lab blk
9	Sample	9	0405LB	508SCAN	04/05 lab blk
10	Sample	10	07631	508SCAN	sample
11	Sample	11	07632	508SCAN	sample
12	Sample	12	07972	508SCAN	sample
13	Sample	13	07973	508SCAN	sample
14	Sample	14	07974	508SCAN	sample
15	Sample	15	07975	508SCAN	sample
16	Sample	16	07976	508SCAN	sample
17	Sample	17	07977	508SCAN	sample
18	Sample	18	07978	508SCAN	sample
19	Sample	19	07979	508SCAN	sample
20	Sample	20	08063	508SCAN	sample
21	Sample	21	08064	508SCAN	sample
22	Sample	22	08065	508SCAN	sample
23	Sample	23	08066	508SCAN	sample
24	Sample	24	08067	508SCAN	sample
25	Sample	25	08068	508SCAN	sample
26	Sample	26	08069	508SCAN	sample
27	Sample	27	08070	508SCAN	sample
28	Sample	28	07766	508SCAN	sample

Method JOP & C19S scan
Instrument 215File Directory 020415

Storage Directory _____


Lab #	Filename	Description	Vial #		Inj.	Standards used - Lot #			Remarks	Initials
			front	rear		Calibration	Reference	Surrogate		
	077001		1		1					AN
	041503	can	2							
	TCMX	fermt	3							
	0404Ry1	by	4				2193			
	↓ 2		5				↓			
	0405Ry1		6							
	↓ 2		7				↓			
	0404LB	lab flk	8							
	0405LB		9							
	07831	sample	10							
	07832		11							
	07922		12							
	↓ 3		13							
	↓ 4		14							
	↓ 5		15							
	↓ 6		16							
	↓ 7		17							
	↓ 8		18							
	↓ 9		19							
	08063		20							
	↓ 4		21							
	↓ 5		22							
	↓ 6		23							
	↓ 7		24							
	↓ 8		25							
	08089		26							
	08020		27							
	02786		28							

Date 04/15/02Extraction date 04/04, 05/02Page 1

DFTPP

Data File : C:\MSDCHEM\1\DATA\020415\DFTPP1.D
Acq On : 15 Apr 2002 10:43 am
Sample :
Misc :
MS Integration Params: events.e
Method : C:\MSDCHEM\1\METHODS\041202SCAN.M (Chemstation Integrator)
Title : 508 Modified GC/MS scan

Vial: 1
Operator: Nefliu
Inst : Instrume
Multiplr: 1.00

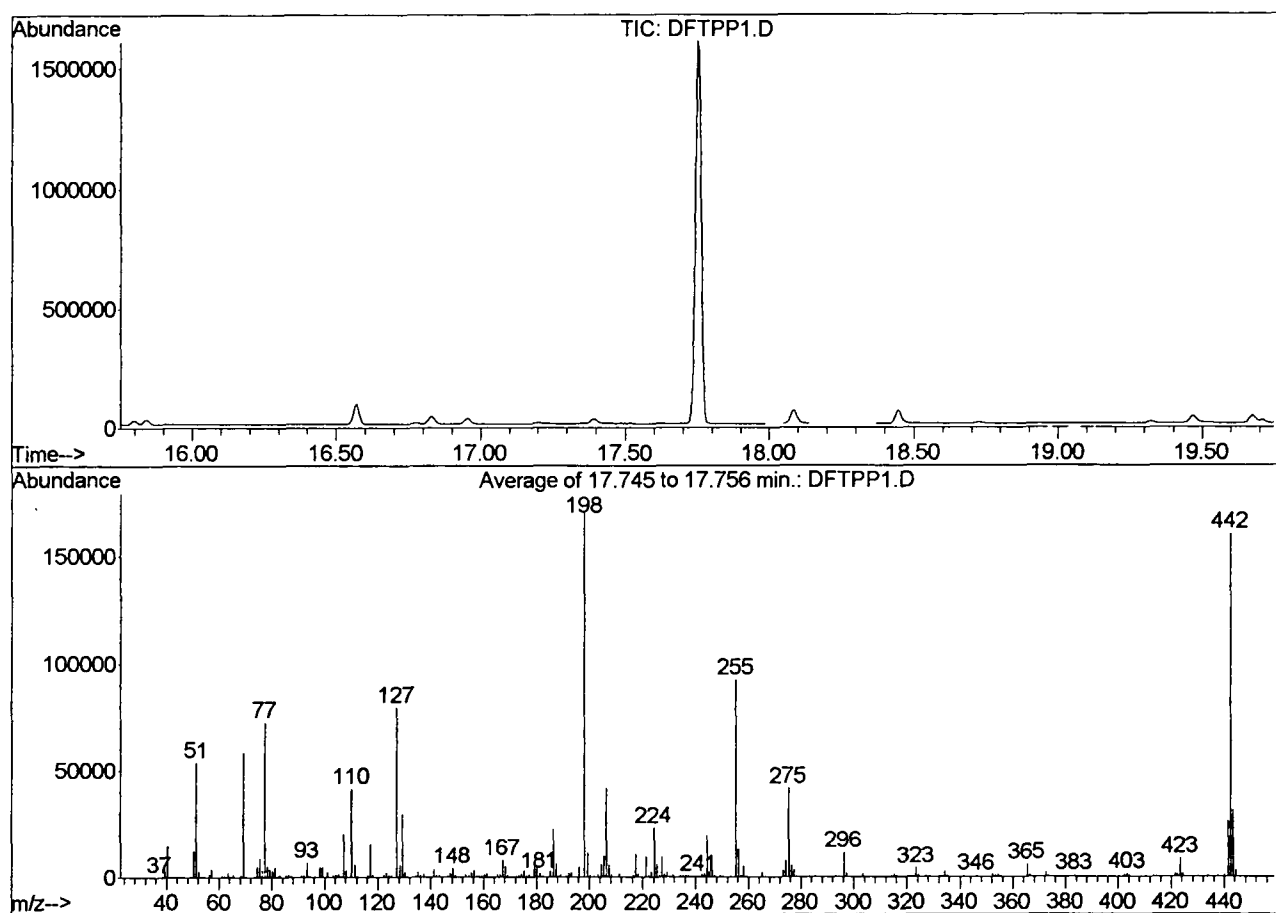

Spectrum Information: Average of 17.745 to 17.756 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	31.4	53720	PASS
68	69	0.00	2	1.4	822	PASS
69	198	0.00	100	34.1	58328	PASS
70	69	0.00	2	0.5	268	PASS
127	198	40	60	46.5	79440	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	170858	PASS
199	198	5	9	6.8	11595	PASS
275	198	10	30	24.3	41549	PASS
365	198	1	100	3.4	5765	PASS
441	443	0.01	100	83.6	26066	PASS
442	198	40	100	93.7	160074	PASS
443	442	17	23	19.5	31173	PASS

DFTPP1.D 041202SCAN.M

Mon Apr 15 11:19:36 2002