

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/24/2002 Time: 09:51:13

Sample: AE08018
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/24/02 09:45 Ended: 4/24/02 09:45 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Quant	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		93		10.0

Comments for Sample AE08018 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-24-2002 Time: 09:51:42

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1102\8018.D
 Acq On : 12 Apr 2002 1:00 pm
 Sample : gc/ms scan 4/4
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 16 12:02 2002

Vial: 24
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Apr 16 11:47:07 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0408

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.23	152	316042	20.00	ug/l	0.00
10) Naphthalene-d8	15.86	136	1155156	20.00	ug/l	-0.02
17) Acenaphthene-d10	21.17	164	643901	20.00	ug/l	0.00
30) Phenanthrene-d10	25.61	188	894489	20.00	ug/l	0.00
39) Chrysene-d12	33.66	240	515225	20.00	ug/l	-0.02
45) Perylene-d12	37.89	264	318210	20.00	ug/l	-0.03

System Monitoring Compounds

28) TCMX	23.30	209	32156	9.28	ug/L	-0.03
Spiked Amount	10.000		Recovery	=	92.80%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	14.57	82	281	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.92	128	227	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	20.52	163	104	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.64	149	972	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

8018.D GCMS0412.M Tue Apr 16 12:03:04 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1102\8018.D Vial: 24
 Acq On : 12 Apr 2002 1:00 pm Operator:
 Sample : gc/ms scan 4/4 Inst : 209
 Misc : Multiplr: 1.00
 MS Integration Params: GOOFY.P
 Quant Time: Apr 16 12:02 2002 Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Apr 16 11:47:07 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0408

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.66	178	382	N.D.	
35) Anthracene	25.66	178	382	N.D.	
36) Di-n-butylphthalate	27.57	149	49097	1.70 ug/l	99
37) Fluoranthene	29.29	202	616	N.D.	
40) Pyrene	29.98	202	673	N.D.	
41) Butylbenzylphthalate	32.11	149	503	N.D.	
42) Benzo(a)anthracene	33.66	228	1288	N.D.	
43) Bis(2-ethylhexyl)phthalate	33.87	149	2022	N.D.	
44) Chrysene	33.73	228	384	N.D.	
46) Di-n-Octylphthalate	35.64	149	405	N.D.	
47) Benzo(b)fluoranthene	36.71	252	291	N.D.	
48) Benzo(k)fluoranthene	36.78	252	313	N.D.	
49) Benzo(a)pyrene	37.90	252	1254	N.D.	
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.	


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR1102\8018.D
Acq On : 12 Apr 2002 1:00 pm
Sample : gc/ms scan 4/4
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 16 12:02 2002

Vial: 24
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue Apr 16 11:47:07 2002
Response via : Initial Calibration

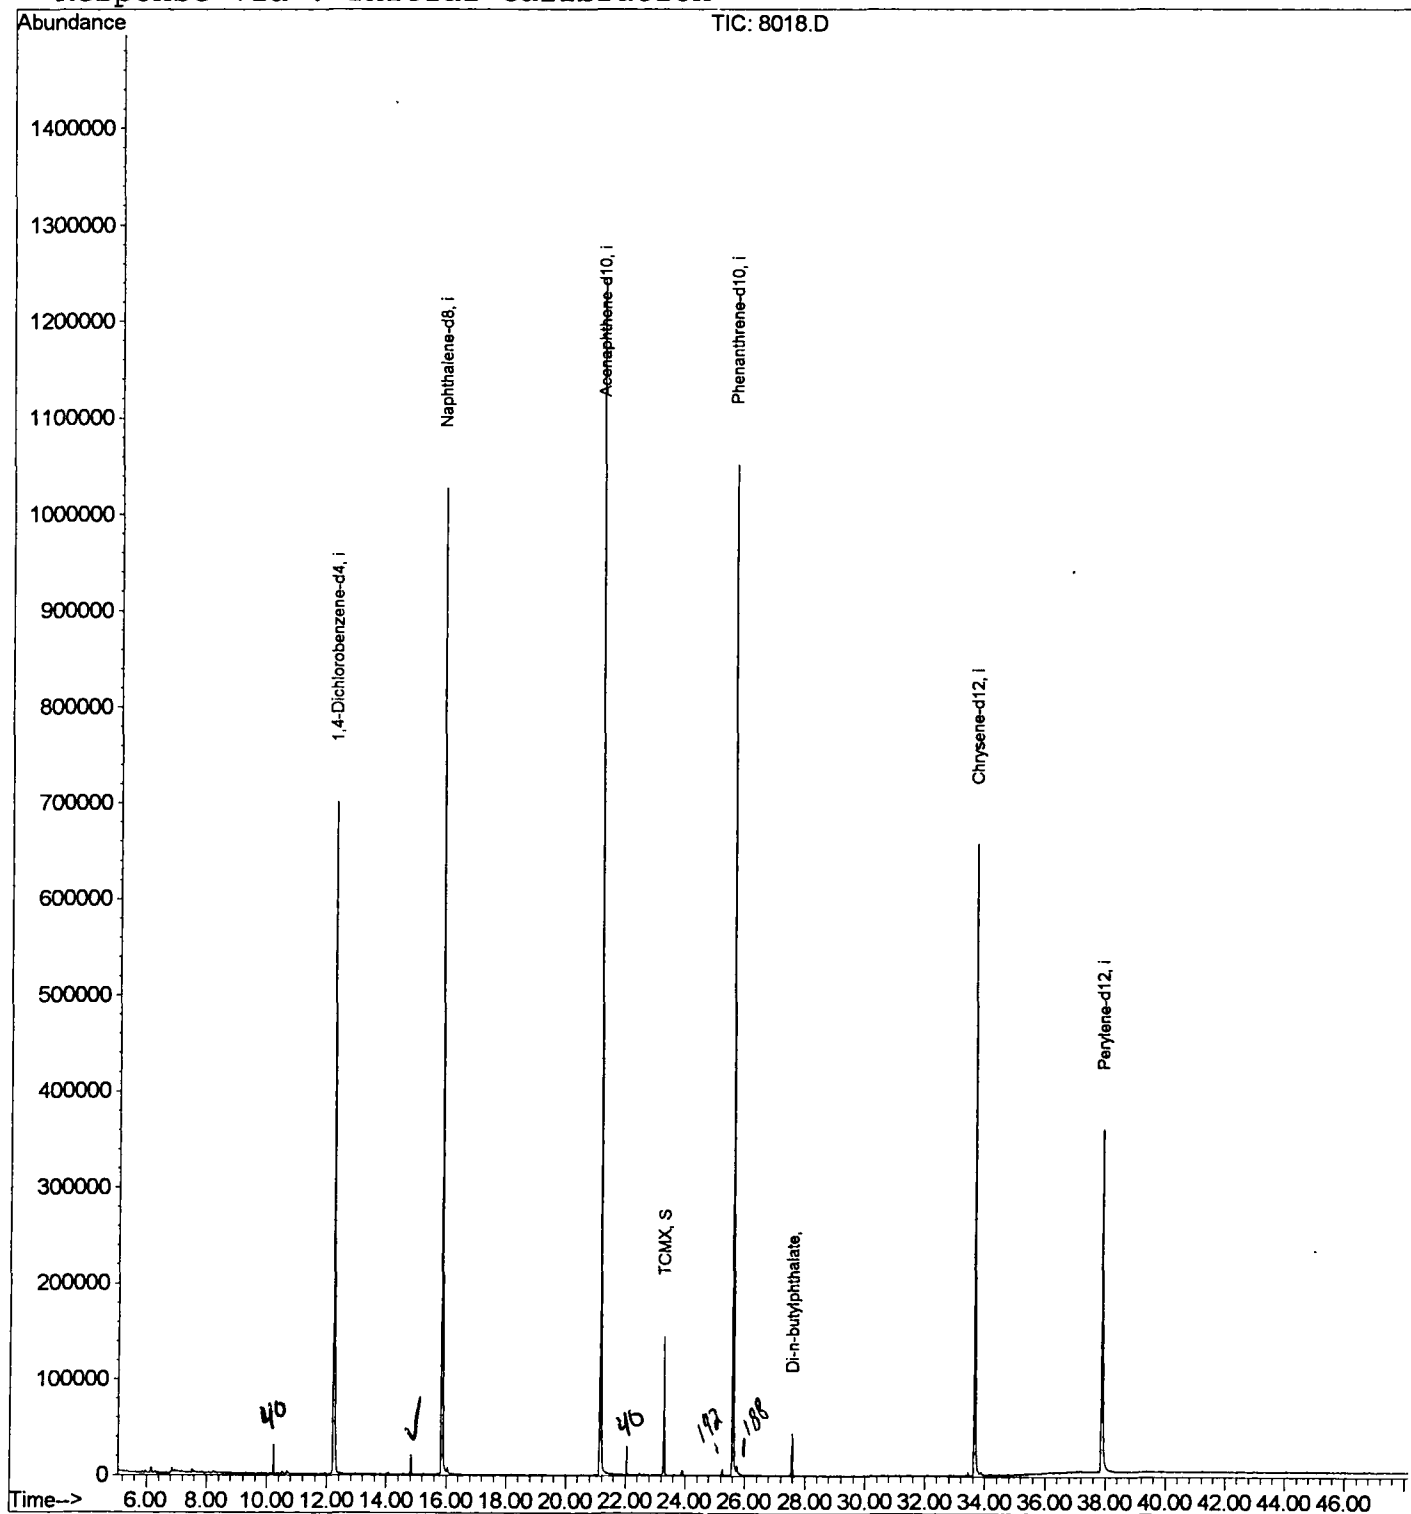

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR1102\8018.D
 Acq On : 12 Apr 2002 1:00 pm
 Sample : gc/ms scan 4/4
 Misc :
 MS Integration Params: LSCINT.P

Vial: 24
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.224	777	782	799	rVB	699080	1719719	69.25%	14.668%
2	14.831	1061	1066	1071	rVB2	19975	39620	1.60%	0.338%
3	15.859	1172	1178	1192	rBV	1026258	2196706	88.46%	18.737%
4	21.165	1750	1756	1769	rBV	1245437	2483379	100.00%	21.182%
5	23.304	1982	1989	1995	rBV	144897	290677	11.70%	2.479%
6	25.608	2233	2240	2252	rBV2	1051131	2298220	92.54%	19.602%
7	27.573	2447	2454	2461	rBV	43960	81080	3.26%	0.692%
8	33.660	3110	3117	3134	rBV2	656904	1520320	61.22%	12.967%
9	37.892	3570	3578	3599	rBV2	355776	1094402	44.07%	9.335%

Sum of corrected areas: 11724123

8018.D GCMS0412.M Tue Apr 16 12:08:33 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR1102\8018.D
Operator :
Acquired : 12 Apr 2002 1:00 pm using AcqMethod GCMS0408
Instrument : 209
Sample Name: gc/ms scan 4/4
Misc Info :
Vial Number: 24
Quant File :GCMS0412.RES (RTE Integrator)

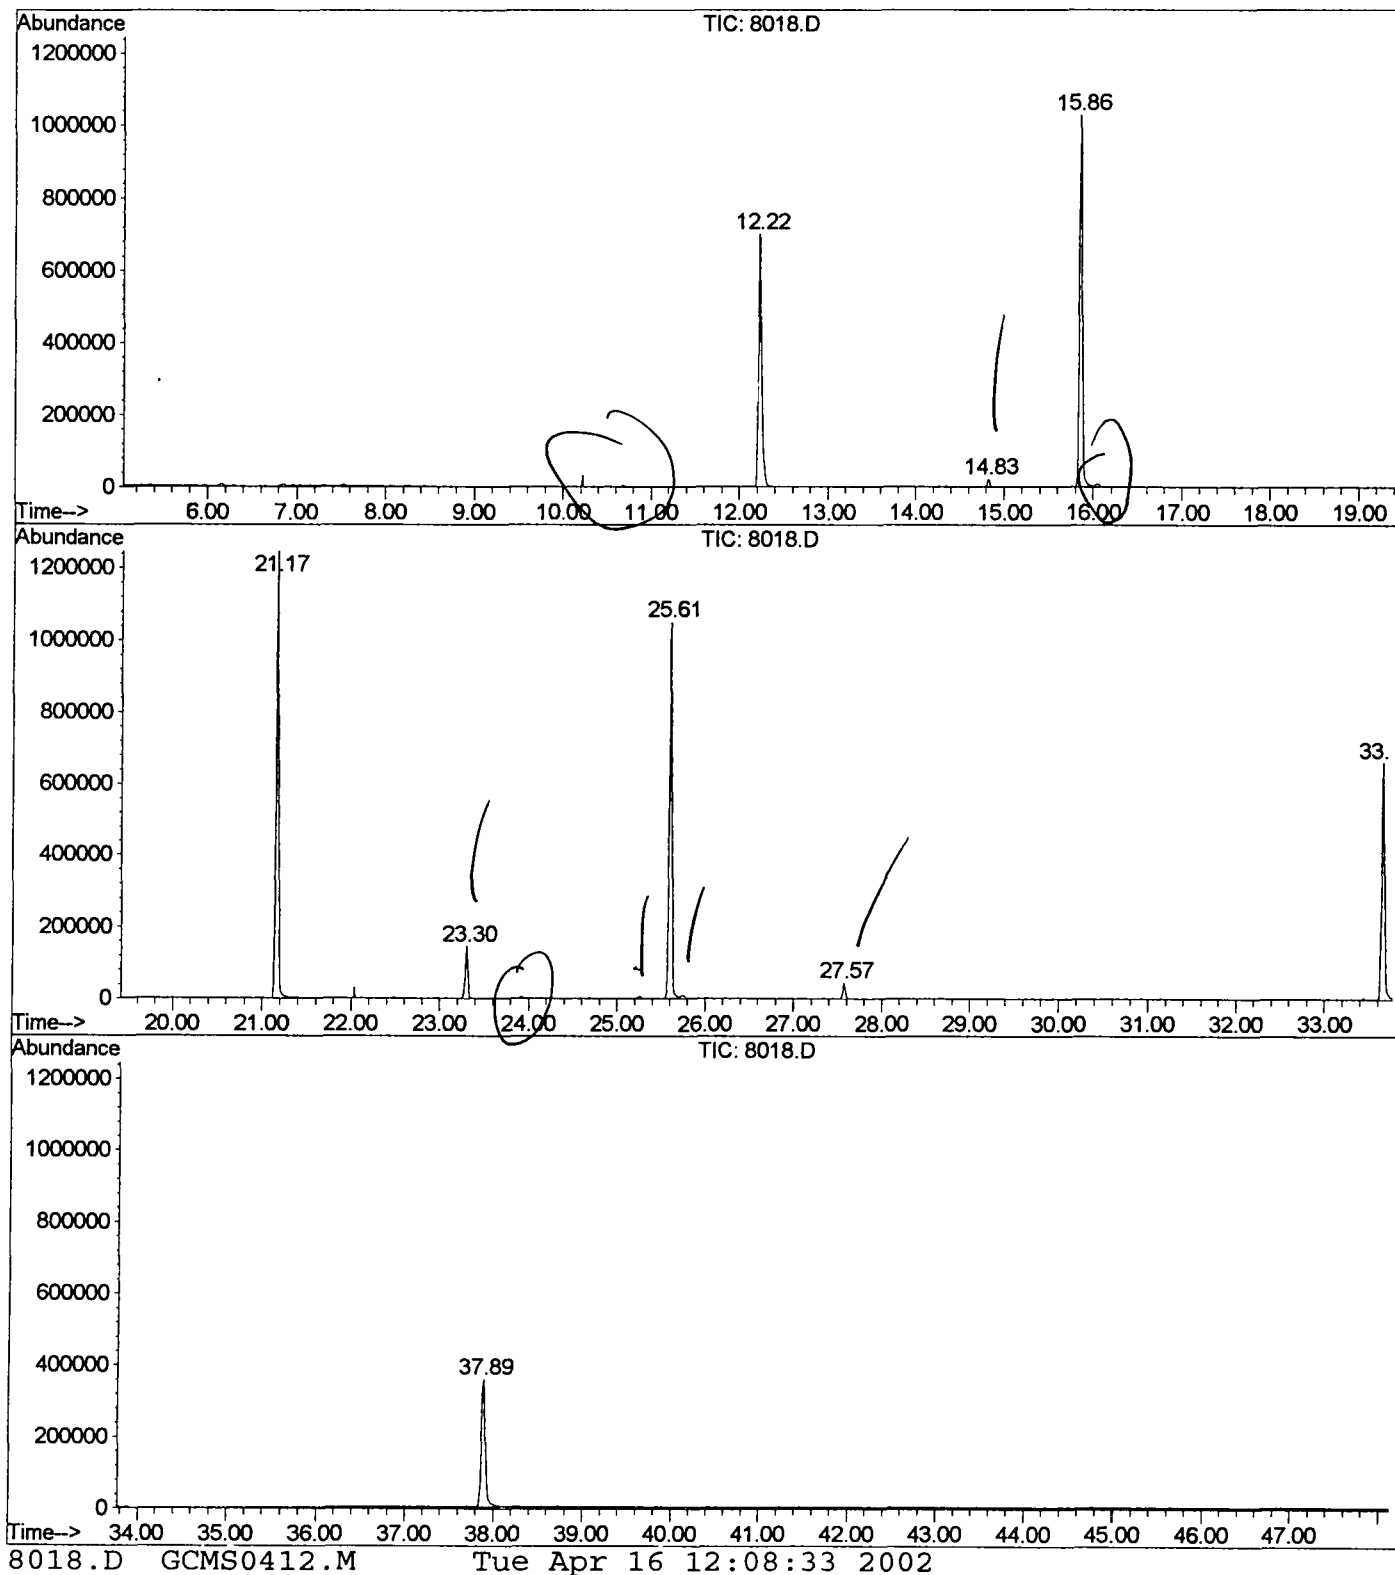

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR1102\8018.D
 Acq On : 12 Apr 2002 1:00 pm
 Sample : gc/ms scan 4/4
 Misc :
 MS Integration Params: LSCINT.P


Vial: 24
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Cyclopentasiloxane, decamethyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.83	0.36 ug/l	39620	Naphthalene-d8	15.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
2			N-(Trifluoroacetyl)-O,O',O''-tris(tri	495	C20H36F3NO4Si3	000000-00-0	43
3			N-(Trifluoroacetyl)-N,O,O',O''-tetr	553	C22H42F3NO4Si4	000000-00-0	43
4			Phenethylamine, N-methyl-.beta.,3,4	399	C18H37NO3Si3	010538-85-9	37

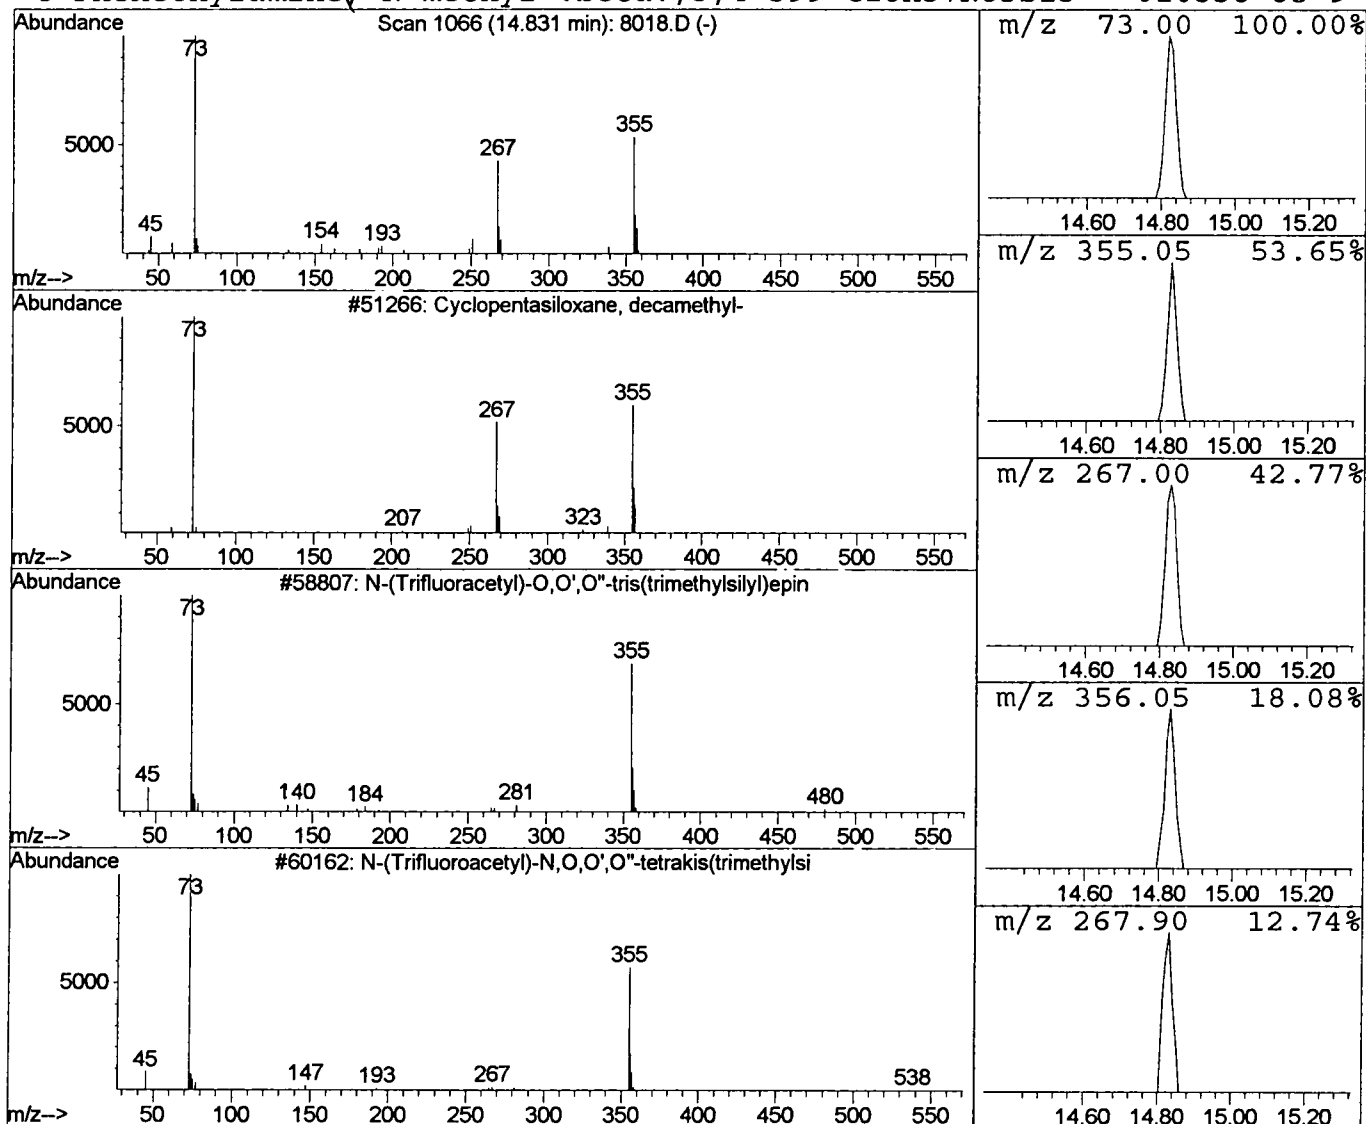

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 12 Apr 2002 1:00 pm
Data File: C:\HPCHEM\1\DATA\APR1102\8018.D
Name: gc/ms scan 4/4
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Cyclopentasiloxane,	14.83	0.4	ug/l	39620	ISTD02	15.86	2196710	20.0

8018.D GCMS0412.M Tue Apr 16 12:08:35 2002