

Method 508mod

Date Extracted 4-8-02

Page 49

Ref

#GCMs-18065

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Sys add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ml		1ml	1ml		1ml	4B	7			
Rep								10B				
Rep								4A				
57492								10A				
8209	see 4/19							1A				
8210								1B				
8211								2A				
8212								2B				
8213								2A				
8214								1A				
8215								4B				
8216	FB							1A				
Remarks												
Reviewed by, <u>CB 8/15/12</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type <u>SEP FM</u> Solv. lot# <u>41470</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V47590</u>												
STANDARD INT STD LOG#												
CALIBRATION <u>HP04100</u>												
SPRINKLE <u>2193</u>												
QC/MDF												
CHECK												
STD. <u>0410802</u>												
NOGATE <u>New Surrogate</u>												
QC												
QC/DO												

EH
4/12/01

Verified by My

Reviewed by DP
Date 4/12/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\APR1702.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\apr1702\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0412	
2	Sample	2	CAL20	GCMS0412	
3	Sample	3	LB	GCMS0412	gc/ms scan 3/19
4	Sample	4	REF1	GCMS0412	gc/ms scan 3/19
5	Sample	5	REF2	GCMS0412	gc/ms scan 3/19
6	Sample	6	6430	GCMS0412	gc/ms scan 3/19 fb
7	Sample	7	6449	GCMS0412	gc/ms scan 3/19
8	Sample	8	6450	GCMS0412	gc/ms scan 3/19
9	Sample	9	6451	GCMS0412	gc/ms scan 3/19
10	Sample	10	6452	GCMS0412	gc/ms scan 3/19
11	Sample	11	6453	GCMS0412	gc/ms scan 3/19
12	Sample	12	6454	GCMS0412	gc/ms scan 3/19
13	Sample	13	6455	GCMS0412	gc/ms scan 3/19
14	Sample	14	6456	GCMS0412	gc/ms scan 3/19 fb
15	Sample	15	6457	GCMS0412	gc/ms scan 3/19
16	Sample	16	LBA	GCMS0412	gc/ms scan 4/8
17	Sample	17	REFA1	GCMS0412	gc/ms scan 4/8
18	Sample	18	REFA2	GCMS0412	gc/ms scan 4/8
19	Sample	19	5749	GCMS0412	gc/ms scan 4/8
20	Sample	20	8209	GCMS0412	gc/ms scan 4/8
21	Sample	21	8210	GCMS0412	gc/ms scan 4/8
22	Sample	22	8211	GCMS0412	gc/ms scan 4/8
23	Sample	23	8212	GCMS0412	gc/ms scan 4/8
24	Sample	24	8213	GCMS0412	gc/ms scan 4/8
25	Sample	25	8214	GCMS0412	gc/ms scan 4/8
26	Sample	26	8215	GCMS0412	gc/ms scan 4/8
27	Sample	27	8216	GCMS0412	gc/ms scan 4/8 fb
28	Sample	3	SURR	GCMS0412	

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1702\DFTPP.D

Vial: 1

Acq On : 17 Apr 2002 8:12 am

Operator:

Sample :

Inst : 209


Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

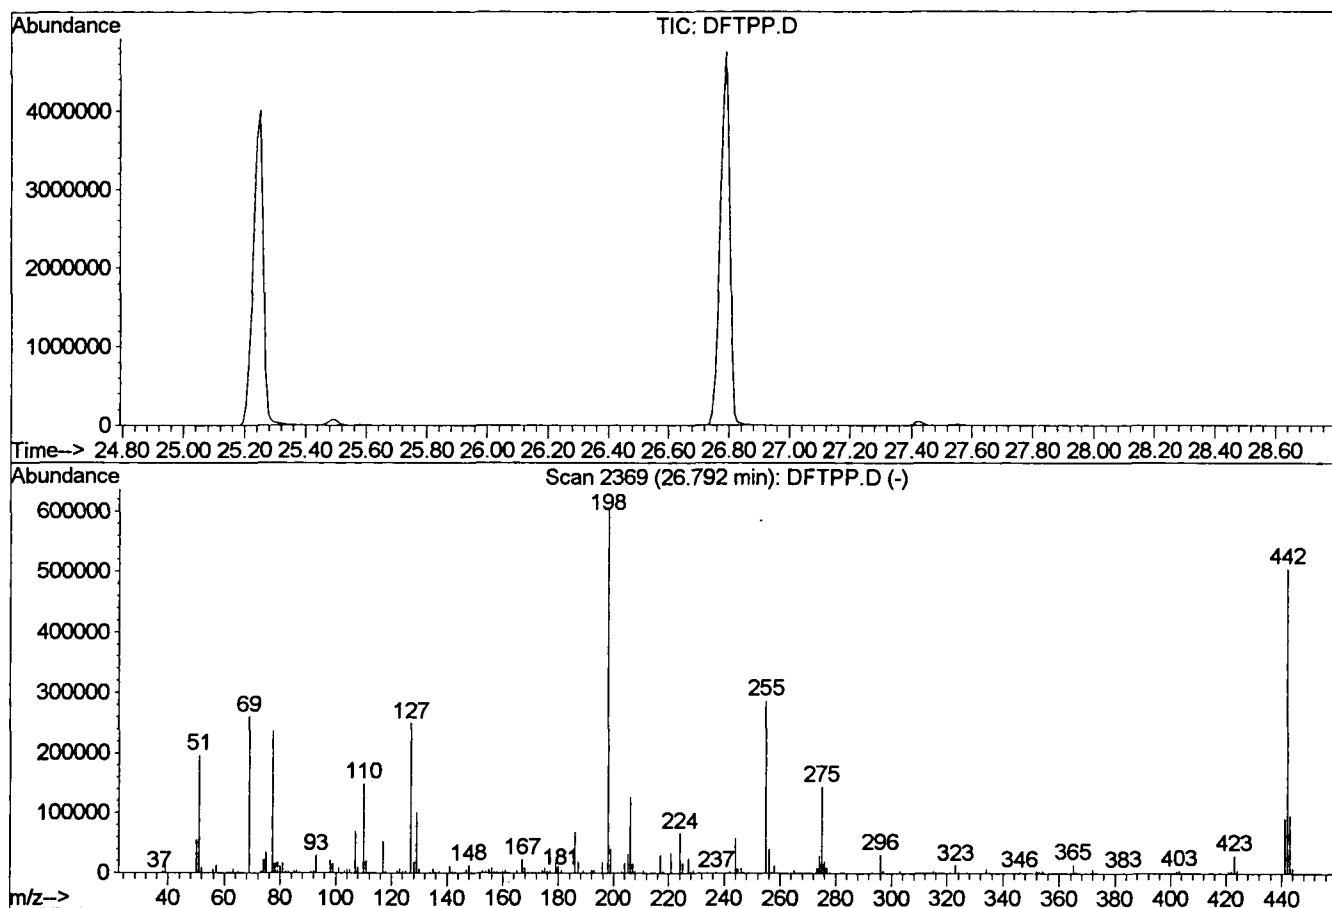

Spectrum Information: Scan 2369

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.5	196608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.0	260672	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.3	249856	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	605564	PASS
199	198	5	9	6.6	40208	PASS
275	198	10	30	24.0	145472	PASS
365	198	1	100	2.5	15138	PASS
441	443	0.01	100	95.3	92704	PASS
442	198	40	110	83.5	505505	PASS
443	442	17	23	19.2	97296	PASS

DFTPP.D GCMS0412.M

Thu Apr 18 12:47:45 2002