


DFTPP

Data File : C:\HPCHEM\1\DATA\APR1202\DFTPP.D
 Acq On : 15 Apr 2002 8:05 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

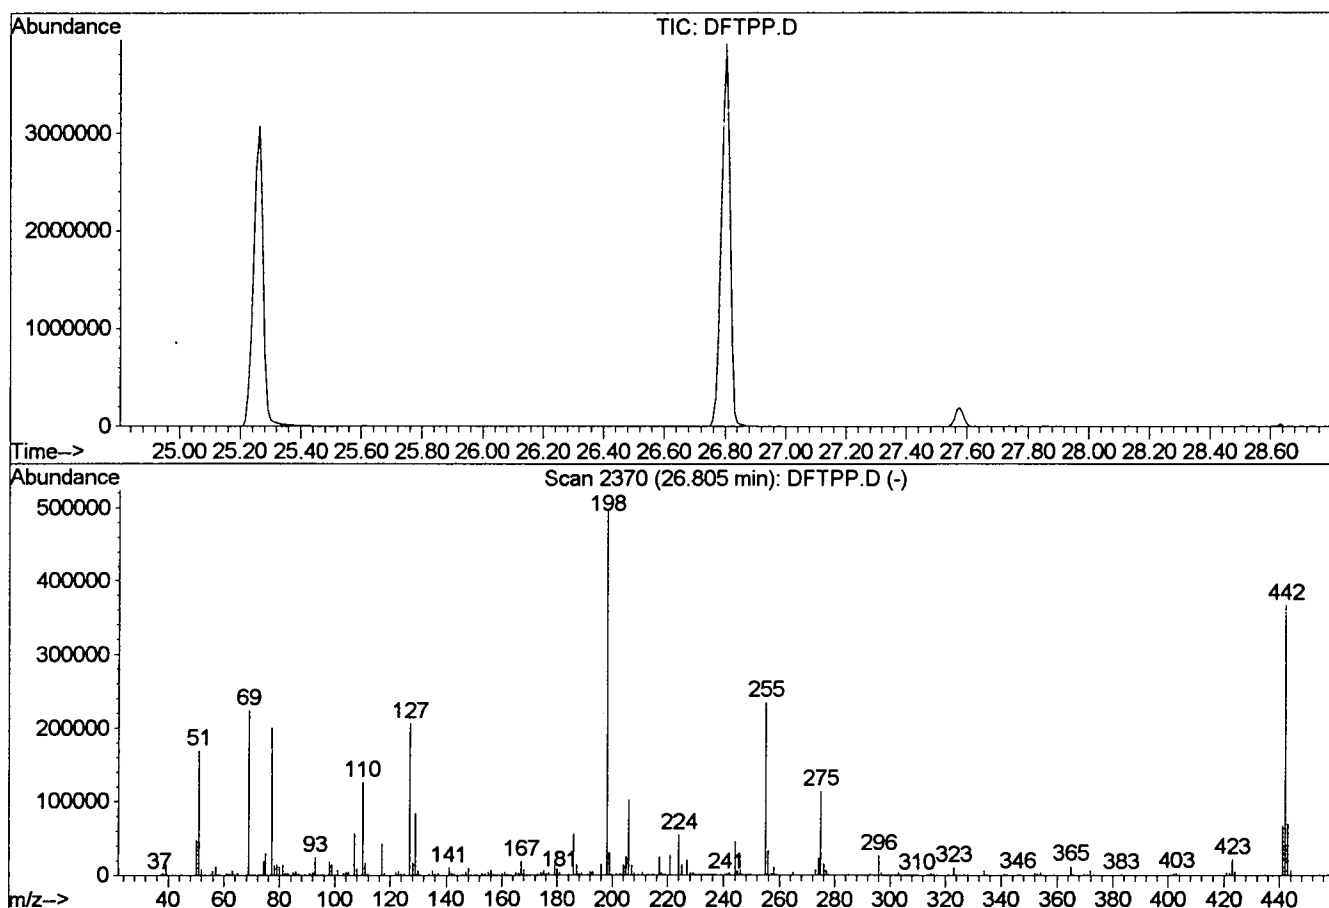

Spectrum Information: Scan 2370

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.0	169649	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.0	224154	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.6	207354	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	498298	PASS
199	198	5	9	6.5	32280	PASS
275	198	10	30	23.3	116016	PASS
365	198	1	100	2.5	12338	PASS
441	443	0.01	100	96.1	68032	PASS
442	198	40	110	73.9	368167	PASS
443	442	17	23	19.2	70812	PASS