

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/23/2002 Time: 14:03:48

Sample: AE06429
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/23/02 14:02 Ended: 4/23/02 14:02 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		84		10.0

Comments for Sample AE06429 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-23-2002 Time: 14:04:25

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1202\6429.D
 Acq On : 15 Apr 2002 6:51 pm
 Sample : re-extract
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 16 15:24 2002

Vial: 12
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Apr 16 14:55:12 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

re-analysis

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.23	152	479080	20.00	ug/l	-0.01
10) Naphthalene-d8	15.86	136	1771561	20.00	ug/l	-0.01
17) Acenaphthene-d10	21.17	164	1015084	20.00	ug/l	0.00
30) Phenanthrene-d10	25.61	188	1475214	20.00	ug/l	0.00
39) Chrysene-d12	33.66	240	920857	20.00	ug/l	-0.01
45) Perylene-d12	37.90	264	601105	20.00	ug/l	-0.01

System Monitoring Compounds

28) TCMX	23.31	209	42667	8.39	ug/L	-0.02
Spiked Amount	10.000		Recovery	=	83.90%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	21.42	165	394	N.D.	
25) Diethylphthalate	22.65	149	958	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

6429.D GCMS0412.M Tue Apr 16 15:25:05 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1202\6429.D

Vial: 12

Acq On : 15 Apr 2002 6:51 pm

Operator:

Sample : re-extract

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 16 15:24 2002

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue Apr 16 14:55:12 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.67	178	400	N.D.		
35) Anthracene	25.67	178	400	N.D.		
36) Di-n-butylphthalate	27.58	149	5131	N.D.		
37) Fluoranthene	29.30	202	446	N.D.		
40) Pyrene	29.99	202	413	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.66	228	2358	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.88	149	2751	N.D.		
44) Chrysene	33.66	228	2358	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	0.00	252	0	N.D.		
48) Benzo(k)fluoranthene	0.00	252	0	N.D.		
49) Benzo(a)pyrene	37.90	252	2172	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

6429.D GCMS0412.M

Tue Apr 16 15:25:06 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR1202\6429.D
Acq On : 15 Apr 2002 6:51 pm
Sample : re-extract
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 16 15:24 2002

Vial: 12
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue Apr 16 14:55:12 2002
Response via : Initial Calibration

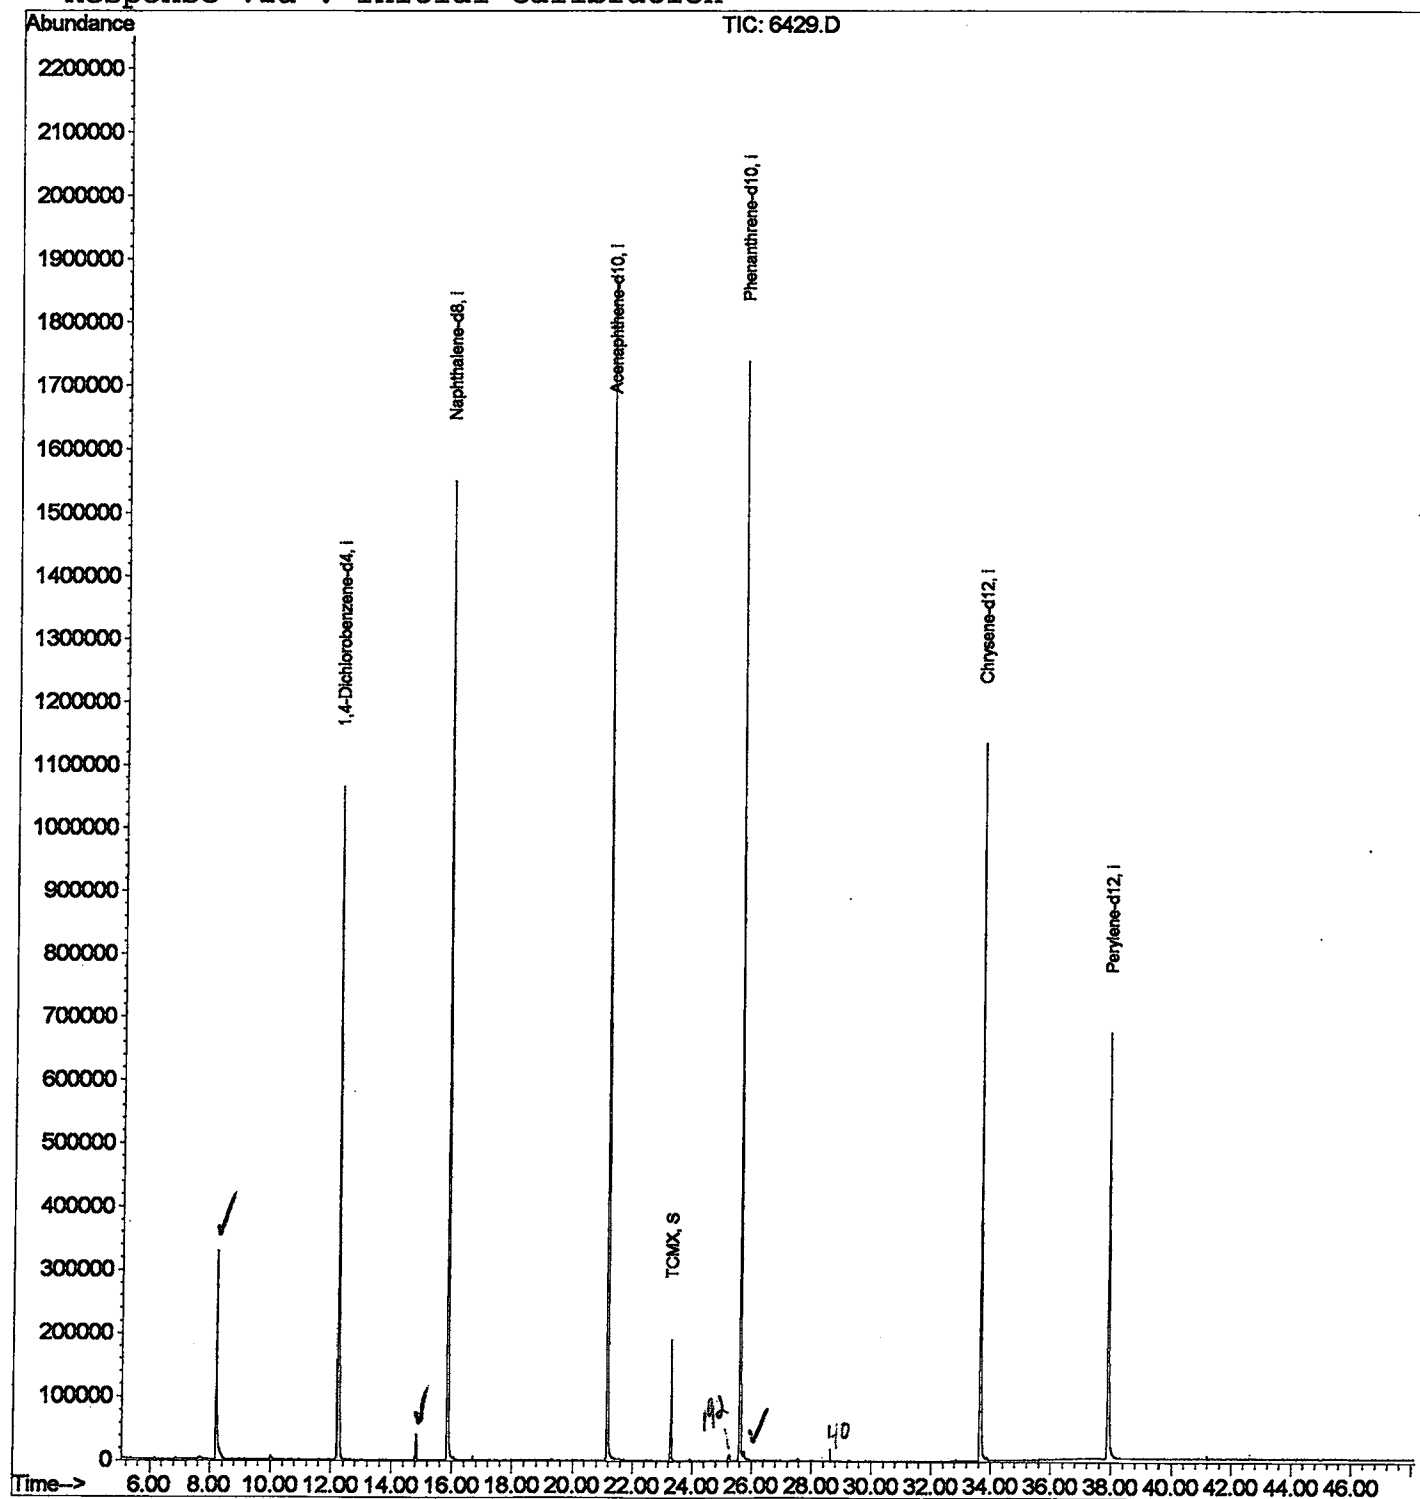

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR1202\6429.D
 Acq On : 15 Apr 2002 6:51 pm
 Sample : re-extract
 Misc :
 MS Integration Params: LSCINT.P

Vial: 12
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.206	340	344	373	rBV	328469	808797	21.01%	4.168%
2	12.227	777	782	798	rBV	1064864	2567976	66.69%	13.233%
3	14.825	1060	1065	1071	rVB	40398	80624	2.09%	0.415%
4	15.862	1172	1178	1195	rBV	1550263	3305415	85.84%	17.034%
5	21.169	1750	1756	1771	rBV	1874030	3850475	100.00%	19.843%
6	23.308	1982	1989	1996	rBV	191729	379548	9.86%	1.956%
7	25.612	2233	2240	2251	rBV2	1738387	3690443	95.84%	19.018%
8	25.750	2251	2255	2267	rVB	13655	45362	1.18%	0.234%
9	33.663	3111	3117	3134	rBV2	1135403	2654713	68.95%	13.680%
10	37.904	3571	3579	3597	rBV	671917	2021806	52.51%	10.419%

Sum of corrected areas: 19405159

6429.D GCMS0412.M Tue Apr 16 15:41:58 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR1202\6429.D
 Operator :
 Acquired : 15 Apr 2002 6:51 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: re-extract
 Misc Info :
 Vial Number: 12
 Quant File :GCMS0412.RES (RTE Integrator)

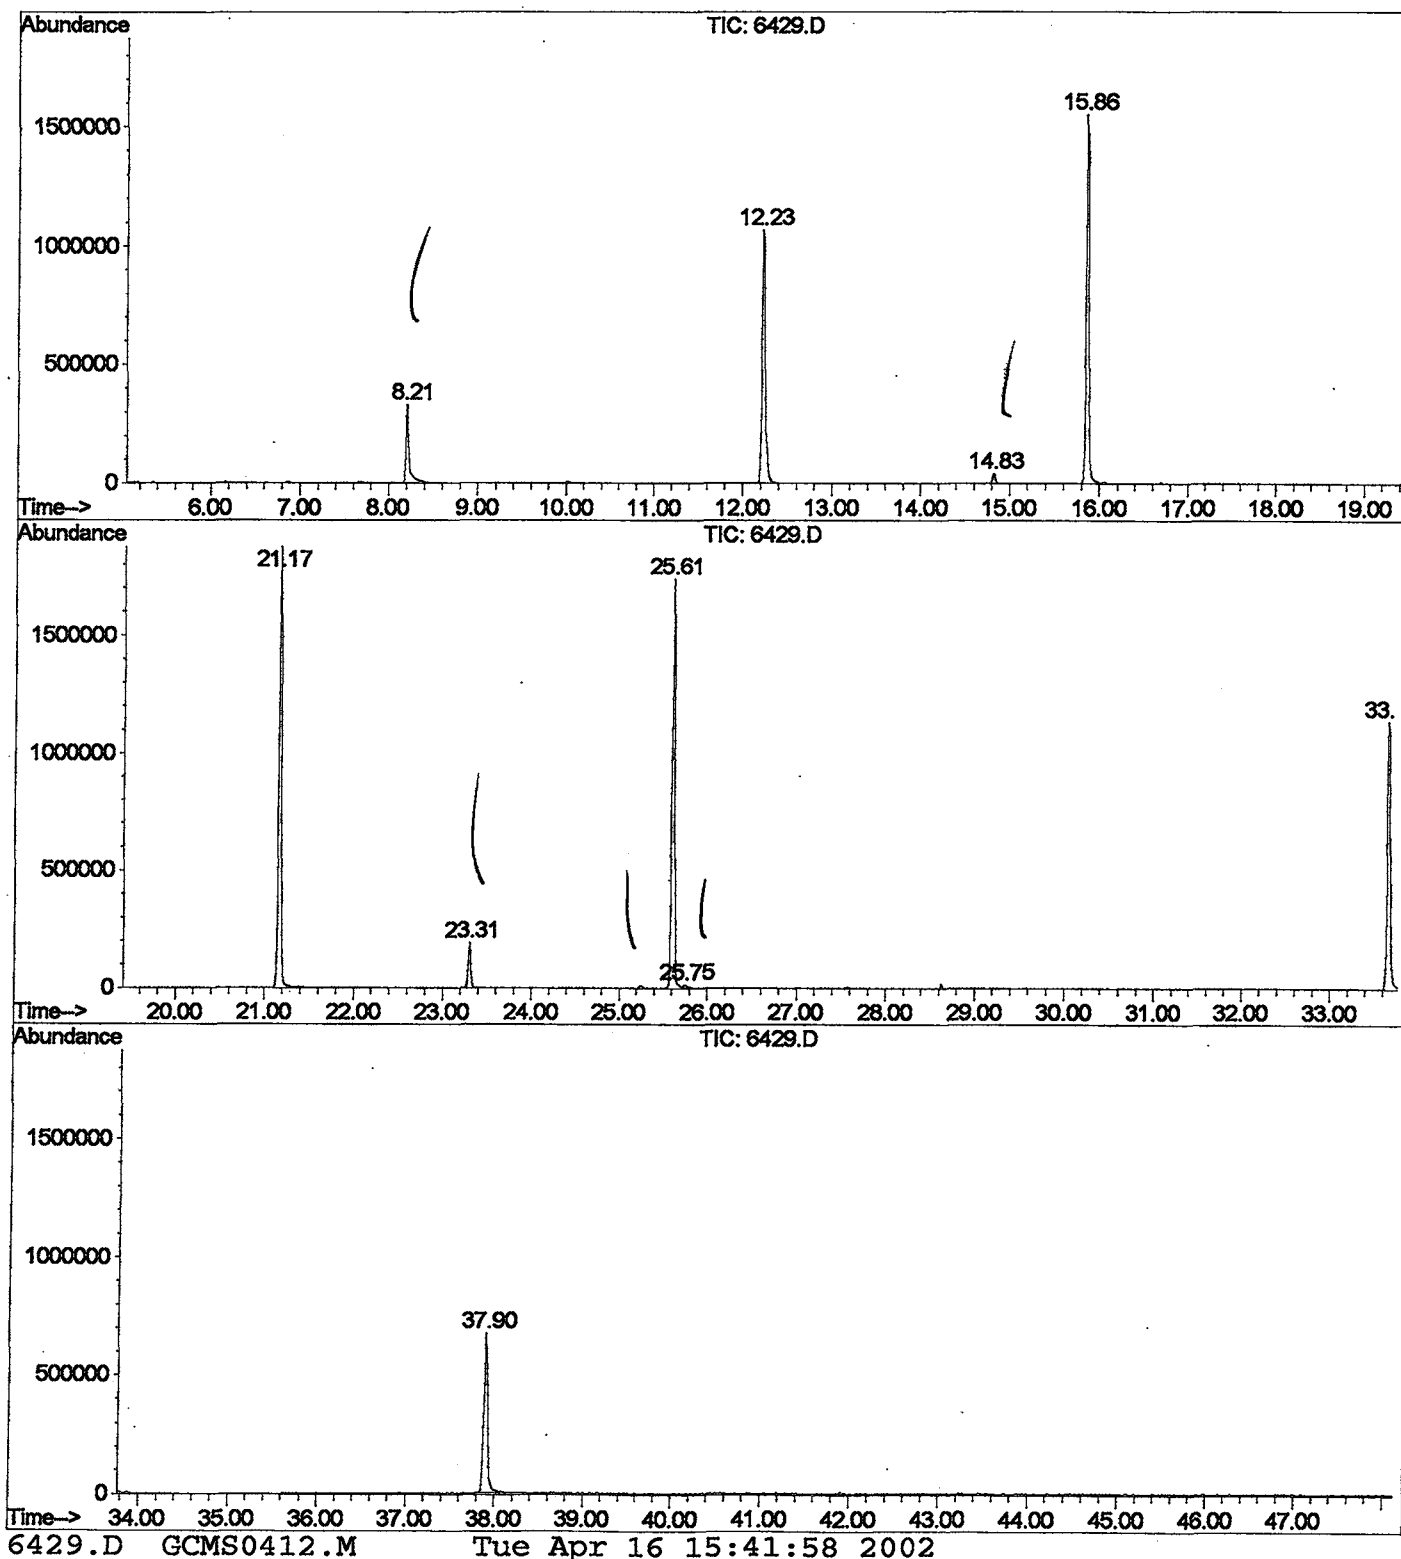

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR1202\6429.D
Acq On : 15 Apr 2002 6:51 pm
Sample : re-extract
Misc :
MS Integration Params: LSCINT.P









Vial: 12
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.21	6.30 ug/l	808797	1,4-Dichlorobenzene-d4	12.23

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2			Acetic acid, cyano-, 1,1-dimethylet	141	C7H11NO2	001116-98-9	17
3			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
4			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9

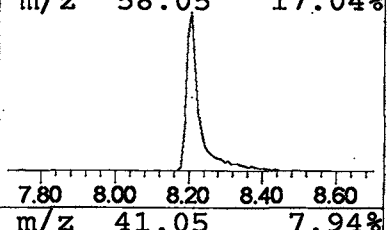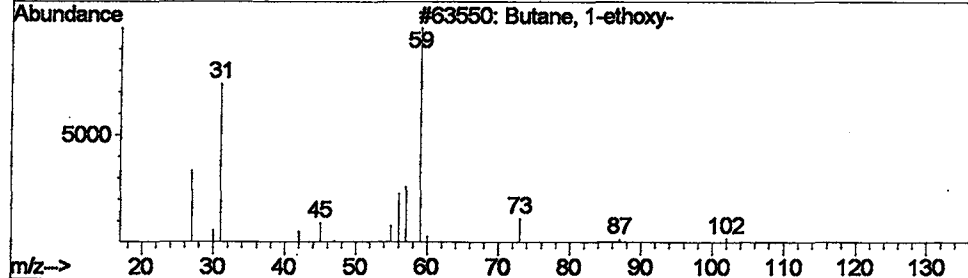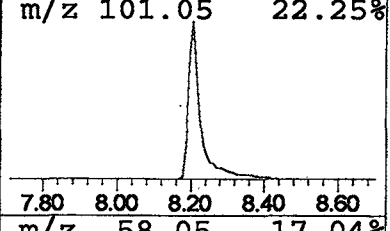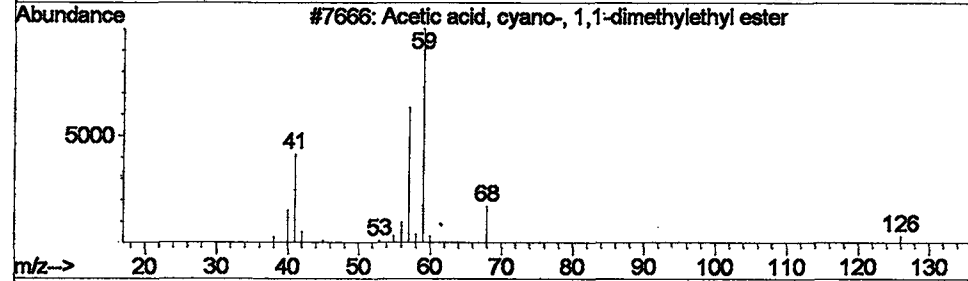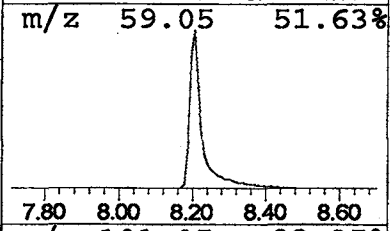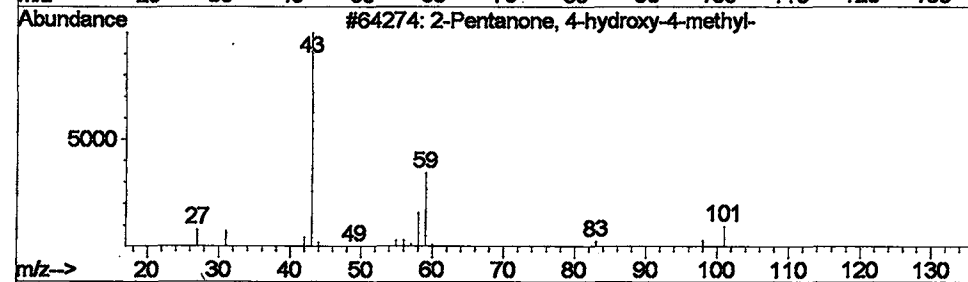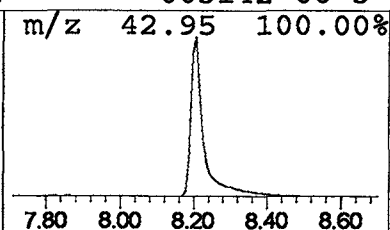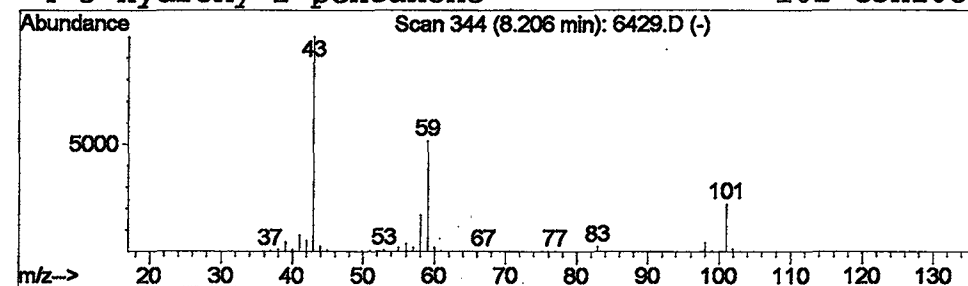

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR1202\6429.D
 Acq On : 15 Apr 2002 6:51 pm
 Sample : re-extract
 Misc :
 MS Integration Params: LSCINT.P


Vial: 12
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.83	0.49 ug/l	80624	Naphthalene-d8	15.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	58
2			3,4-Dihydroxybenzyl alcohol, tris(tr	356	C16H32O3Si3	068595-79-9	52
3			N-(Trifluoroacetyl)-N,O,O',O''-tetr	553	C22H42F3NO4Si4	000000-00-0	35
4			Benzeneethanamine, N-[(pentafluorop	563	C24H34F5NO3Si3	055429-13-5	32

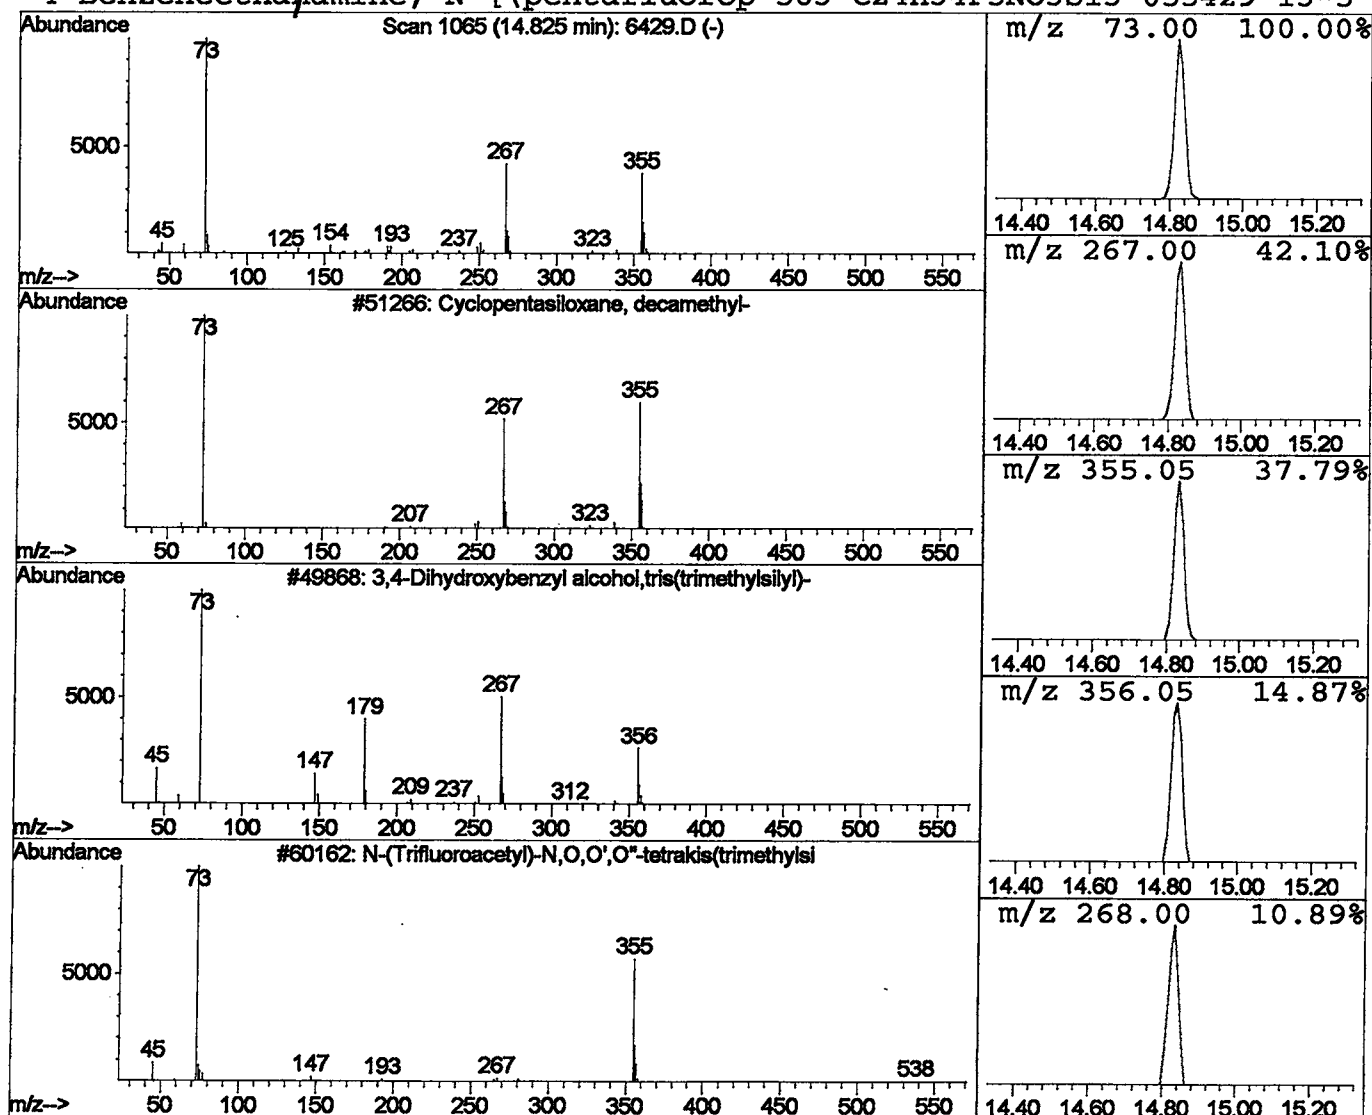

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR1202\6429.D
Acq On : 15 Apr 2002 6:51 pm
Sample : re-extract
Misc :
MS Integration Params: LSCINT.P


Vial: 12
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 3 Anthracene-d10- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.75	0.25 ug/l	45362	Phenanthrene-d10	25.61

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Anthracene-d10-	188	C14D10	001719-06-8	50
2	Phenanthrene-d10	188	C14D10	001517-22-2	47
3	Antipyrine	188	C11H12N2O	000060-80-0	45
4	Naphthalene, 1,7-dimethoxy-	188	C12H12O2	005309-18-2	45

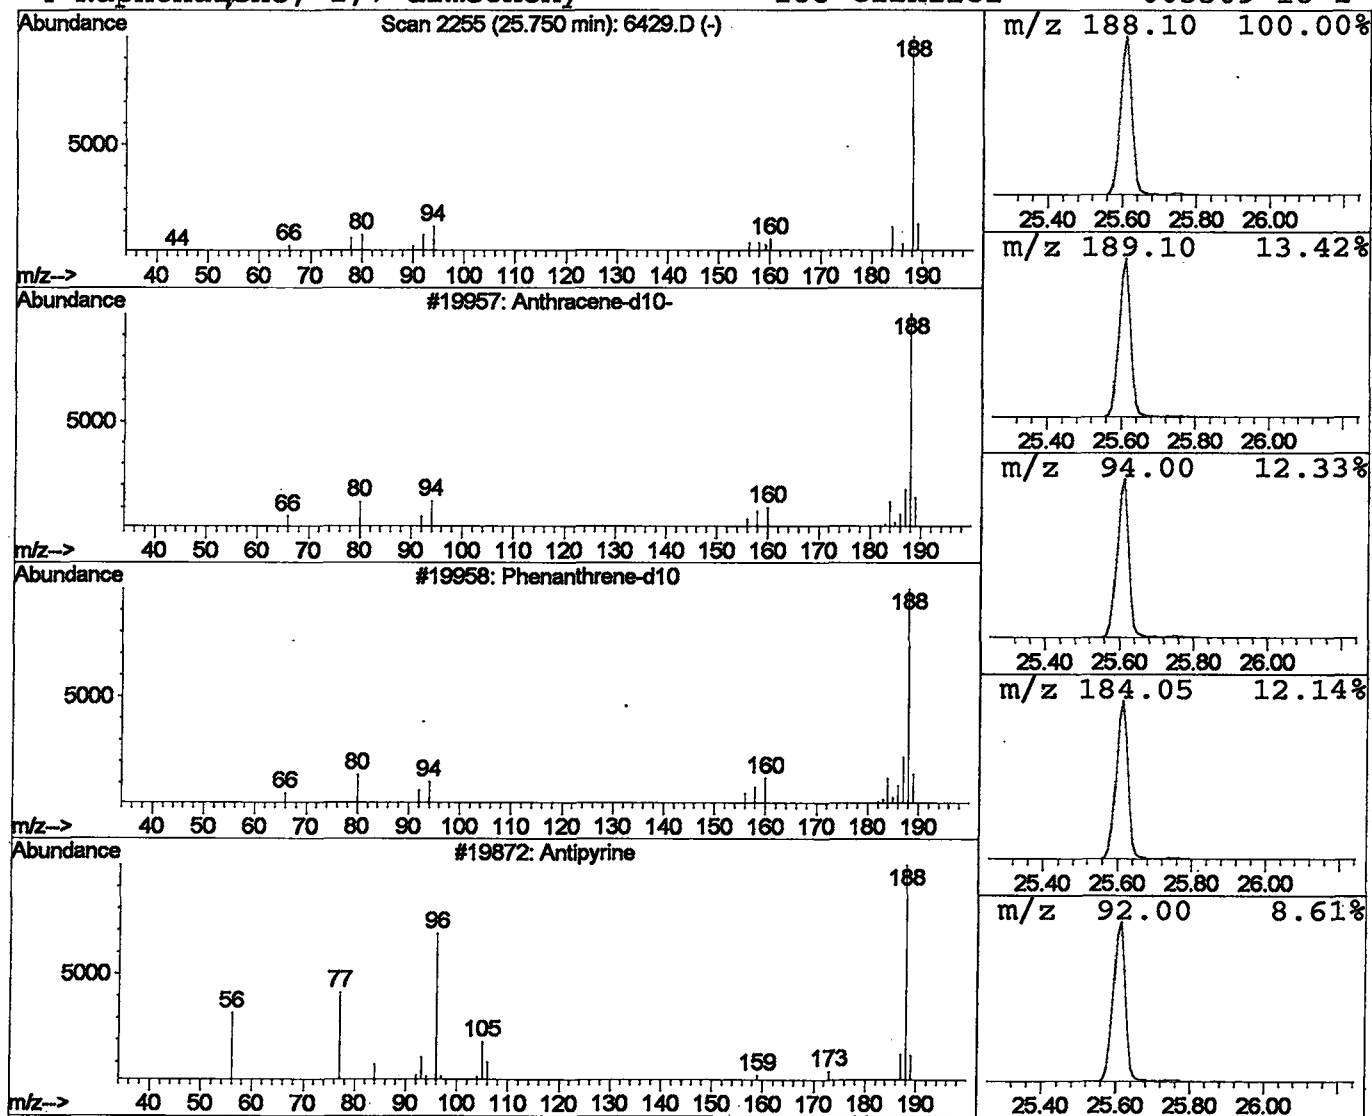

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 15 Apr 2002 6:51 pm
Data File: C:\HPCHEM\1\DATA\APR1202\6429.D
Name: re-extract
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.21	6.3	ug/l	808797	ISTD01	12.23	2567980	20.0
Cyclopentasiloxane,	14.83	0.5	ug/l	80624	ISTD02	15.86	3305420	20.0
Anthracene-d10-	25.75	0.2	ug/l	45362	ISTD04	25.61	3690440	20.0

6429.D GCMS0412.M Tue Apr 16 15:42:02 2002

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0405\6429.D
 Acq On : 6 Apr 2002 3:47 am
 Sample : gc/ms scan 3/19
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 10 12:21 2002

Vial: 15
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 10 10:43:06 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0403

original

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	430352	20.00	ug/l	-0.01
10) Naphthalene-d8	15.89	136	1560096	20.00	ug/l	-0.02
17) Acenaphthene-d10	21.19	164	876957	20.00	ug/l	-0.01
30) Phenanthrene-d10	25.63	188	1202363	20.00	ug/l	-0.03
39) Chrysene-d12	33.69	240	574996	20.00	ug/l	-0.03
45) Perylene-d12	37.93	264	317951	20.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	0.00	209	0	0.00	ug/mL	
Spiked Amount	4.000		Recovery	=	0.00%	
38) 2,4-DDD	30.70	235	60081	5.42	ug/mL	0.20
Spiked Amount	5.000		Recovery	3.4	100.40%	64%

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.93	128	108	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.68	149	620	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

6429.D GCMS0408.M Wed Apr 10 12:21:26 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0405\6429.D

Vial: 15

Acq On : 6 Apr 2002 3:47 am

Operator:

Sample : gc/ms scan 3/19

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 10 12:21 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Apr 10 10:43:06 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.63	178	276	N.D.	
35) Anthracene	25.63	178	276	N.D.	
36) Di-n-butylphthalate	27.60	149	10741	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo(a)anthracene	33.69	228	1164	N.D.	
43) Bis(2-ethylhexyl)phthalate	33.91	149	31400	1.84 ug/l	99
44) Chrysene	33.69	228	1164	N.D.	
46) Di-n-Octylphthalate	0.00	149	0	N.D.	
47) Benzo(b)fluoranthene	0.00	252	0	N.D.	
48) Benzo(k)fluoranthene	0.00	252	0	N.D.	
49) Benzo(a)pyrene	37.94	252	1235	N.D.	
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

6429.D GCMS0408.M Wed Apr 10 12:21:27 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0405\6429.D
 Acq On : 6 Apr 2002 3:47 am
 Sample : gc/ms scan 3/19
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 10 12:21 2002

Vial: 15
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0408.RES

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 10 10:43:06 2002
 Response via : Initial Calibration

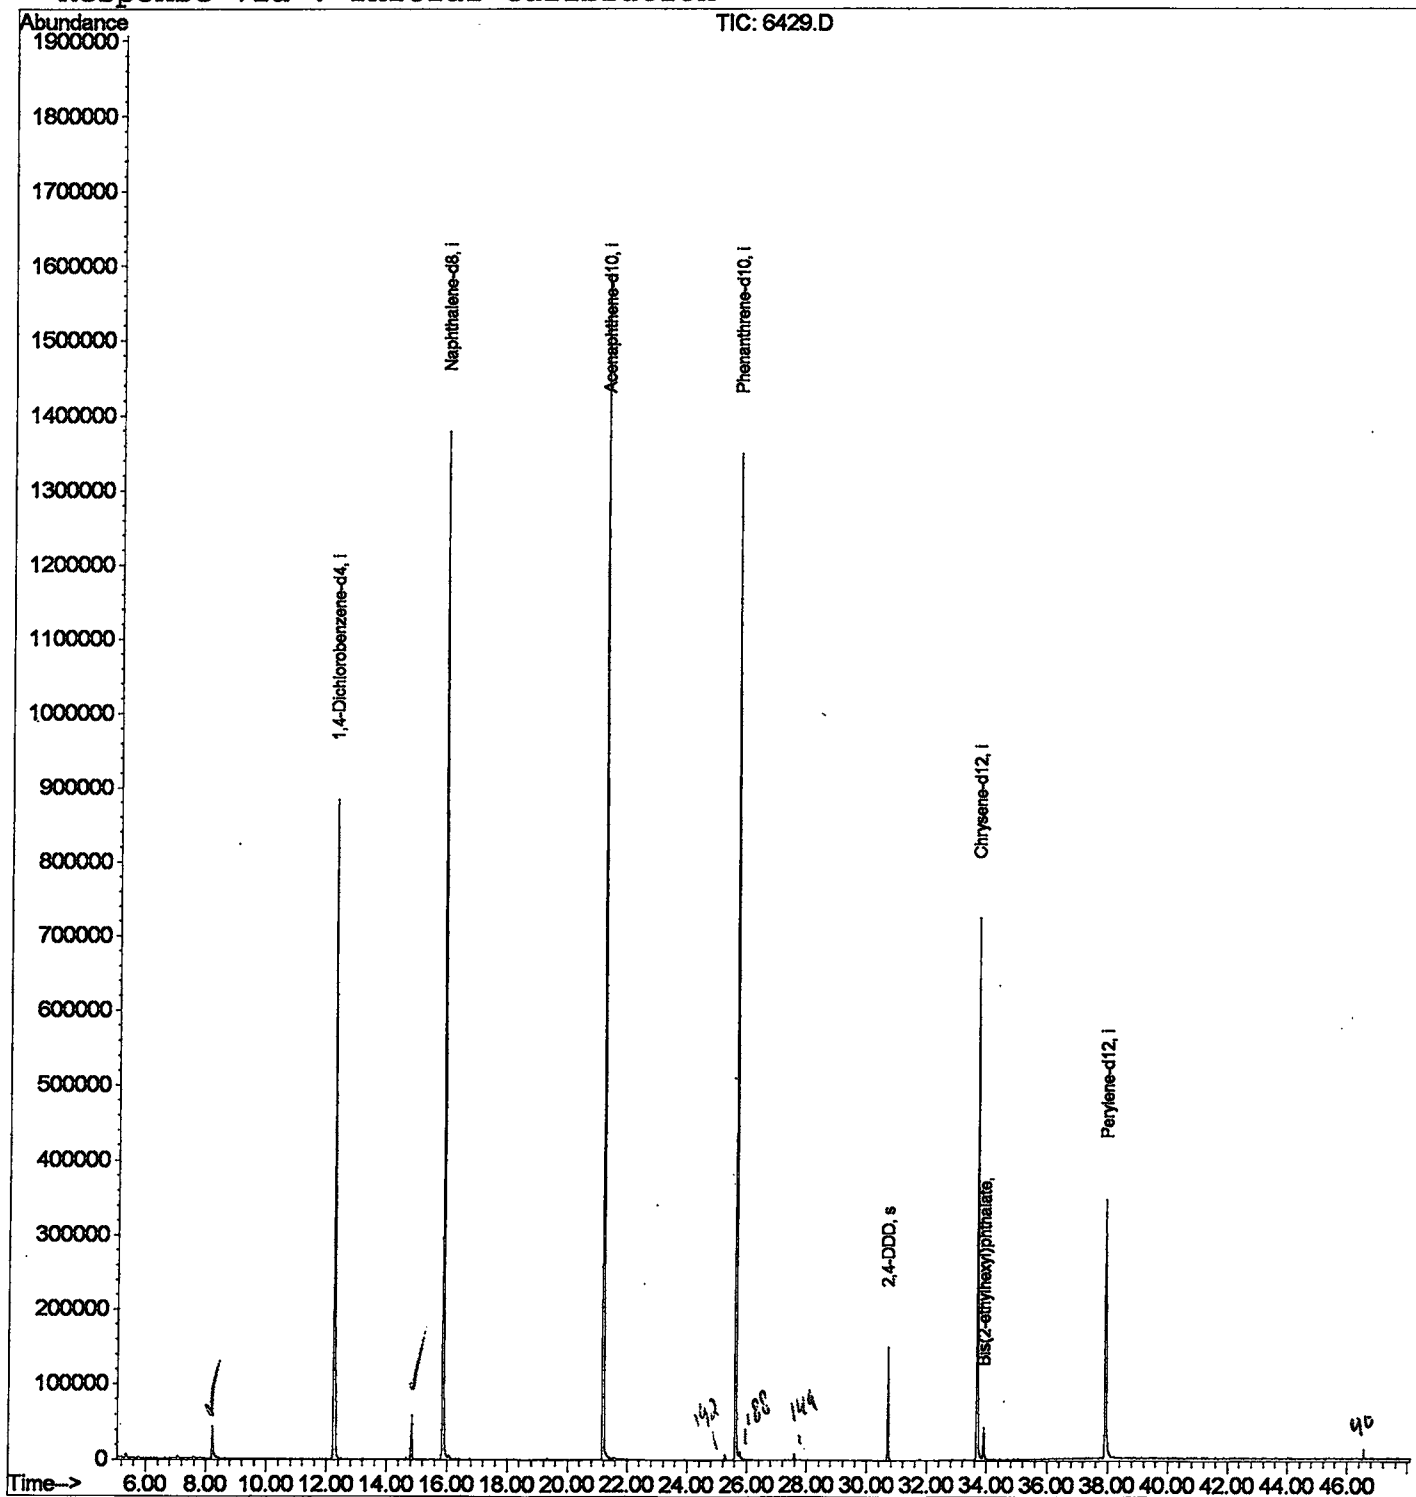

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0405\6429.D

Acq On : 6 Apr 2002 3:47 am

Sample : gc/ms scan 3/19

Misc :

MS Integration Params: LSCINT.P

Vial: 15

Operator:

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.219	343	346	362	rBV	43607	112485	3.35%	0.750%
2	12.240	779	784	801	rBV	883141	2309990	68.73%	15.407%
3	14.848	1064	1068	1073	rVB	59780	119508	3.56%	0.797%
4	15.885	1174	1181	1198	rBV	1379618	2942074	87.53%	19.623%
5	21.191	1752	1759	1777	rBV	1588614	3361136	100.00%	22.418%
6	25.625	2236	2242	2254	rBV2	1349928	3018132	89.79%	20.130%
7	30.702	2790	2795	2804	rBV	150618	298935	8.89%	1.994%
8	33.686	3114	3120	3133	rBV2	725153	1654010	49.21%	11.032%
9	33.906	3139	3144	3152	rVB	43260	100322	2.98%	0.669%
10	37.927	3573	3582	3603	rBV2	346463	1076649	32.03%	7.181%


Sum of corrected areas: 14993241

6429.D GCMS0408.M

Wed Apr 10 12:24:15 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0405\6429.D
 Operator :
 Acquired : 6 Apr 2002 3:47 am using AcqMethod GCMS0403
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/19
 Misc Info :
 Vial Number: 15
 Quant File :GCMS0408.RES (RTE Integrator)

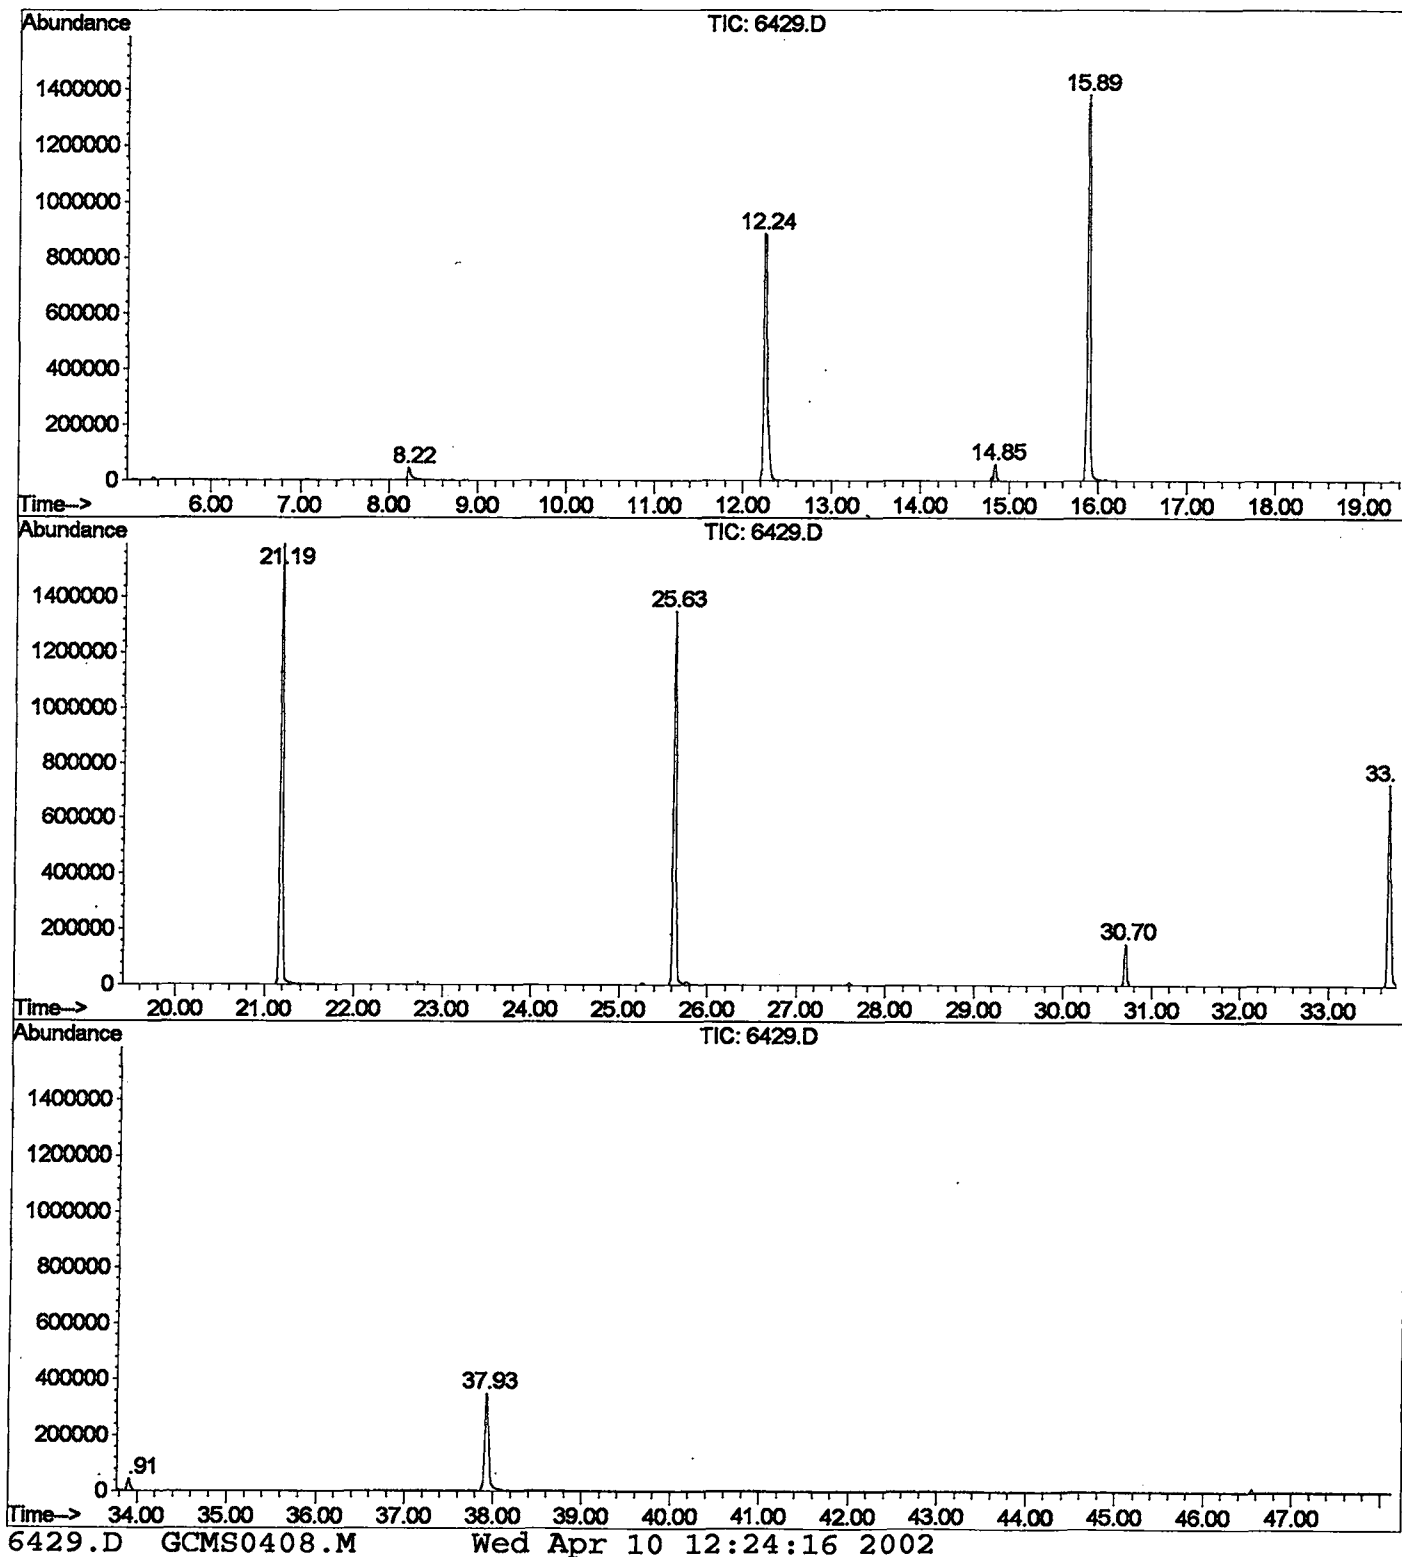

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0405\6429.D

Acq On : 6 Apr 2002 3:47 am

Sample : gc/ms scan 3/19

Misc :

MS Integration Params: LSCINT.P

Vial: 15

Operator:

Inst : GC/MS 209

Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.22	0.97 ug/l	112485	1,4-Dichlorobenzene-d4	12.25

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Acetone	58	C3H6O	000067-64-1	9
3		3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

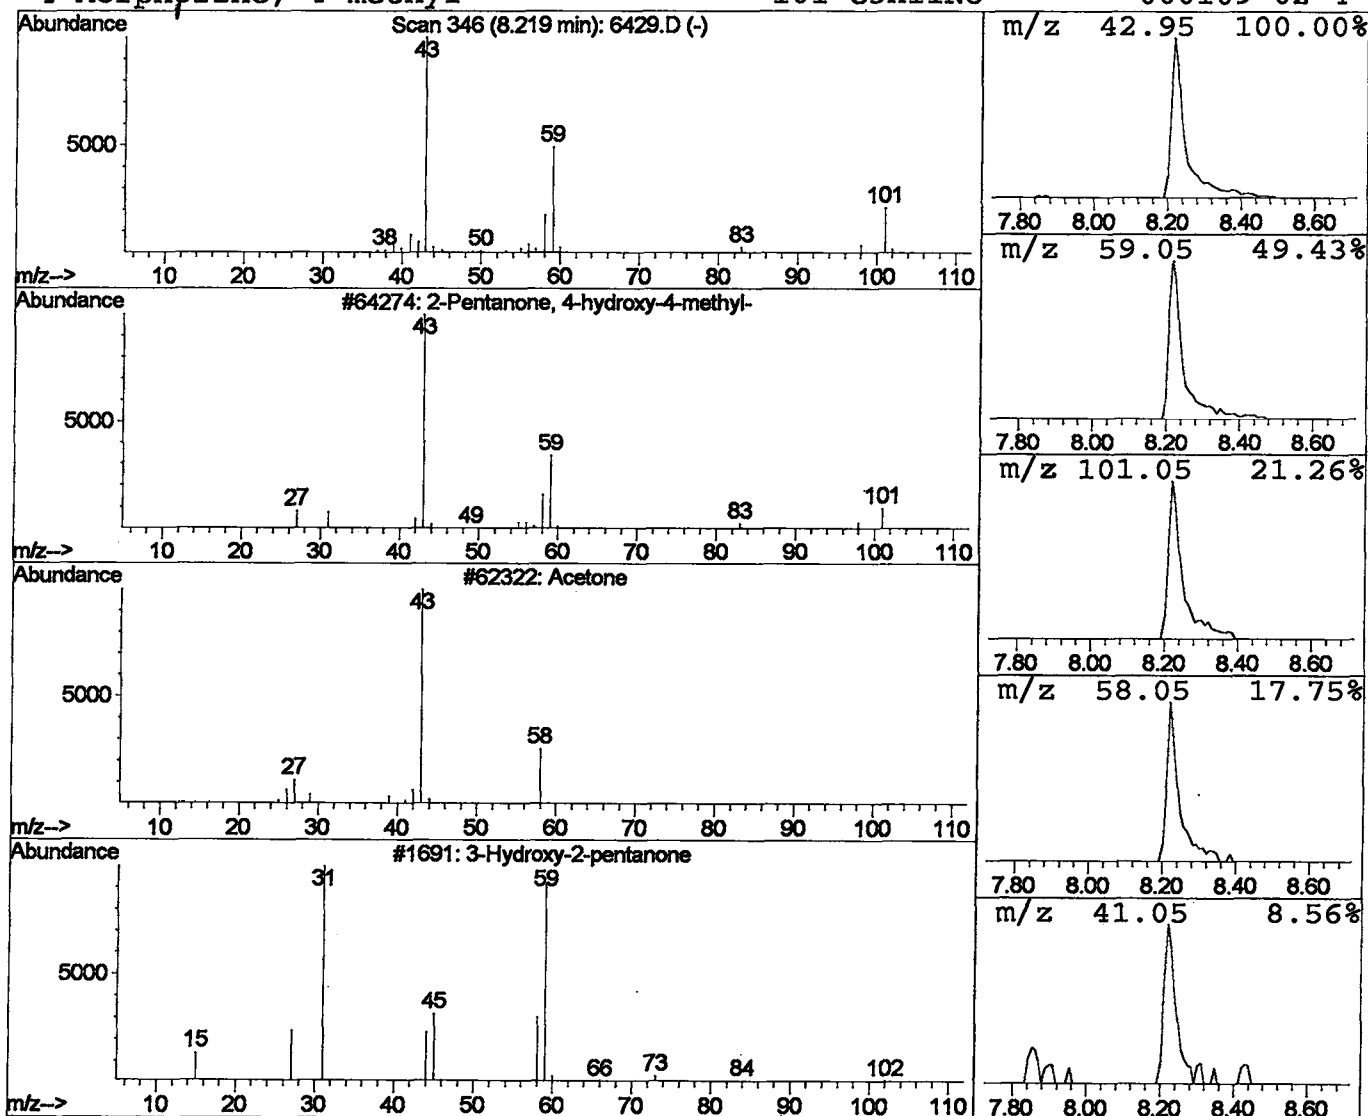

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0405\6429.D
Acq On : 6 Apr 2002 3:47 am
Sample : gc/ms scan 3/19
Misc :
MS Integration Params: LSCINT.P

Vial: 15
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Library : C:\DATABASE\NBS75K.L

Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.85	0.81 ug/l	119508	Naphthalene-d8	15.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	52
2			Phenethylamine, N-methyl-.beta.,3,4	399	C18H37NO3Si3	010538-85-9	38
3			N-(Trifluoroacetyl)-O,O',O''-tris(t	481	C19H34F3NO4Si3	000000-00-0	38
4			N-(Trifluoroacetyl)-N,O,O',O''-tetr	553	C22H42F3NO4Si4	000000-00-0	38

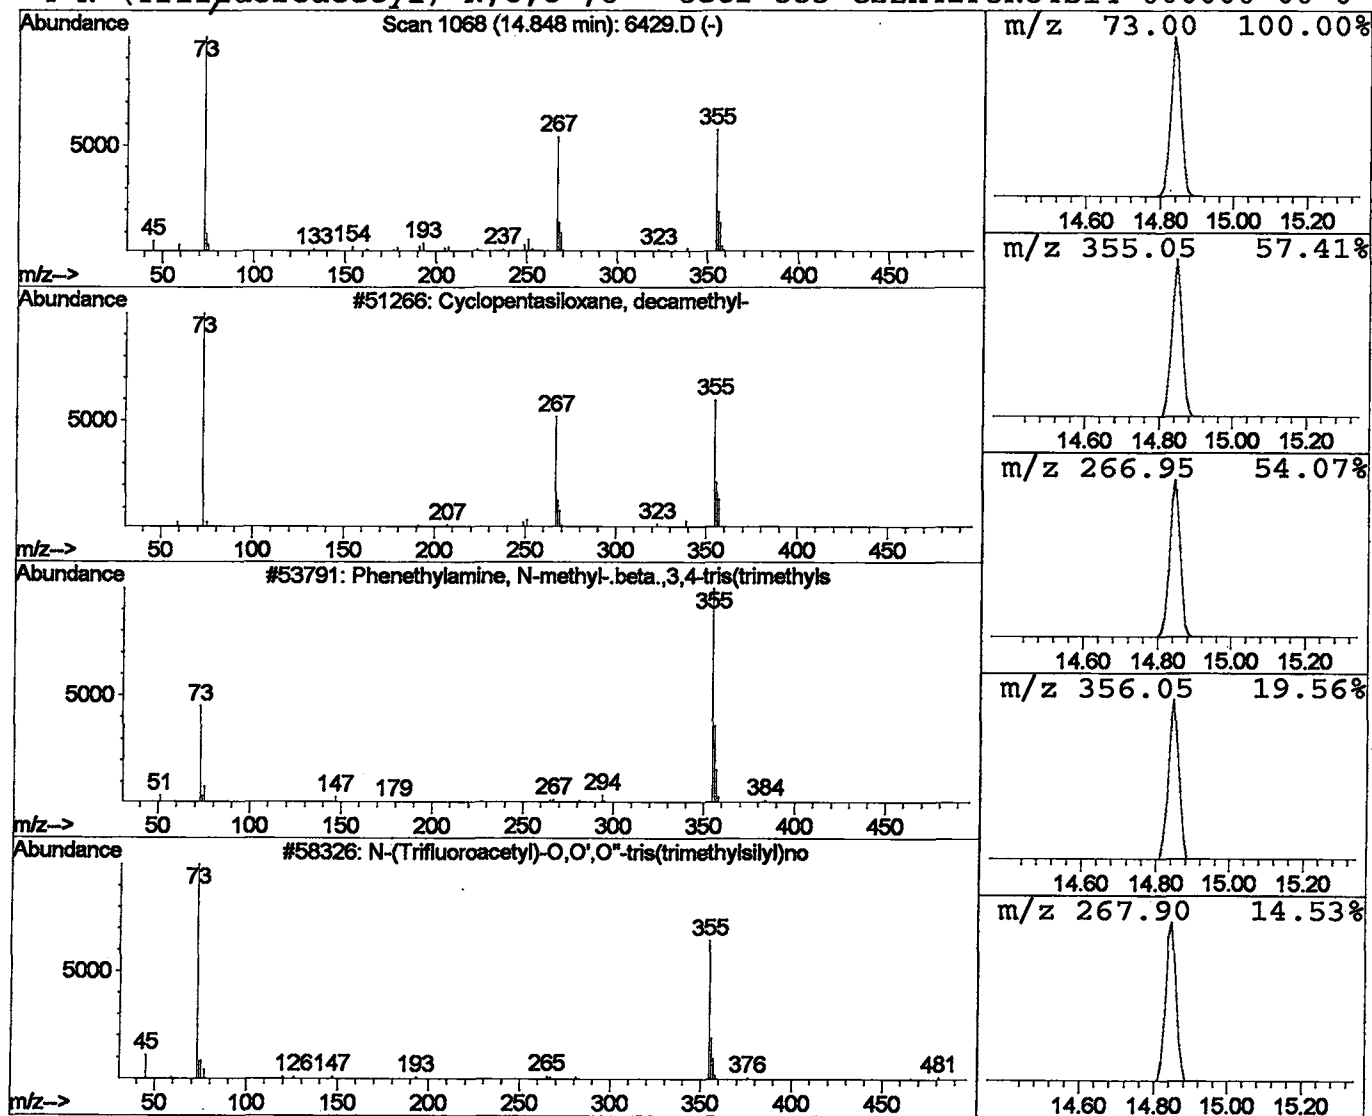

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 6 Apr 2002 3:47 am
 Data File: C:\HPCHEM\1\DATA\APR0405\6429.D
 Name: gc/ms scan 3/19
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone/4-hydro	8.22	1.0	ug/l	112485	ISTD01	12.25	2309990	20.0
Cyclopentasiloxane,	14.85	0.8	ug/l	119508	ISTD02	15.89	2942070	20.0

6429.D GCMS0408.M Wed Apr 10 12:24:18 2002