

Method 508 MOD.

Date Extracted 4/12/02

Page 58

Rob

\$GCMS-18143

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500ml		1ml			1ml	4A	7			
Ref 1					1ml			10B				
Ref 2					1ml			10A				
7770	Re-EXT.							9A				
7710	Re-EXT.							2B				
7715	Re-EXT.							7B				
8760								1B				
8761								2A				
8762	FB.							7A				
8833								1A				
8834								4B				
8835								7B				
8836								6A				
Remarks												
Reviewed by, <u>C/B 9/16/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type - <u>Sep. Fun.</u> Solv. lot# <u> </u> NaCl lot# <u>V 396/4</u> Na2SO4 lot# <u>V 46648</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>1104100</u>											
REF SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>1504190</u>											
SURROGATE												
LPC												
ENDRIN/DDT												

Analyst A.D.
revision 4/12/01

Verified by [Signature]

Reviewed by [Signature]
Date 4/25/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\APR2202.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\apr2202\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

☒ Full Method☐ Reprocessing Only

On A Barcode Mismatch


☒ Inject Anyway☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0412	
2	Sample	2	CAL80	GCMS0412	
3	Sample	3	LB	GCMS0412	gc/ms scan 4/11
4	Sample	4	REF1	GCMS0412	gc/ms scan 4/11
5	Sample	5	REF2	GCMS0412	gc/ms scan 4/11
6	Sample	6	8684	GCMS0412	gc/ms scan 4/11
7	Sample	7	8685	GCMS0412	gc/ms scan 4/11
8	Sample	8	8686	GCMS0412	gc/ms scan 4/11
9	Sample	9	8687	GCMS0412	gc/ms scan 4/11
10	Sample	10	8688	GCMS0412	gc/ms scan 4/11 fb
11	Sample	11	8755	GCMS0412	gc/ms scan 4/11
12	Sample	12	8756	GCMS0412	gc/ms scan 4/11
13	Sample	13	8757	GCMS0412	gc/ms scan 4/11
14	Sample	14	8758	GCMS0412	gc/ms scan 4/11 fb
15	Sample	15	8759	GCMS0412	gc/ms scan 4/11
16	Sample	16	LBA	GCMS0412	gc/ms scan 4/12
17	Sample	17	REFA1	GCMS0412	gc/ms scan 4/12
18	Sample	18	REFA2	GCMS0412	gc/ms scan 4/12
19	Sample	19	7770	GCMS0412	re-ext
20	Sample	20	7110	GCMS0412	re-ext
21	Sample	21	7115	GCMS0412	re-ext
22	Sample	22	8760	GCMS0412	gc/ms scan 4/12
23	Sample	23	8761	GCMS0412	gc/ms scan 4/12
24	Sample	24	8762	GCMS0412	gc/ms scan 4/12 fb
25	Sample	25	8833	GCMS0412	gc/ms scan 4/12
26	Sample	26	8834	GCMS0412	gc/ms scan 4/12
27	Sample	27	8835	GCMS0412	gc/ms scan 4/12
28	Sample	28	8836	GCMS0412	gc/ms scan 4/12

DFTPP

Data File : C:\HPCHEM\1\DATA\APR2202\DFTPP.D
 Acq On : 22 Apr 2002 8:27 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

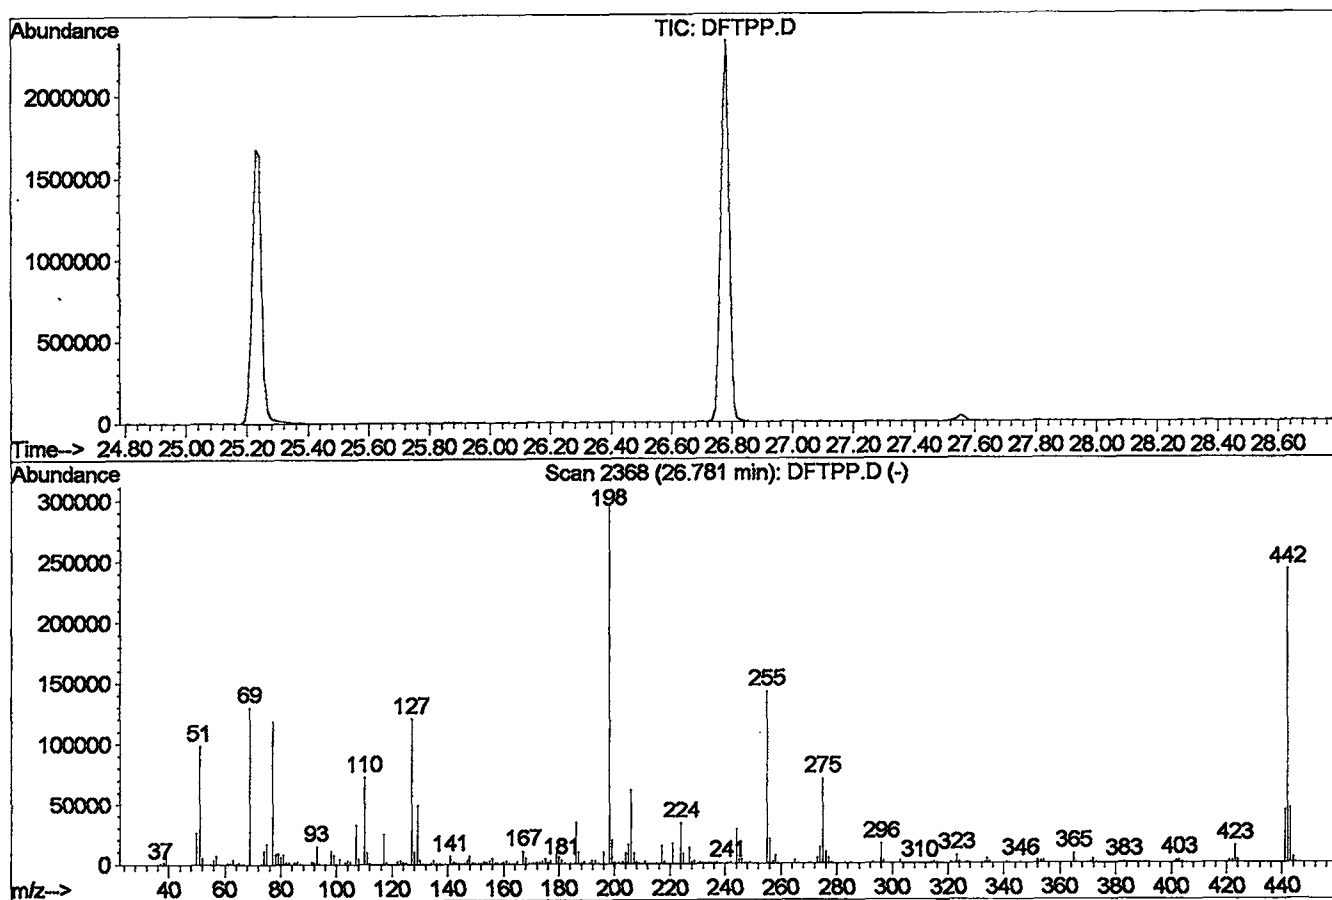

Spectrum Information: Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.2	98688	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.8	130160	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	40.7	120912	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	296896	PASS
199	198	5	9	6.6	19696	PASS
275	198	10	30	23.9	70992	PASS
365	198	1	100	2.6	7777	PASS
441	443	0.01	100	94.8	43256	PASS
442	198	40	110	81.5	242048	PASS
443	442	17	23	18.8	45616	PASS