

Method 508mod

Date Extracted 4-15-02

Page 59

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	Notes
LB		500ml		1ml	1ml		1ml	1A	7		Need
REF					1ml			1B			
REF					↓			4A			
89362								4B			
8937	FB							1B			
8949								2B			
8950								1A			
8951								2A			✓
8952	FB							7B			
8953								6A			
8954								8B			
8955								7A			
8956	FB							8A			
Remarks											
Reviewed by, <u>SPB 8/16/02</u>											
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -											
Extraction type <u>sep fun</u> Solv. lot# <u>N44470</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V46648</u>											
STANDARD	INT STD LOG#										
CALIBRATION											
REF SPIKE	2193										
MDL/MDRF											
Q. CHECK											
INT. STD.											
SURROGATE	TCM X										
LPC											
ENDRIN/DDT											

Analyst FH
Revision 4/12/01

Verified by _____

Reviewed by
Date 4/29/02

5085CAN

Method 525.2

Instrument 213

File Directory 042202

Storage Directory


Lab #	Filename	Description	Vial #		Inj.	Standards used - Lot #			Int. Std.	Remarks	Initials
			front	rear		Calibration	Reference	Surrogate			
	DFTAD422	DFTPP	1		1	21106					TB
	C10AD422	C10	2			020412					
	C25AD422	C25	3			1					
	SURRAD422	Surrogate	4			2284F				TCMX, 4/18/02	
	LBAA422	LB	5						2286b		
	REFAA422	Ref	6						1		
	REFBB422	Ref	7								
	MCA40422	MC	8								
	8936	Sample	9						2286b	based on	
	8937		10							cal of	
	8949		11							4/12/02	
	50		12								
	51		13								
	52		14								
	53		15								
	54		16								
	55		17								
	8956		18								

Date 4/22/02

Extraction date 4/15/02

Page

File : C:\MSDCHEM\1\DATA\042202\DFTA0422.D
 Operator : Bohlk
 Acquired : 22 Apr 2002 9:55 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: DFTPP
 Misc Info :
 Vial Number: 1

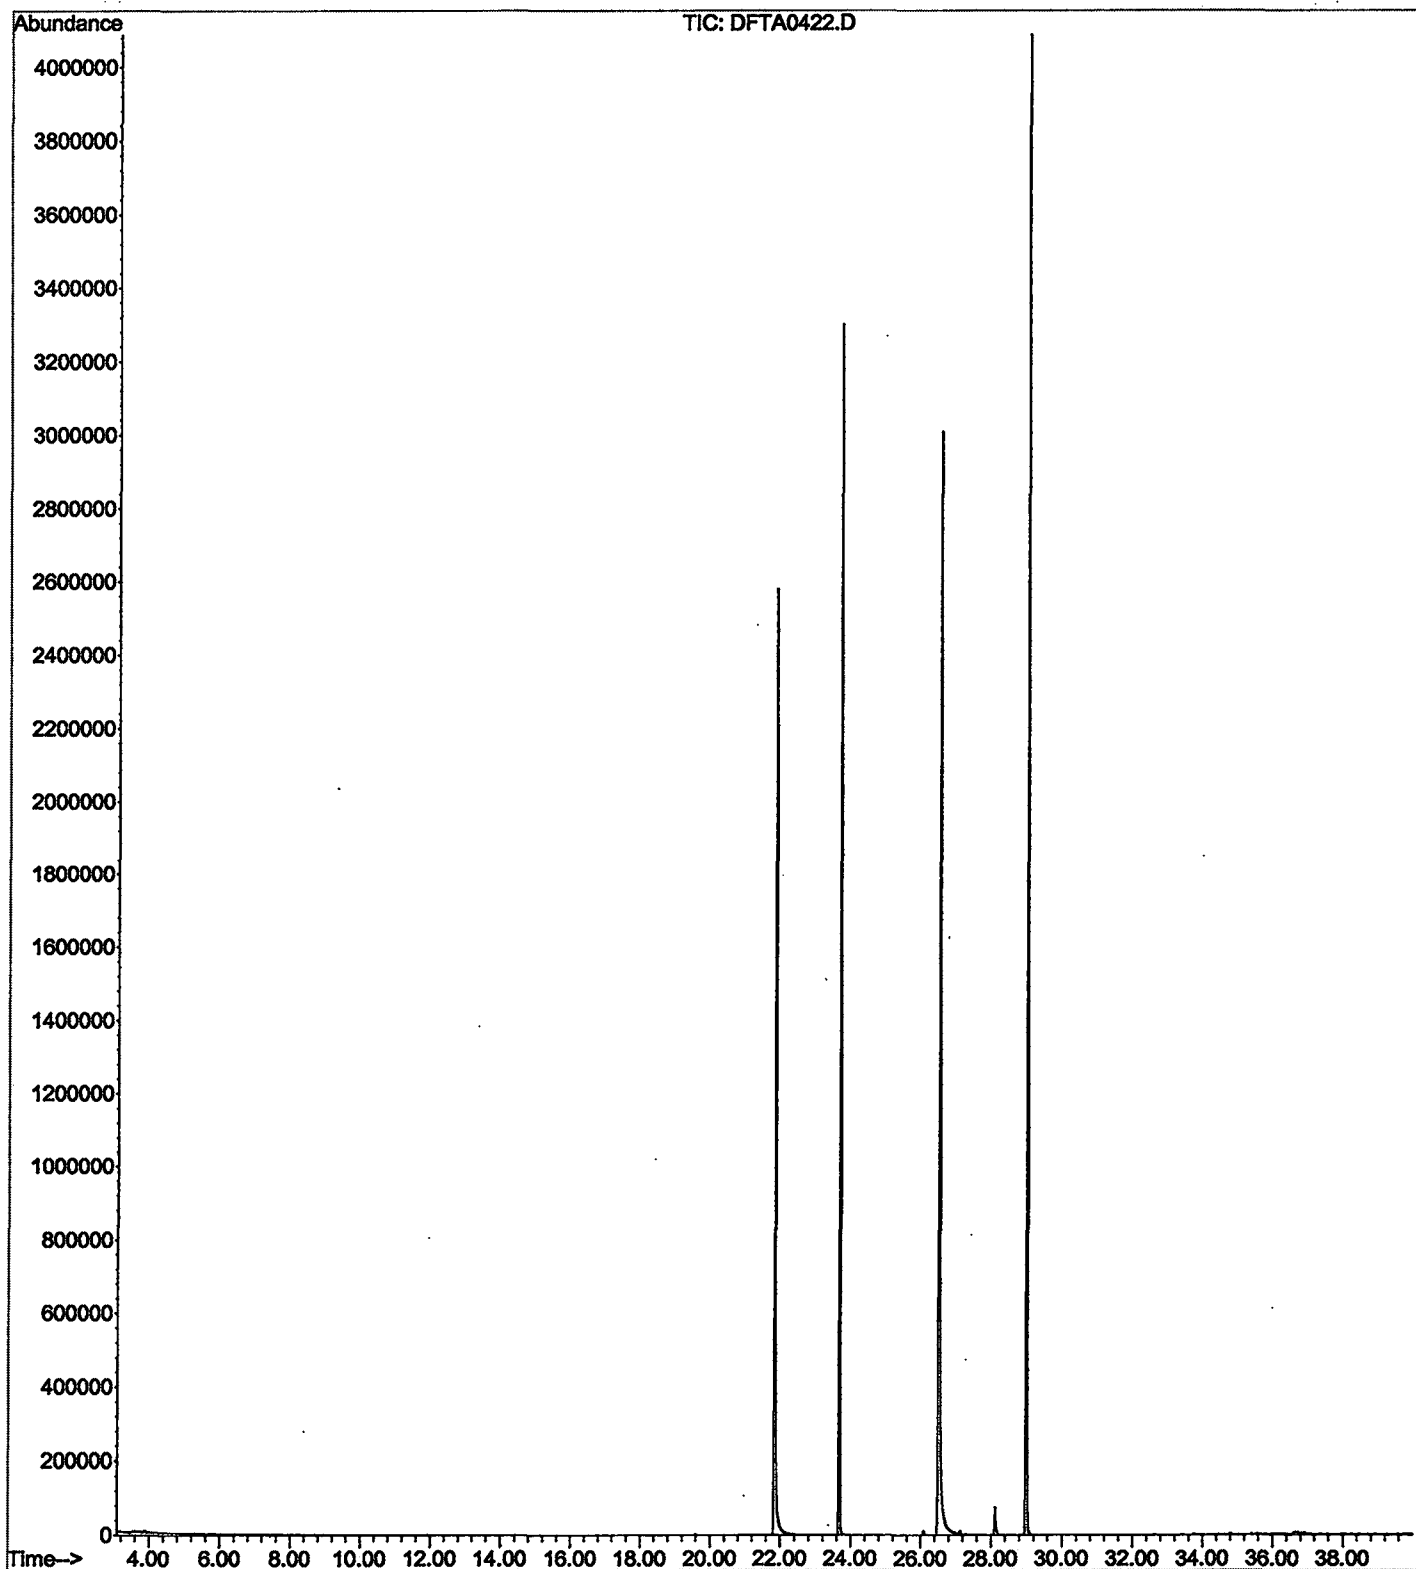

DFTPP

Data File : C:\MSDCHEM\1\DATA\042202\DFTA0422.D
Acq On : 22 Apr 2002 9:55 am
Sample : DFTPP
Misc :
MS Integration Params: BENZO.P

Vial: 1
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
Title : Quantitation For Method 508gcscan

Spectrum Information: Scan 3507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.7	176640	PASS
68	69	0.00	2	1.7	3191	PASS
69	198	0.00	100	46.4	183296	PASS
70	69	0.00	2	0.5	988	PASS
127	198	40	60	53.0	209280	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	395008	PASS
199	198	5	9	6.6	25904	PASS
275	198	10	30	20.4	80720	PASS
365	198	1	100	2.5	9767	PASS
441	443	0.01	100	74.4	36088	PASS
442	198	40	110	61.2	241664	PASS
443	442	17	23	20.1	48536	PASS

DFTA0422.D 5080402BBC.M

Mon Apr 22 10:40:57 2002