

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/29/2002 Time: 09:20:08

Sample: AE08955
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/29/02 09:19 Ended: 4/29/02 09:19 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		73		10.0

Comments for Sample AE08955 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-29-2002 Time: 09:20:45

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\042202\8955.D

Vial: 17

Acq On : 23 Apr 2002 12:16 am

Operator: Bohlk

Sample : SAMPLE 8955 4/15/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 26 12:06:42 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 26 09:52:24 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	402186	40.00	ug/L	0.00
10) Naphthalene-d8	12.88	136	1885012	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1105328	40.00	ug/L	0.00
30) Phenanthrene-d10	22.34	188	1501434	40.00	ug/L	0.00
39) Chrysene-d12	30.14	240	1172056	40.00	ug/L	-0.01
45) Perylene-d12	34.02	264	709828	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	19.95	244	32260	7.31	ug/L	0.00
Spiked Amount 10.000			Recovery	=	73.10%	
38) 2,4-DDD (SURR)	0.00	235	0	0.00	ug/L	
Spiked Amount 10.000			Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	0.00	149	0	N.D. d	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo (a) anthracene	0.00	228	0	N.D.	
43) Bis (2-ethylhexyl) phthala	0.00	149	0	N.D.	
44) Chrysene	0.00	228	0	N.D.	

(#)= qualifier out of range (m) = manual integration

8955.D 5080402BBC.M

Fri Apr 26 12:07:38 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\042202\8955.D

Acq On : 23 Apr 2002 12:16 am

Sample : SAMPLE 8955 4/15/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 26 12:06:42 2002

Vial: 17

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 26 09:52:24 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.		
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

8955.D 5080402BBC.M

Fri Apr 26 12:07:39 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\042202\8955.D

Vial: 17

Acq On : 23 Apr 2002 12:16 am

Operator: Bohlk

Sample : SAMPLE 8955 4/15/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 26 12:07 2002


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 26 09:52:24 2002

Response via : Initial Calibration

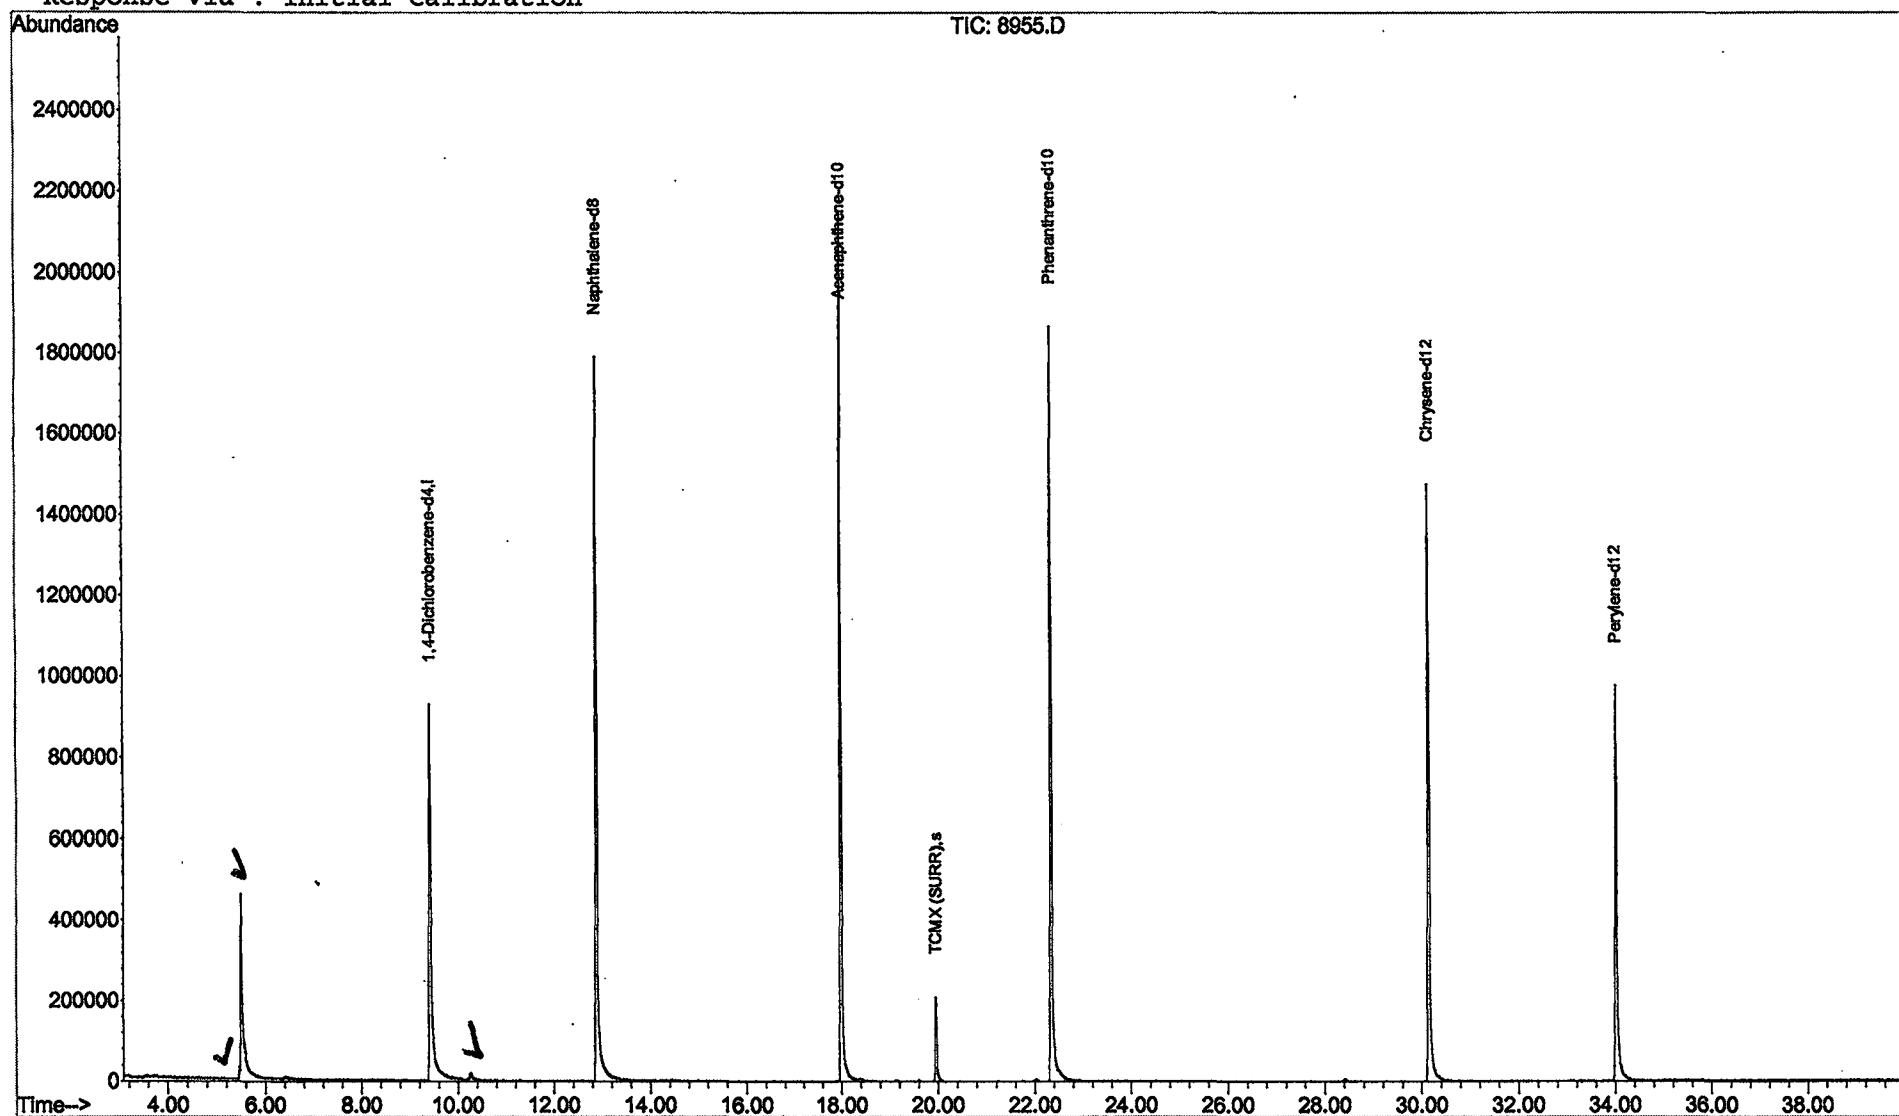

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\042202\8955.D
Acq On : 23 Apr 2002 12:16 am
Sample : SAMPLE 8955 4/15/02
Misc :
MS Integration Params: LSCINT.P

Vial: 17
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.470	403	407	409	rBV	30272	46863	1.02%	0.198%
2	5.500	409	412	438	rVB	450016	1106661	24.04%	4.674%
3	9.413	1071	1078	1101	rBV	928763	2754438	59.84%	11.632%
4	12.879	1661	1668	1704	rBV	1790316	4226766	91.83%	17.850%
5	17.985	2528	2537	2555	rBV	2149823	4602645	100.00%	19.438%
6	19.948	2864	2871	2884	rBV2	209721	491370	10.68%	2.075%
7	22.339	3270	3278	3300	rBV2	1866896	4341949	94.34%	18.337%
8	30.142	4597	4606	4625	rBV2	1474701	3596988	78.15%	15.191%
9	34.020	5256	5266	5285	rBV	974586	2511154	54.56%	10.605%

Sum of corrected areas: 23678834

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\042202\8955.D
 Operator : Bohlk
 Acquired : 23 Apr 2002 12:16 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 8955 4/15/02
 Misc Info :
 Vial Number: 17
 Quant File :5080402BBC.RES (RTE Integrator)

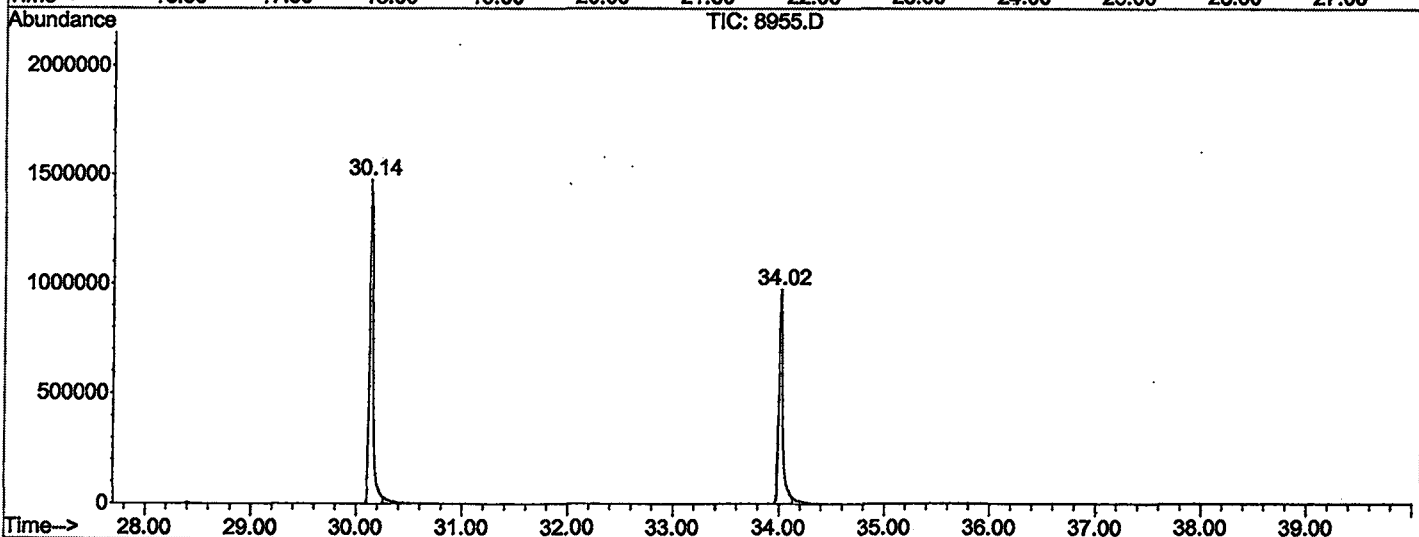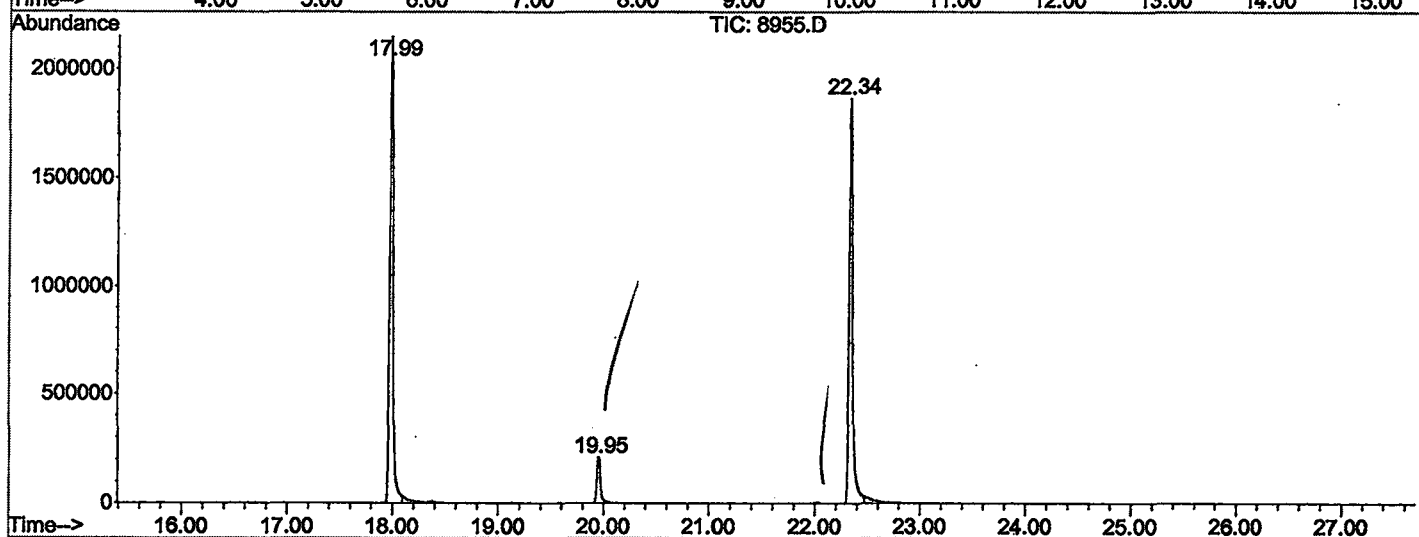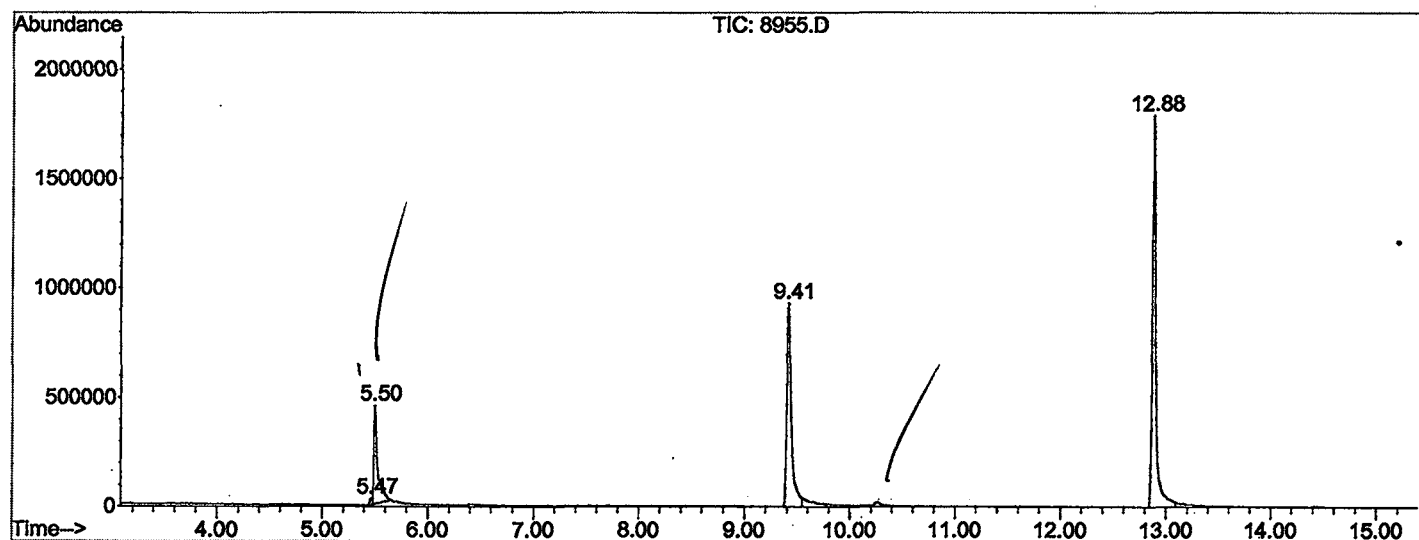

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\042202\8955.D
Acq On : 23 Apr 2002 12:16 am
Sample : SAMPLE 8955 4/15/02
Misc :
MS Integration Params: LSCINT.P










Vial: 17
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Library : C:\DATABASE\WILEY7N.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.50	16.07 ug/L	1106660	1,4-Dichlorobenzene-d4	9.41

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	74	
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53	
3	2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	53	
4	2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	50	

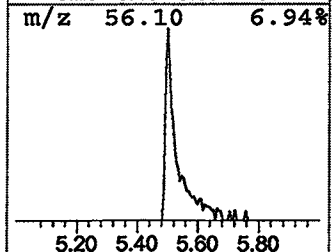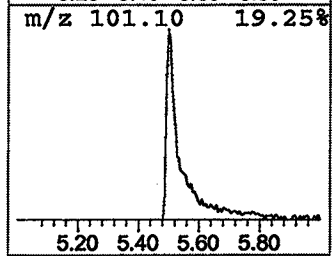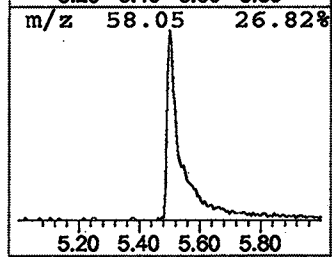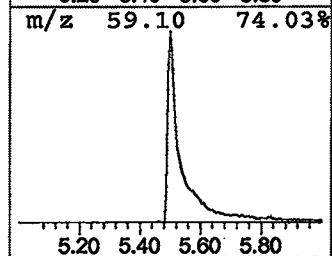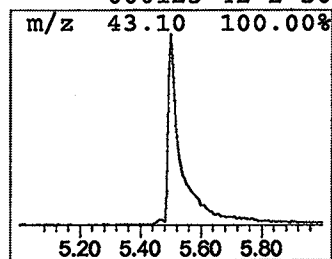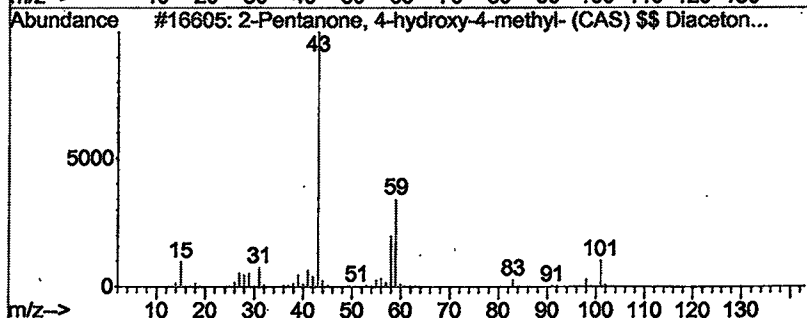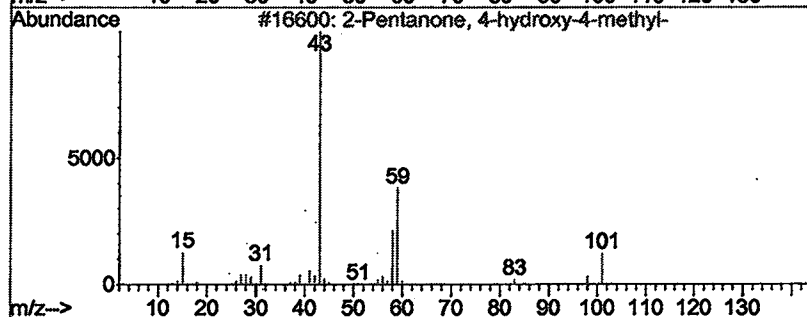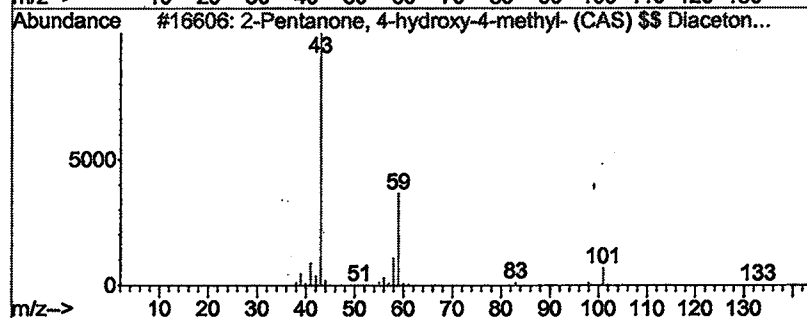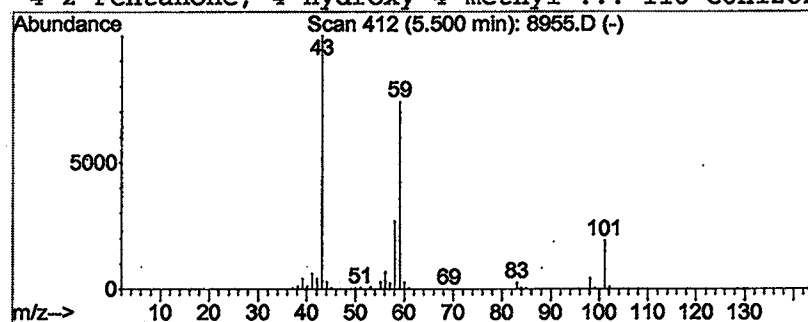

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 23 Apr 2002 12:16 am
 Data File: C:\MSDCHEM\1\DATA\042202\8955.D
 Name: SAMPLE 8955 4/15/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.50	16.1	ug/L	1106660	1	9.41	2754440	40.0