

Method 508 MOD.Date Extracted 4/15/02Page 60


Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
L.B.		500 ml		1 ml			1 ml	1B	7	
Ref 1					1 ml			4B		
Ref 2					1 ml			2B		
88 37	see 4/24							4A		
88 38	see 4/24							8B		
88 39								7A		
88 40	F.B.							8A		
89 30								7B		
89 31								2A		
89 32								6A		
89 33								2A		
89 34	see 4/24							1A		
89 35								1A		
Remarks										
Reviewed by: <u>C/S 8/16/02</u> drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type - <u>SEP. Fun.</u> Solv. lot# <u>X06E27</u> NaCl lot# <u>V39614</u> Na2SO4 lot# <u>V46648</u> STANDARD INT STD LOG# <u>APD 4/10/02</u> CALIBRATION <u>2193</u> REF SPIKE MDL/MDRF Q. CHECK INT. STD. <u>041902</u> SURROGATE LPC ENDRIN/DDT										

Analyst A.D.
revision 4/12/01Verified by myReviewed by DW
Date 4/26/02

DFTPP

Data File : C:\HPCHEM\1\DATA\APR2302\DFTPP.D
 Acq On : 23 Apr 2002 2:17 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

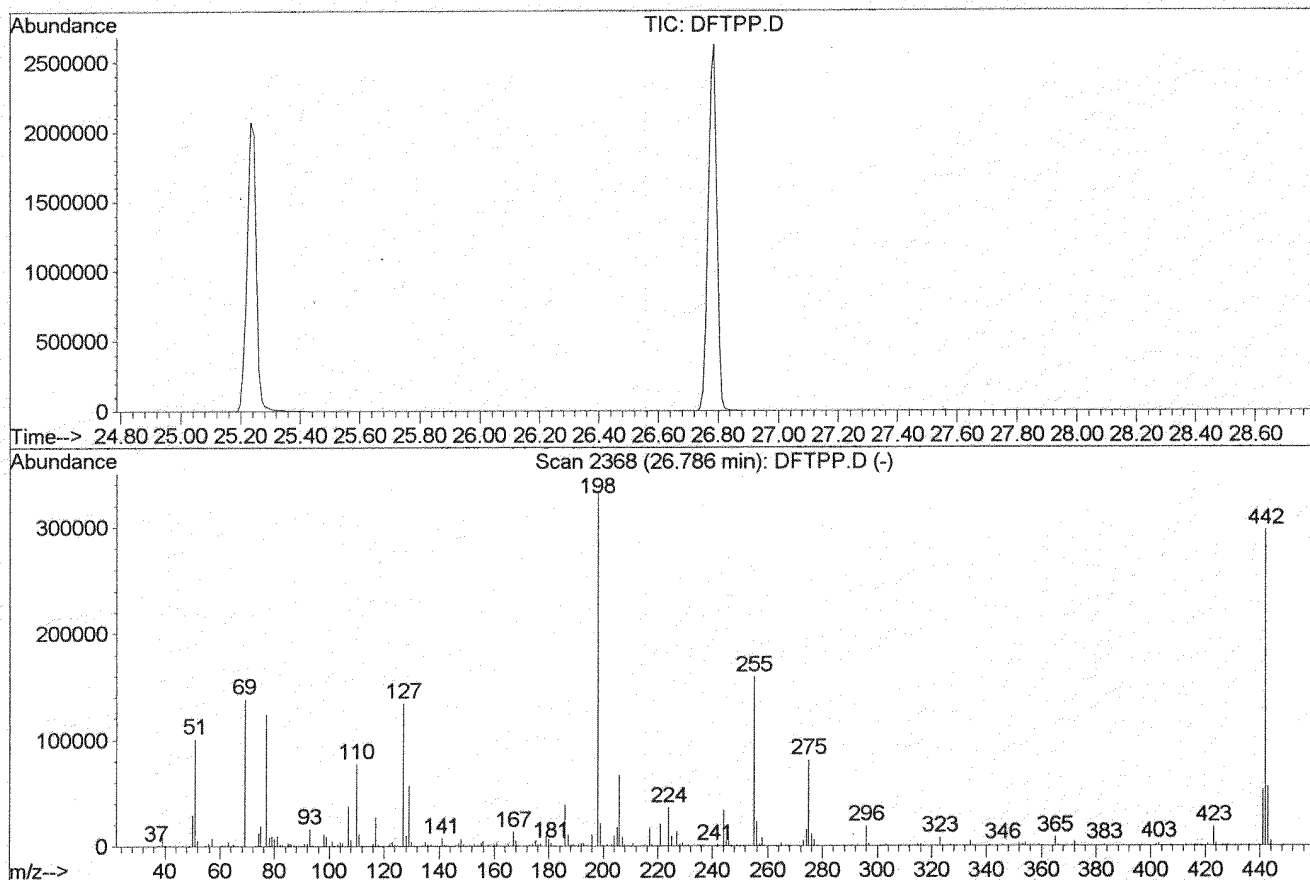

Spectrum Information: Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	30.4	101317	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.5	138404	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	40.3	134200	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	333384	PASS
199	198	5	9	6.4	21360	PASS
275	198	10	30	24.3	81132	PASS
365	198	1	100	2.5	8170	PASS
441	443	0.01	100	95.2	53491	PASS
442	198	40	110	89.0	296814	PASS
443	442	17	23	18.9	56175	PASS