

Method SD8 mod.

Date Extracted 1/3/02

Page 6

REF

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
LB		500ml		1ml			1ml	6B	7	
REF					0.5ml			7B		
31639								7A		
31631								6A		
31643								4A		
31585								5B		
31644								8B		
31673								4B		
31672								2A		
31671								3A		
31670								8A		
31638								3B		
31643										
31637								5A		

Remarks
Part #
GCMS-16526

Reviewed by
7/5/17/02

drip rate must be between 5-15 ml/min for liq-liq extractors
 Extraction type - SD8 Solv. lot# V39466 NaCl lot# V11599 Na2SO4 lot# V39400

STANDARD	INT STD LOG#
CALIBRATION	
REF/SPIKE	<u>91759</u>
MDL/MDRF	
Q. CHECK	
INT. STD.	
SURROGATE	<u>111901</u> <u>GCMS</u>
LPC	
ENDRIN/DDT	

Analyst [Signature]
 revision 4/12/01


Verified by _____

Reviewed by [Signature]
 Date 1/28/02

DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN17\0117DFT.D
 Acq On : 17 Jan 2002 8:30 am
 Sample : dftpp
 Misc : January 17, 2002
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

Vial: 1
 Operator:
 Inst : Instrume
 Multiplr: 1.00

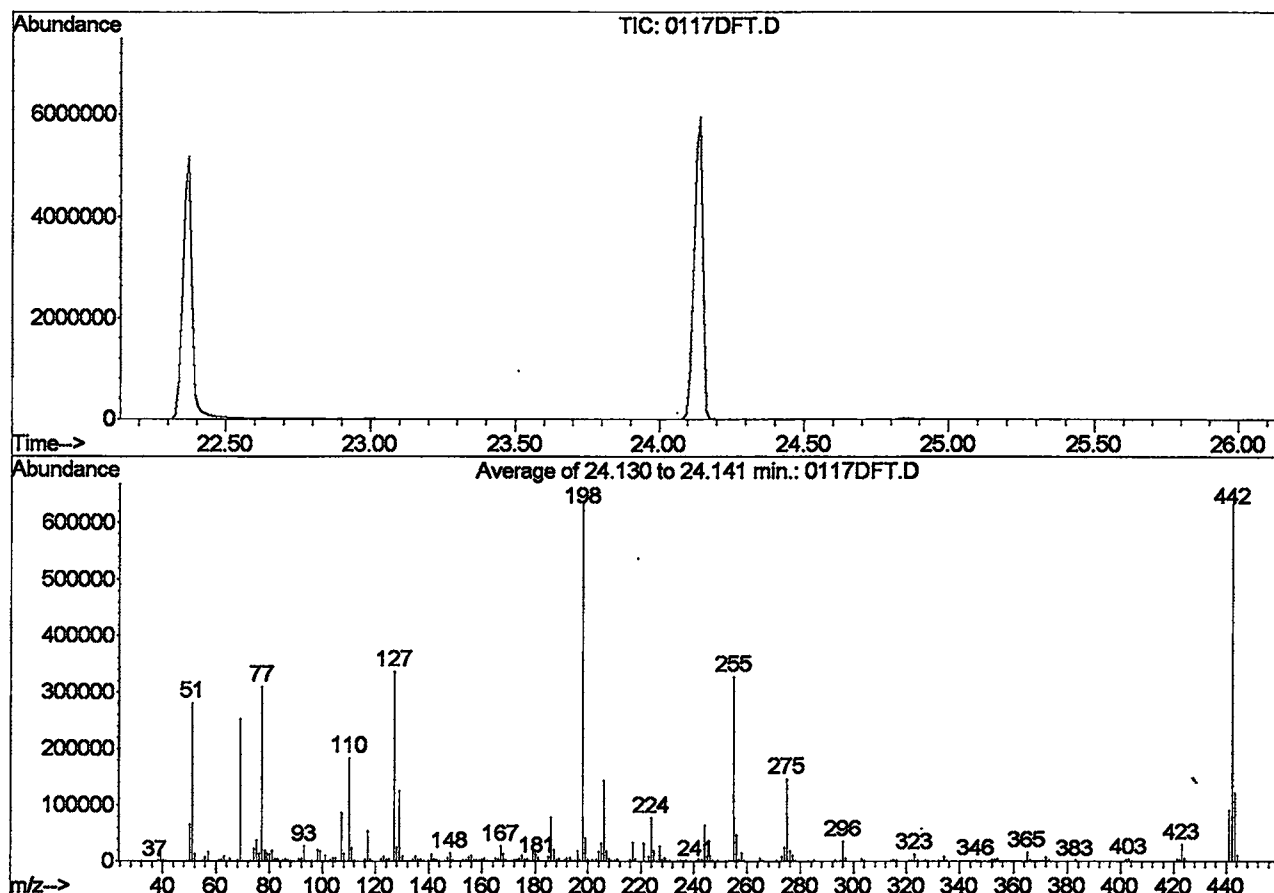

Spectrum Information: Average of 24.130 to 24.141 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.2	281984	PASS
68	69	0.00	2	0.9	2365	PASS
69	198	0.00	100	39.7	253184	PASS
70	69	0.00	2	0.6	1497	PASS
127	198	40	60	53.0	337600	PASS
197	198	0.00	1	0.3	2211	PASS
198	198	100	100	100.0	637568	PASS
199	198	5	9	6.7	42940	PASS
275	198	10	30	23.1	147296	PASS
365	198	1	99	2.7	17424	PASS
441	443	1	99	75.1	92668	PASS
442	198	40	110	99.5	634080	PASS
443	442	17	23	19.5	123464	PASS