

DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN23\0123DFT.D

Vial: 1

Acq On : 23 Jan 2002 11:01 am

Operator:

Sample : dftpp

Inst : Instrume


Misc : January 22, 2002

Multiplr: 1.00

MS Integration Params: SPLIT.P

Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)

Title : 508 scan method

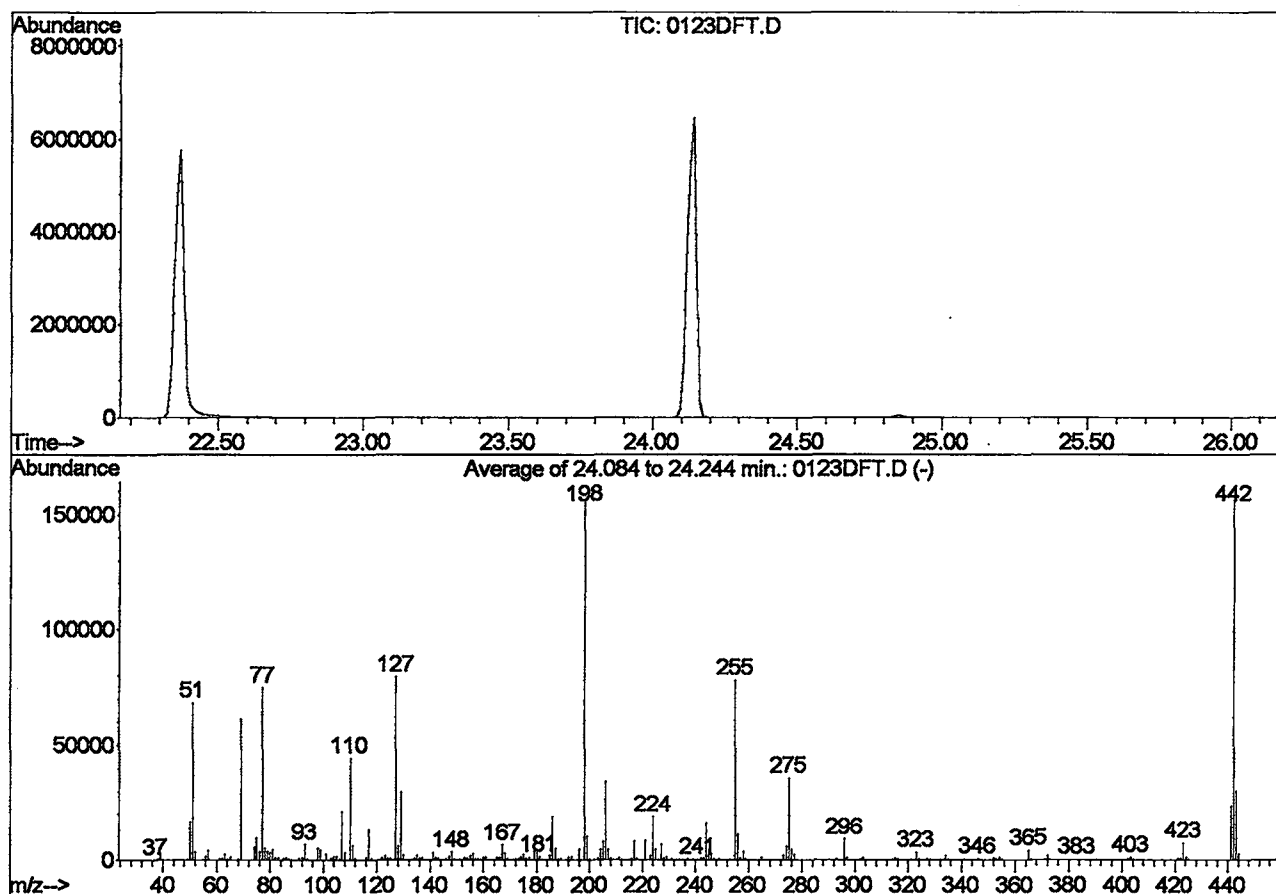

Spectrum Information: Average of 24.084 to 24.244 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	43.9	68251	PASS
68	69	0.00	2	0.9	540	PASS
69	198	0.00	100	39.6	61565	PASS
70	69	0.00	2	0.4	244	PASS
127	198	40	60	51.3	79703	PASS
197	198	0.00	1	0.2	319	PASS
198	198	100	100	100.0	155435	PASS
199	198	5	9	6.8	10585	PASS
275	198	10	30	23.2	36042	PASS
365	198	1	99	2.7	4142	PASS
441	443	1	99	77.9	23552	PASS
442	198	40	110	100.8	156616	PASS
443	442	17	23	19.3	30218	PASS

0123DFT.D SCAN508.M

Wed Jan 23 12:05:17 2002