


DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN24\0124DFT.D
 Acq On : 24 Jan 2002 9:08 am
 Sample : dftpp
 Misc : January 24, 2002
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

Vial: 1
 Operator:
 Inst : Instrume
 Multiplr: 1.00

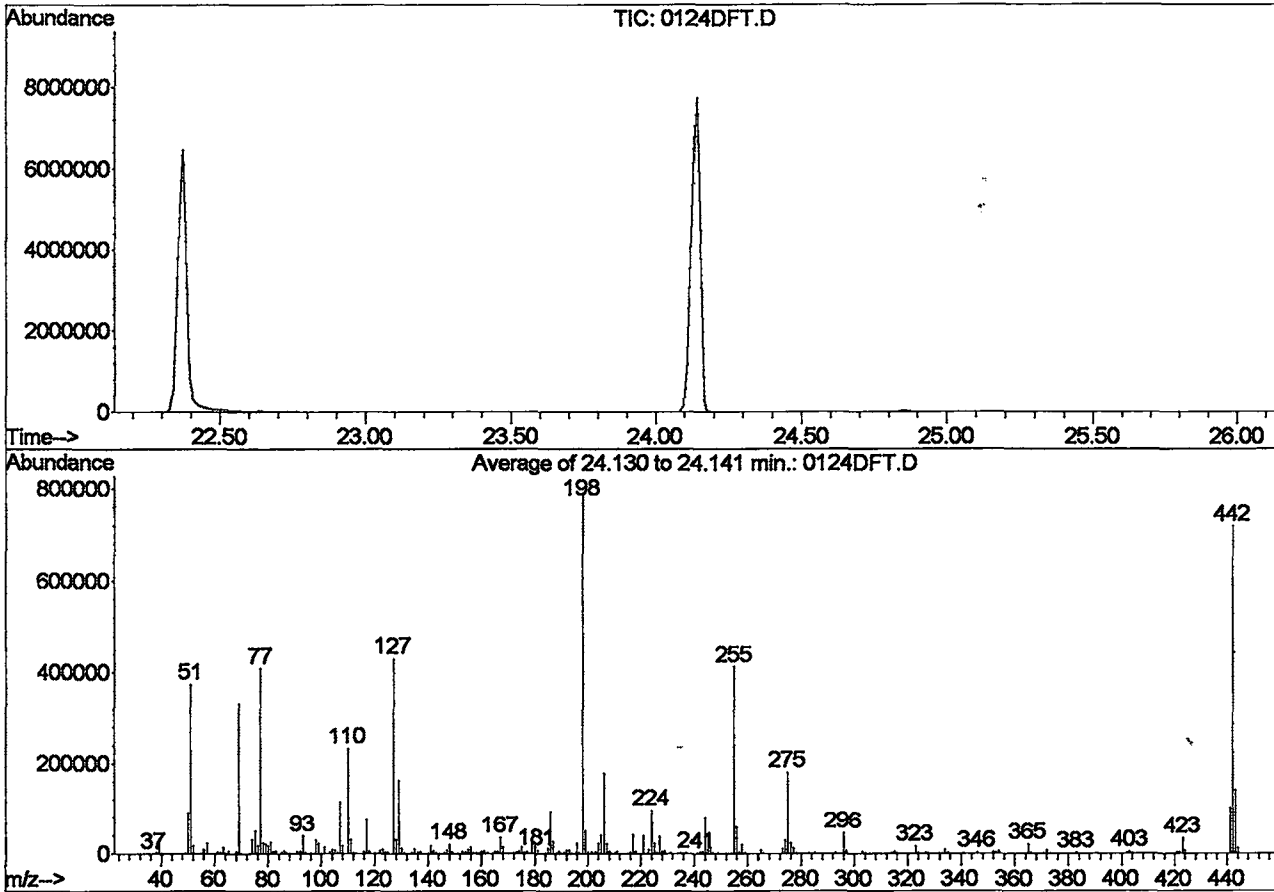

Spectrum Information: Average of 24.130 to 24.141 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	47.5	375360	PASS
68	69	0.00	2	1.7	5712	PASS
69	198	0.00	100	42.2	333056	PASS
70	69	0.00	2	0.5	1595	PASS
127	198	40	60	54.7	431808	PASS
197	198	0.00	1	0.4	3020	PASS
198	198	100	100	100.0	789408	PASS
199	198	5	9	6.6	51760	PASS
275	198	10	30	23.0	181888	PASS
365	198	1	99	2.7	20964	PASS
441	443	1	99	72.9	103244	PASS
442	198	40	110	91.0	718048	PASS
443	442	17	23	19.7	141720	PASS