

Method 508 mod.

Date Extracted 1/4/02

Page 11

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ml		1ml			1ml	7B	7			
REF					5ml			8B				
109 ✓								6A				
110 ✓								8A				
111 ✓								6B				
162 ✓								8A				
163 ✓								7A				
164 ✓								7B				
165 ✓								8B				
166 ✓								7A				

BATCH #
GCMS-16821

- BATCH INCLUDES ~~THE~~ CIRCLED NUMBERS ONLY.
ALL OTHERS FAILED DUE TO LOW SURROGATE RECOVERY
AND WILL BE RE-EXTRACTED & PLACED IN
OTHER BATCHES.

- LB ALSO HAD LOW SURROGATE RECOVERY

Remarks

Reviewed by
JLB 5/17/02

drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -

Extraction type Sepfun Solv. lot# V39466 NaCl lot# V11599 Na2SO4 lot# V39400

STANDARD	INT STD LOG#
CALIBRATION	
REF SPIKE	91759
MDL/MDRF	
Q. CHECK	
INT. STD.	
SURROGATE	GCMS 010302
LPC	
ENDRIN/DDT	

Analyst E. Heath
Revision 4/12/01

Verified by _____

Reviewed by DN
Date 2/13/02

DFTPP

Data File : C:\MSDCHEM\1\5973N\02FEB04\0204DF.D

Acq On : 4 Feb 2002 8:39 am

Sample : dftpp

Misc : February 4, 2002

MS Integration Params: SPLIT.P

Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)


Title : 508 scan method

Vial: 1

Operator:

Inst : Instrume

Multiplr: 1.00

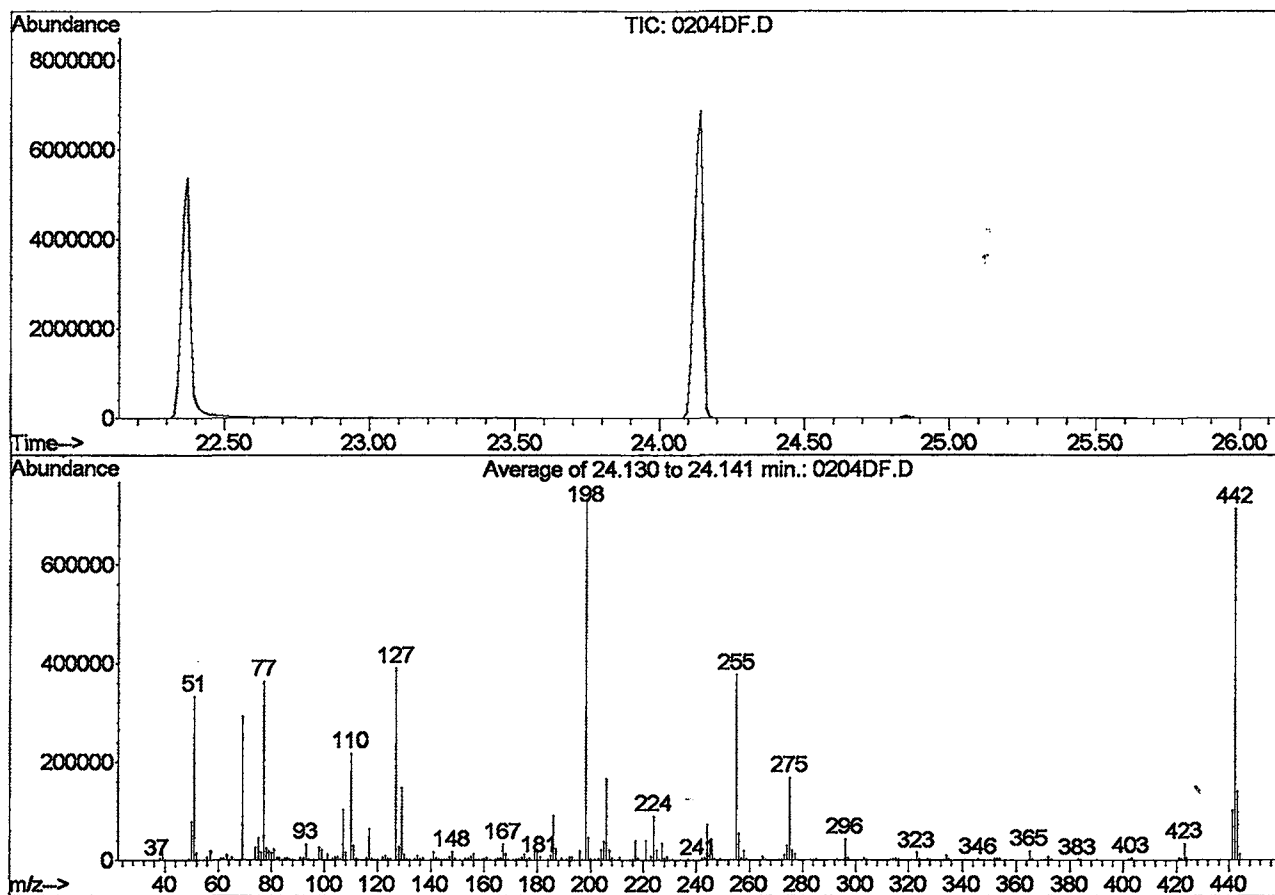

Spectrum Information: Average of 24.130 to 24.141 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	45.5	333568	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.2	294336	PASS
70	69	0.00	2	0.6	1806	PASS
127	198	40	60	53.4	391424	PASS
197	198	0.00	1	0.4	2640	PASS
198	198	100	100	100.0	732480	PASS
199	198	5	9	6.5	47884	PASS
275	198	10	30	23.2	169984	PASS
365	198	1	99	2.6	19396	PASS
441	443	1	99	73.6	103460	PASS
442	198	40	110	97.5	714080	PASS
443	442	17	23	19.7	140652	PASS

0204DF.D SCAN508.M

Mon Feb 04 09:55:01 2002