

Method 508 mod

Date Extracted 1/4/02

Page 8

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
LB		500 mL		1 mL			1 mL		7	
Ref					0.5 mL					
00003										
00004										
00027								1B		
00028								3A		
00029								2A		
00105								2B		
00106								1A		
00108										
BATCH # EGCMS-16829; INCLUDES ONLY THOSE LAB #'S THAT ARE CIRCLED. THE REMAINDER FAILED IN SURROGATE RECOVERY AND WILL BE RE-EXTRACTED & RE-BATCHED. LAB BLANK HAD LOW SURR. RECOVERY AS WELL, BUT HAD NO CONTAMINANTS OTHER THAN THOSE CAUSED BY THE EXTRACTION SOLVENTS										
(WB)										
Remarks										
Reviewed by LB 5/17/02										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type <u>sep fun</u> Solv. lot#										
NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39H00</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>91759</u>									
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE										
LPC										
ENDRIN/DDT										


Analyst LF
revision 4/12/01

Verified by _____

Reviewed by DN
Date 2/7/02

DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN25\0125DF.D Vial: 1
 Acq On : 25 Jan 2002 8:31 am Operator:
 Sample : dftpp Inst : Instrume
 Misc : January 25, 2002 Multiplr: 1.00
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

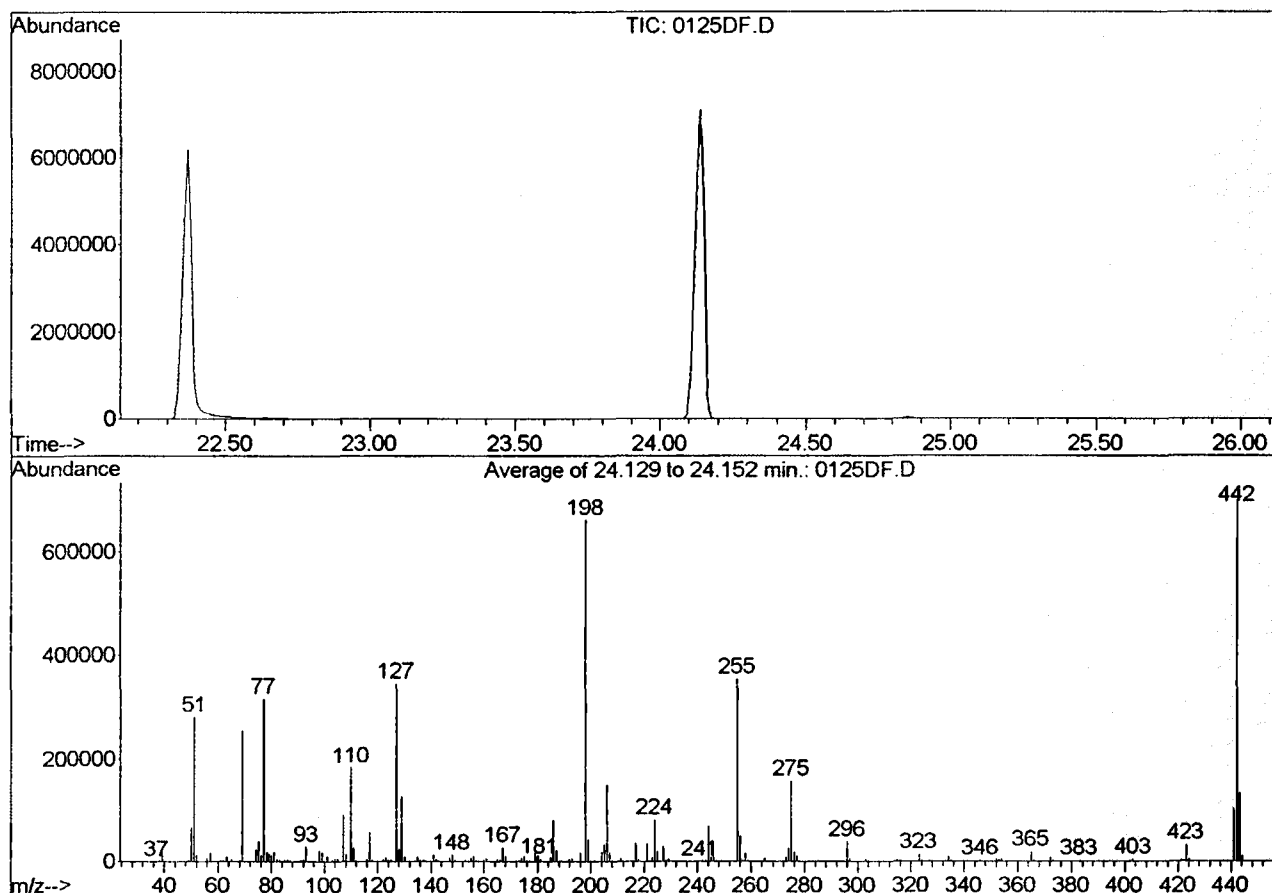

Spectrum Information: Average of 24.129 to 24.152 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.5	281408	PASS
68	69	0.00	2	1.0	2452	PASS
69	198	0.00	100	38.5	254720	PASS
70	69	0.00	2	0.6	1467	PASS
127	198	40	60	52.3	346005	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	661802	PASS
199	198	5	9	6.6	43874	PASS
275	198	10	30	23.8	157760	PASS
365	198	1	99	3.0	19670	PASS
441	443	1	99	77.8	103885	PASS
442	198	40	110	105.7	699520	PASS
443	442	17	23	19.1	133506	PASS

0125DF.D SCAN508.M Fri Jan 25 14:38:51 2002