

8 GCM8-16515

Method SDS mod.

Date Extracted 1/7/02

Page 13

REF

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
LB REF		500ml		1ml			1ml	4A	7	
310	FB				5ml			8A		
316								3B		
317								6B		
280								8B		
279								7B		
278								4B		
277								6A		
281								3A		
282	FB							8A		
								7A		
Remarks: ① BATCH # GCMS-16373 ② 277-310 analyzed on 1/9/02; 316 & 317 on 1/10/02 ③ Cal STD. corresponding to 316 & 317 has been added as a test to 316. drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type <i>sep fur</i> Solv. lot# <i>V39466</i> NaCl lot# <i>V11599</i> Na2SO4 lot# <i>V39 H00</i> STANDARD INT STD LOG# CALIBRATION REF SPIKE <i>91759</i> MDL/MDRF Q. CHECK INT. STD. SURROGATE <i>GCMS 010302</i> LPC ENDRIN/DDT Reviewed by, <i>CS 5/17/02</i>										


Analyst [Signature]
revision 4/12/01

Verified by

Reviewed by
Date

Data File : C:\MSDCHEM\1\5973N\02JAN09\0109DFT1.D
 Acq On : 9 Jan 2002 12:19 pm
 Sample : dftpp
 Misc : January 9, 2002
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

Vial: 1
 Operator:
 Inst : Instrume
 Multiplr: 1.00

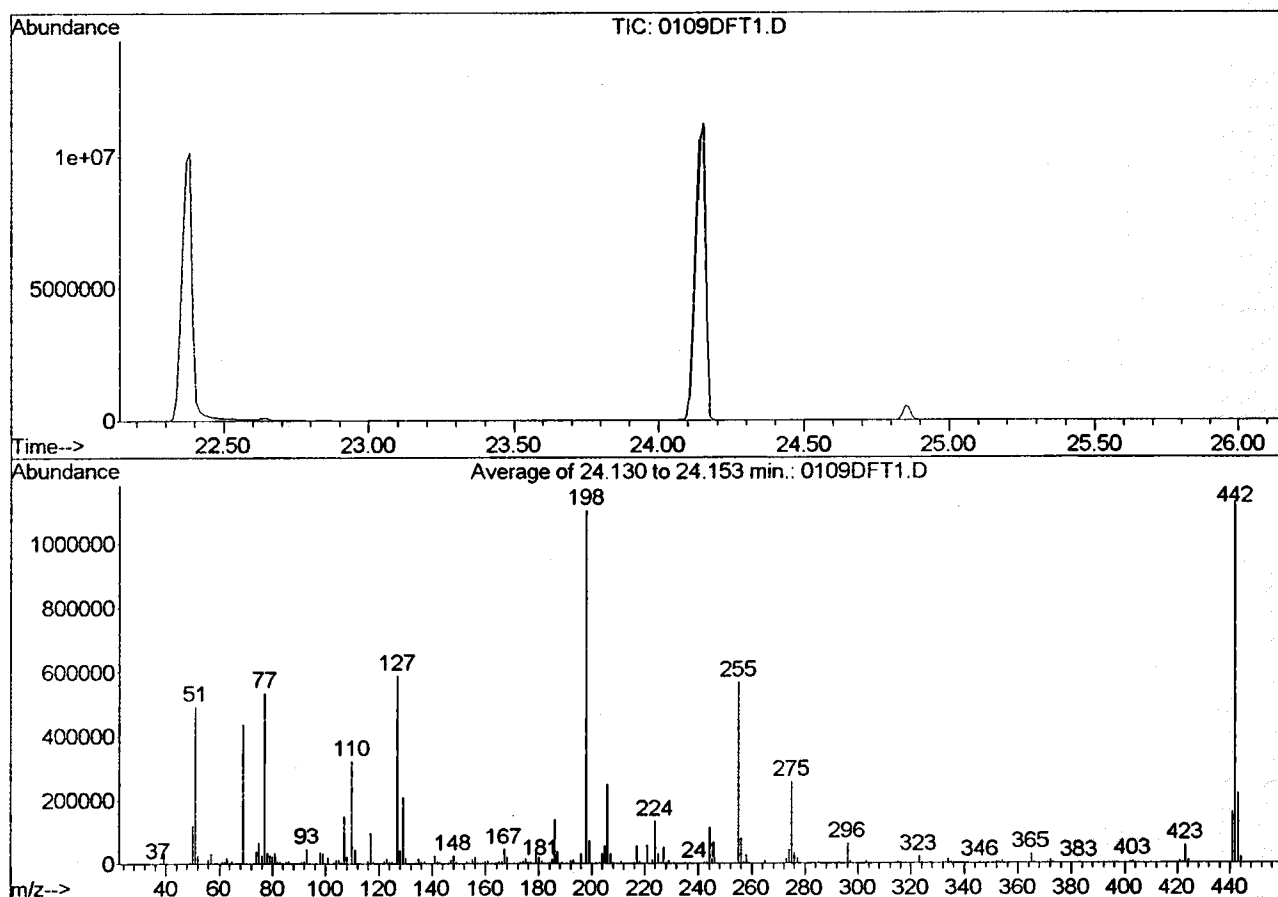


Spectrum Information: Average of 24.130 to 24.153 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.7	493312	PASS
68	69	0.00	2	0.5	2058	PASS
69	198	0.00	100	39.6	437546	PASS
70	69	0.00	2	0.4	1883	PASS
127	198	40	60	53.4	589738	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	1104512	PASS
199	198	5	9	6.7	73792	PASS
275	198	10	30	23.3	257237	PASS
365	198	1	99	2.7	30026	PASS
441	443	1	99	73.2	162416	PASS
442	198	40	110	102.3	1129770	PASS
443	442	17	23	19.6	221866	PASS

0109DFT1.D SCAN508.M Thu Jan 10 08:36:38 2002

Data File : C:\MSDCHEM\1\5973N\02JAN10\0110DFT1.D
 Acq On : 10 Jan 2002 8:24 am
 Sample : dftpp
 Misc : January 10, 2002
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

Vial: 1
 Operator:
 Inst : Instrume
 Multiplr: 1.00

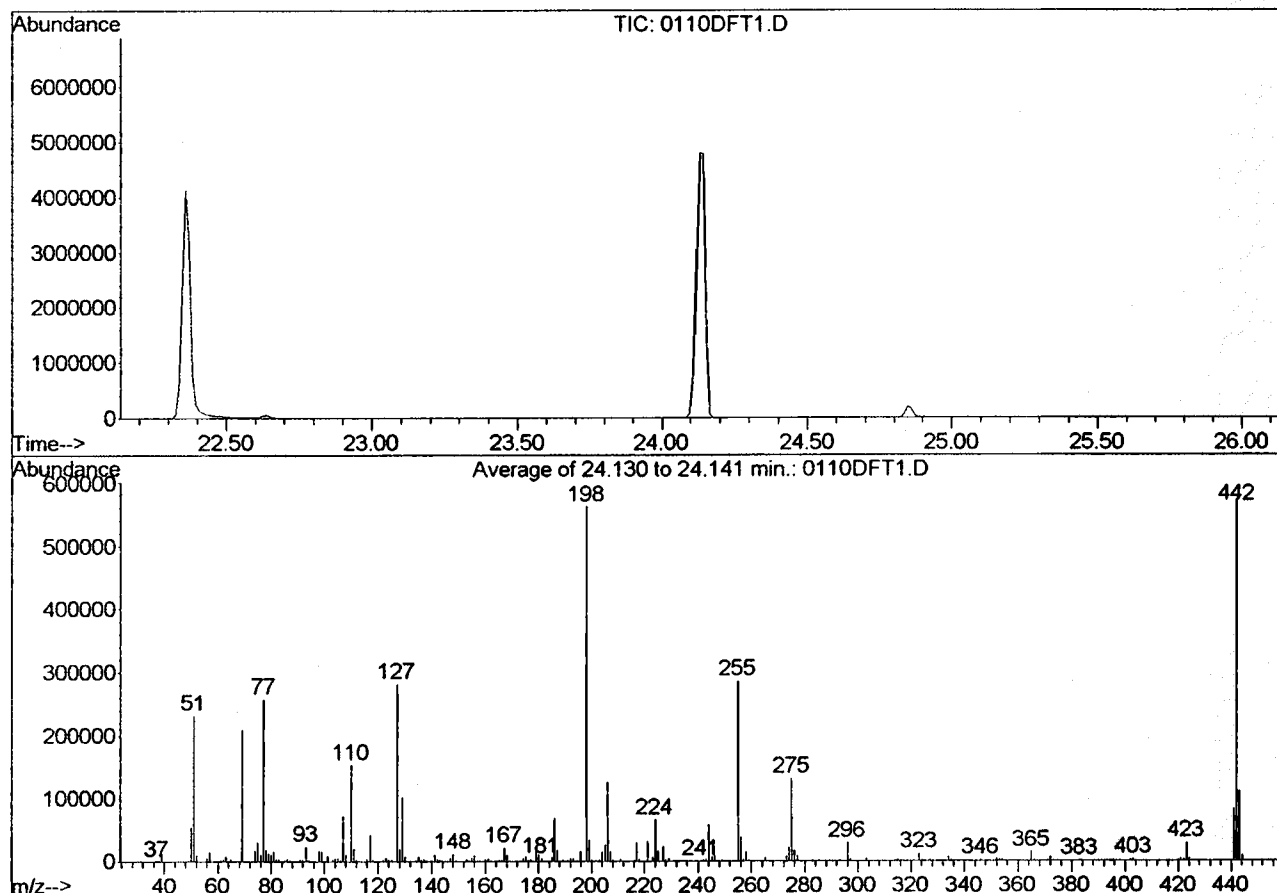

Spectrum Information: Average of 24.130 to 24.141 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.2	232128	PASS
68	69	0.00	2	0.7	1533	PASS
69	198	0.00	100	37.3	210080	PASS
70	69	0.00	2	0.5	1110	PASS
127	198	40	60	50.1	282368	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	563744	PASS
199	198	5	9	6.3	35704	PASS
275	198	10	30	23.5	132228	PASS
365	198	1	99	2.7	15050	PASS
441	443	1	99	74.2	82704	PASS
442	198	40	110	101.7	573344	PASS
443	442	17	23	19.4	111484	PASS

0110DFT1.D SCAN508.M

Thu Jan 10 11:46:11 2002