

Method 508 mod

Date Extracted 1/7/02

Page 14

ref ref

Lab #	Description	Sample vol/wt	Drip rate ml/min	Sytr add	Spr add	IS add	Final vol.	T.V. pos.	pH	Count
LB		500ml		1ml			1ml	10A	7	
Ref	2				0.5ml			10B		
00318								9A		
00319								9B		
00320								8B		
00307								2B		
00308								1B		
00276								2A		
00275								5A		
00309								1A		
Remarks BATCH# SGCMS-16355 Reviewed by, <u>CB</u> 5/18/02 drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type - <u>sep-fun</u> Solv.lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V391700</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	91759									
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	010302									
LPC										
ENDRIN/DDT										

Analyst LF
revision 4/12/01


Verified by _____

Reviewed by DN
Date 1/10/02

DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN08\0108DFT1.D
 Acq On : 8 Jan 2002 8:40 am
 Sample : dftpp
 Misc : January 8, 2002
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

Vial: 1
 Operator:
 Inst : Instrume
 Multiplr: 1.00

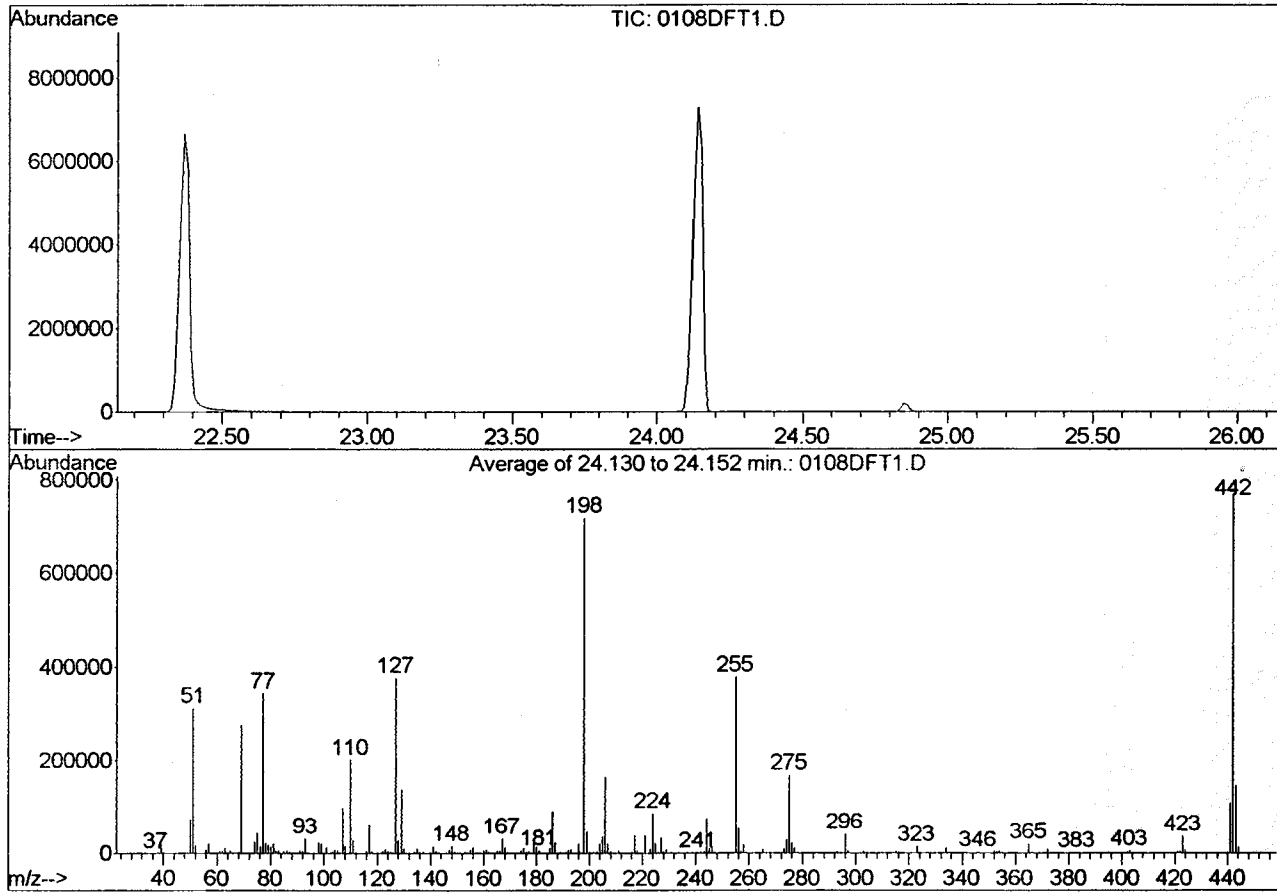

Spectrum Information: Average of 24.130 to 24.152 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	43.5	312960	PASS
68	69	0.00	2	1.2	3251	PASS
69	198	0.00	100	38.5	276821	PASS
70	69	0.00	2	0.5	1375	PASS
127	198	40	60	52.4	377002	PASS
197	198	0.00	1	0.2	1450	PASS
198	198	100	100	100.0	718826	PASS
199	198	5	9	6.6	47282	PASS
275	198	10	30	23.7	170218	PASS
365	198	1	99	3.0	21421	PASS
441	443	1	99	74.5	110994	PASS
442	198	40	110	107.0	769301	PASS
443	442	17	23	19.4	148912	PASS

0108DFT1.D SCAN508.M Tue Jan 08 09:53:30 2002