


DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN11\0111DFT.D Vial: 1
 Acq On : 11 Jan 2002 8:47 am Operator:
 Sample : dftpp Inst : Instrume
 Misc : January 11, 2002 Multiplr: 1.00
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

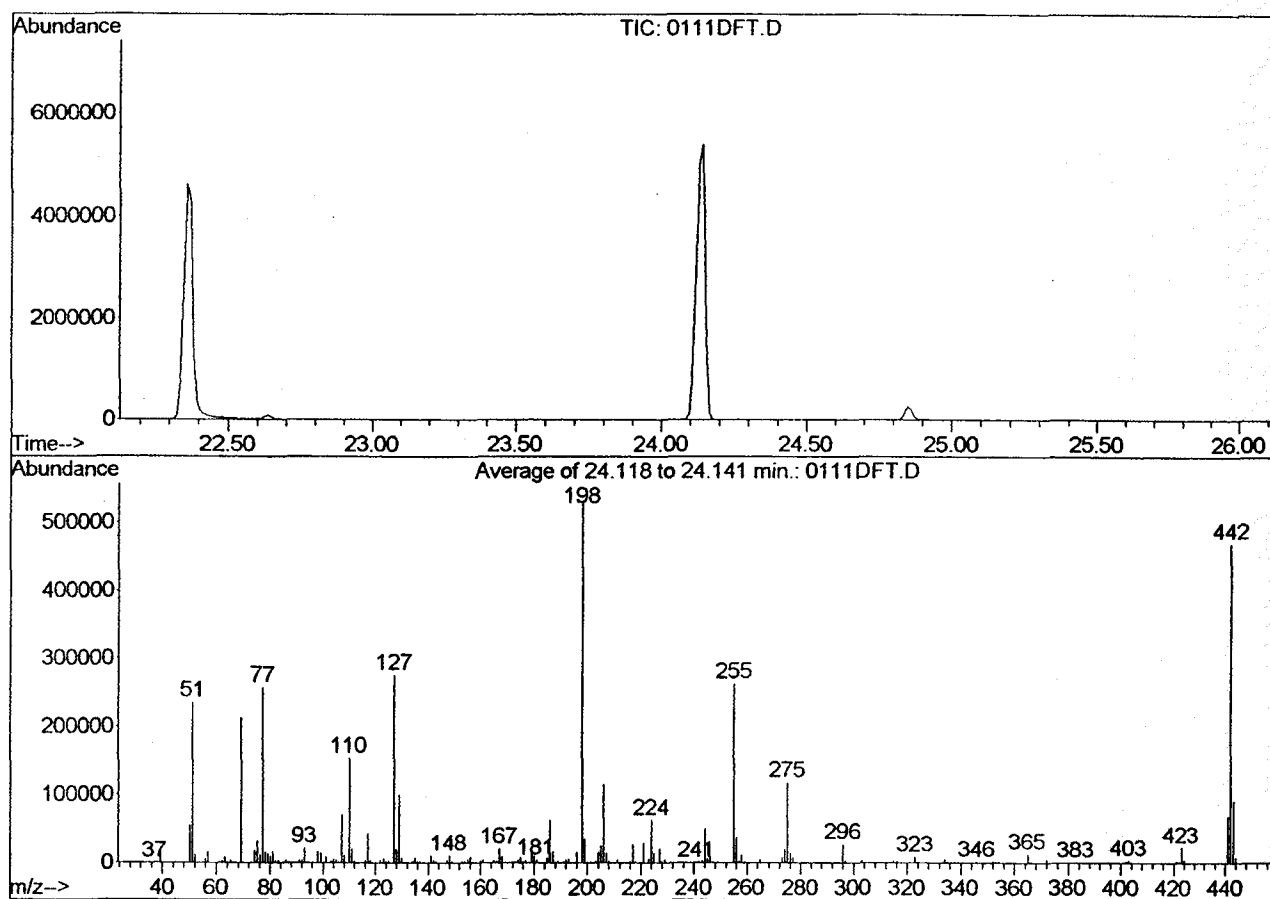


Spectrum Information: Average of 24.118 to 24.141 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.3	235690	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.1	212949	PASS
70	69	0.00	2	0.5	1008	PASS
127	198	40	60	52.0	276608	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	531498	PASS
199	198	5	9	6.8	35986	PASS
275	198	10	30	22.3	118528	PASS
365	198	1	99	2.5	13178	PASS
441	443	1	99	74.6	68874	PASS
442	198	40	110	88.4	470037	PASS
443	442	17	23	19.6	92320	PASS

0111DFT.D SCAN508.M Mon Jan 14 10:31:34 2002

DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN14\0114DFT.D Vial: 1
 Acq On : 14 Jan 2002 8:39 am Operator:
 Sample : dftpp Inst : Instrume
 Misc : January 14, 2002 Multiplr: 1.00
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

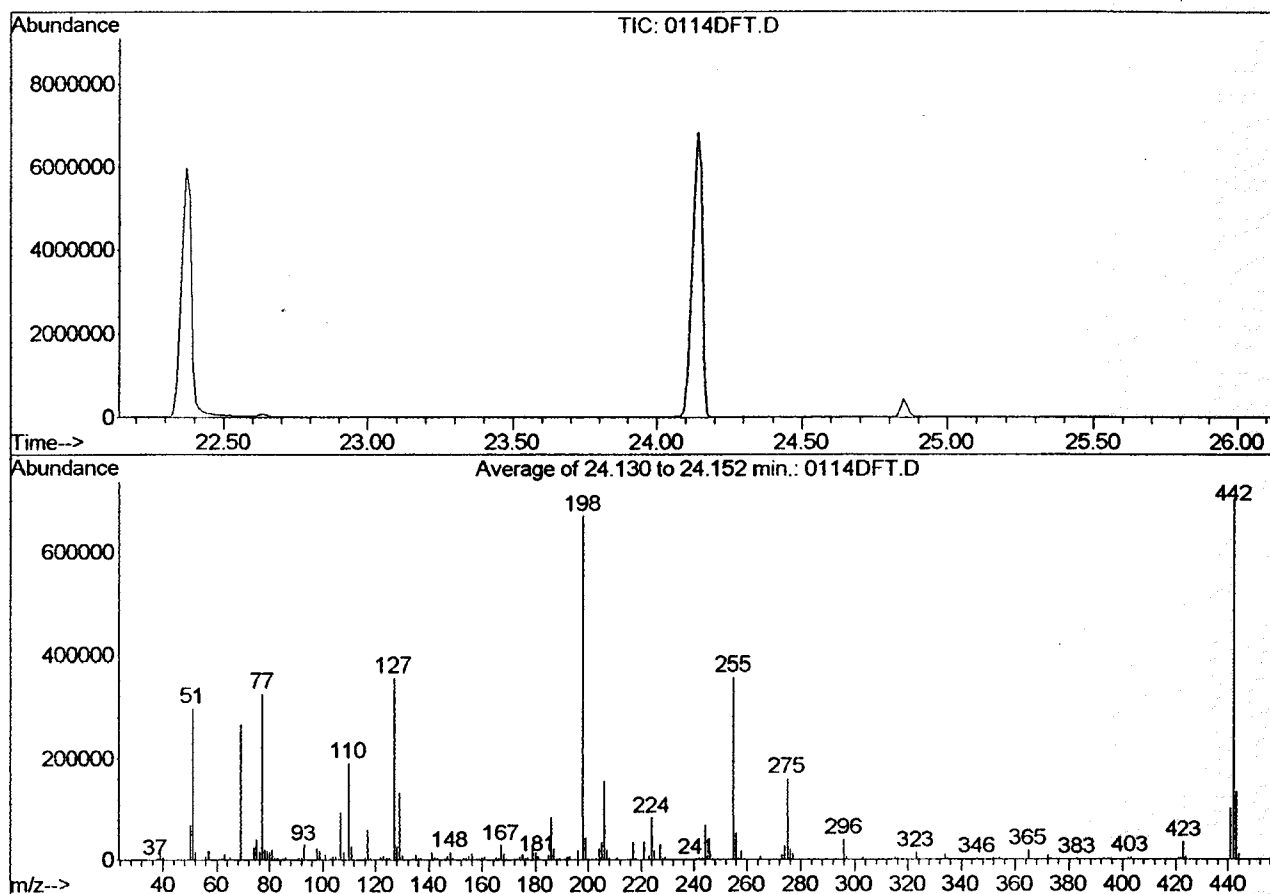

Spectrum Information: Average of 24.130 to 24.152 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.3	297365	PASS
68	69	0.00	2	0.7	1883	PASS
69	198	0.00	100	39.6	266346	PASS
70	69	0.00	2	0.5	1439	PASS
127	198	40	60	53.0	356352	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	671765	PASS
199	198	5	9	6.6	44496	PASS
275	198	10	30	24.0	161322	PASS
365	198	1	99	2.9	19700	PASS
441	443	1	99	76.3	103517	PASS
442	198	40	110	104.9	704981	PASS
443	442	17	23	19.2	135661	PASS

0114DFT.D SCAN508.M Mon Jan 14 11:33:30 2002