

Method 508 MOD.

Date Extracted 1-9-02

Page 17

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Surr add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500 ml		1 ml			1 ml	5A	7			
Ref.					0.5 ml			5B				
610 F.B. → F.B.								4A				
613								4B				
614								3A				
556								3B				
555								2A				
615								2B				
562 F.B. → F.B.								1A				
Remarks												
BATCH # GEMS - 16689 (0055)												
Reviewed by JB 5/08/02												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - <u>sep. fun.</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39H00</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	91759											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	GEMS 010302											
LPC												
ENDRIN/DDT												

Analyst A.D.
revision 4/12/01

Verified by _____

Reviewed by [Signature]
Date 2/11/02

DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN29\0129DF.D

Vial: 1

Acq On : 29 Jan 2002 8:26 am

Operator:

Sample : dftpp

Inst : Instrume


Misc : January 29, 2002

Multiplr: 1.00

MS Integration Params: SPLIT.P

Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)

Title : 508 scan method

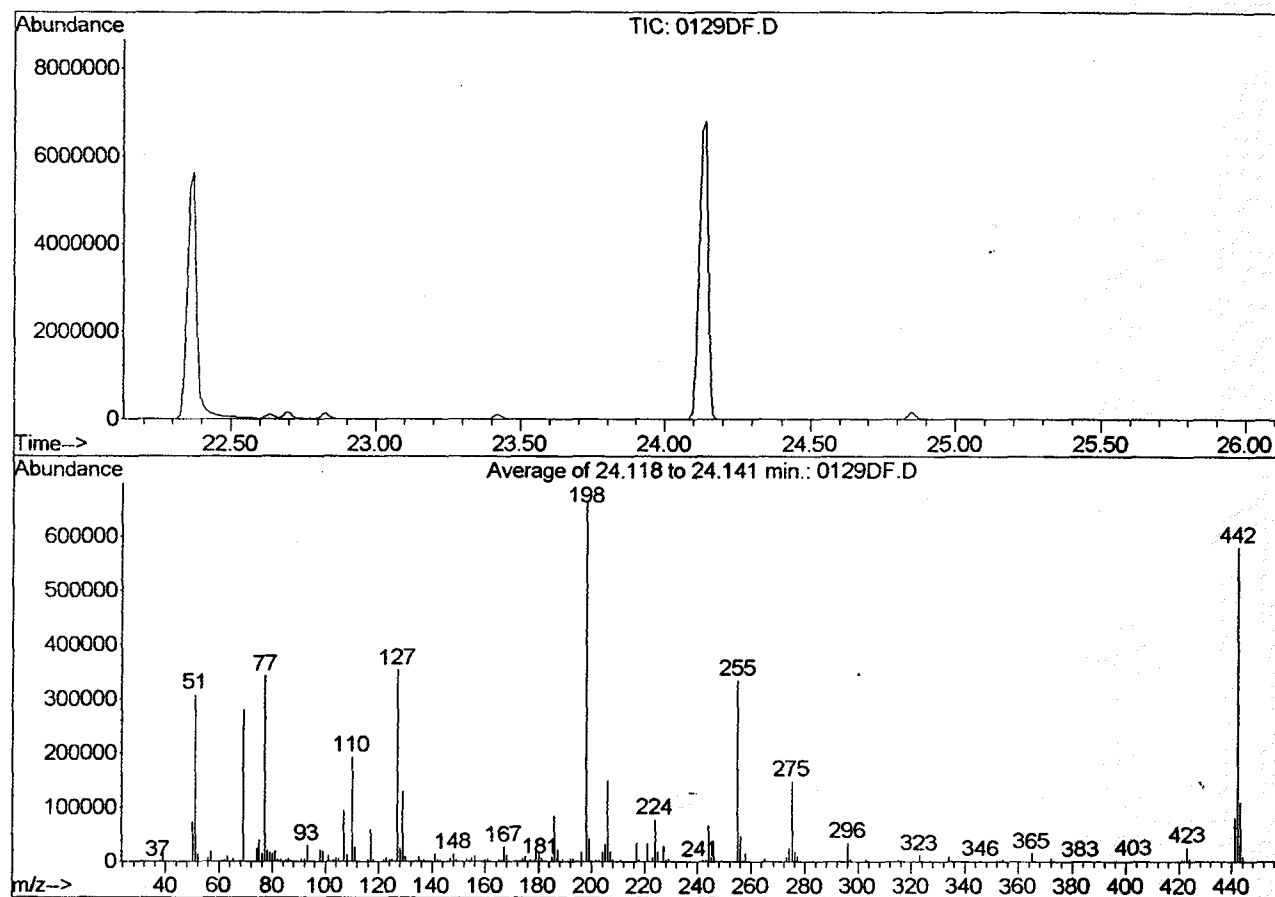

Spectrum Information: Average of 24.118 to 24.141 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	46.3	308224	PASS
68	69	0.00	2	1.0	2747	PASS
69	198	0.00	100	42.1	280512	PASS
70	69	0.00	2	0.5	1369	PASS
127	198	40	60	53.1	353578	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	665877	PASS
199	198	5	9	6.6	44080	PASS
275	198	10	30	22.4	149336	PASS
365	198	1	99	2.6	17293	PASS
441	443	1	99	73.7	82834	PASS
442	198	40	110	87.3	581525	PASS
443	442	17	23	19.3	112432	PASS

0129DF.D SCAN508.M

Tue Jan 29 10:10:52 2002