


Reviewed by
Date 11/7/2

0115

Data File : C:\MSDCHEM\1\5973N\02JAN15\0115DFT.D
Acq On : 15 Jan 2002 8:32 am
Sample : dftpp
Misc : January 15, 2002
MS Integration Params: SPLIT.P
Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
Title : 508 scan method

Vial: 1
Operator:
Inst : Instrume
Multiplr: 1.00

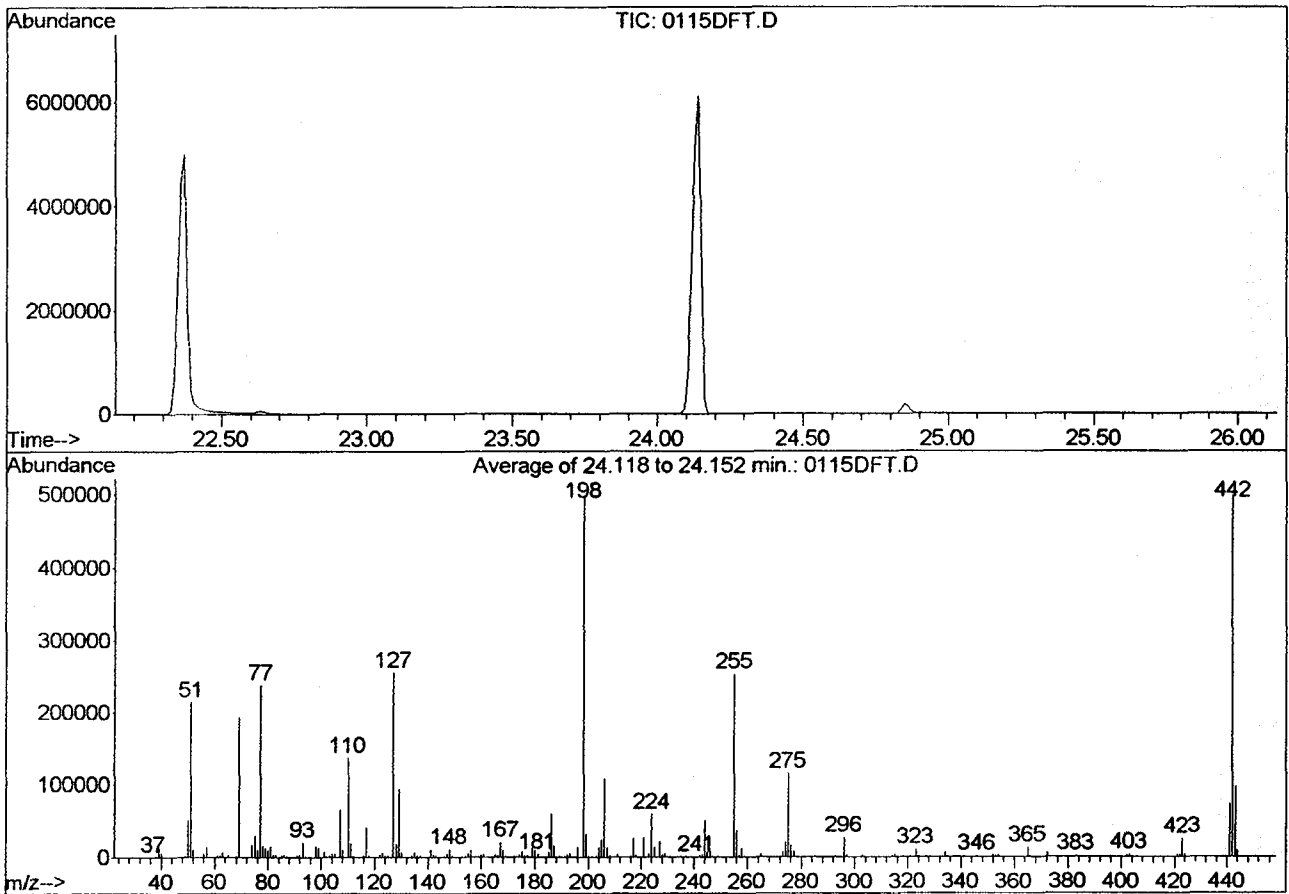

Spectrum Information: Average of 24.118 to 24.152 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	43.2	214424	PASS
68	69	0.00	2	0.9	1654	PASS
69	198	0.00	100	38.9	193004	PASS
70	69	0.00	2	0.4	795	PASS
127	198	40	60	51.6	255888	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	495968	PASS
199	198	5	9	6.5	32476	PASS
275	198	10	30	23.4	115832	PASS
365	198	1	99	2.7	13171	PASS
441	443	1	99	74.4	72670	PASS
442	198	40	110	100.4	498112	PASS
443	442	17	23	19.6	97652	PASS