

Method 508 mod.

Date Extracted 1-11-02

Page 23

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	Next
LB		500ml		1ml			1ml	2A	7		
REF					5ml			5B			
830	see 1/15							3A			✓
831								1A			
832								4A			
833								6A			
838								3B			
839								4B			
840								6B			
843	see 1/15							5A			✓
845								1B			
BATCH # <u>GCMS-16718</u>											
Remarks: Samples # 830, 831 + 832 were yellowish in color due to the glasswares that were used from a soil extraction before. Lab blank dried out on the Turbo Vap.											
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -											
Extraction type <u>Sip</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39400</u>											
STANDARD	INT STD LOG#										
CALIBRATION											
REF SPIKE	91759										
MDL/MDRF											
Q. CHECK											
INT. STD.											
SURROGATE	GCMS	010302									
LPC											
ENDRIN/DDT											


Analyst OH
revision 4/12/01

Verified by _____

Reviewed by DN
Date 2/4/2

DFTPP

Data File : C:\MSDCHEM\1\5973N\02JAN31\0131DF.D Vial: 1
 Acq On : 31 Jan 2002 8:43 am Operator:
 Sample : dftpp Inst : Instrume
 Misc : January 31, 2002 Multiplr: 1.00
 MS Integration Params: SPLIT.P
 Method : C:\MSDCHEM\1\METHODS\METHODS\SCAN508.M (RTE Integrator)
 Title : 508 scan method

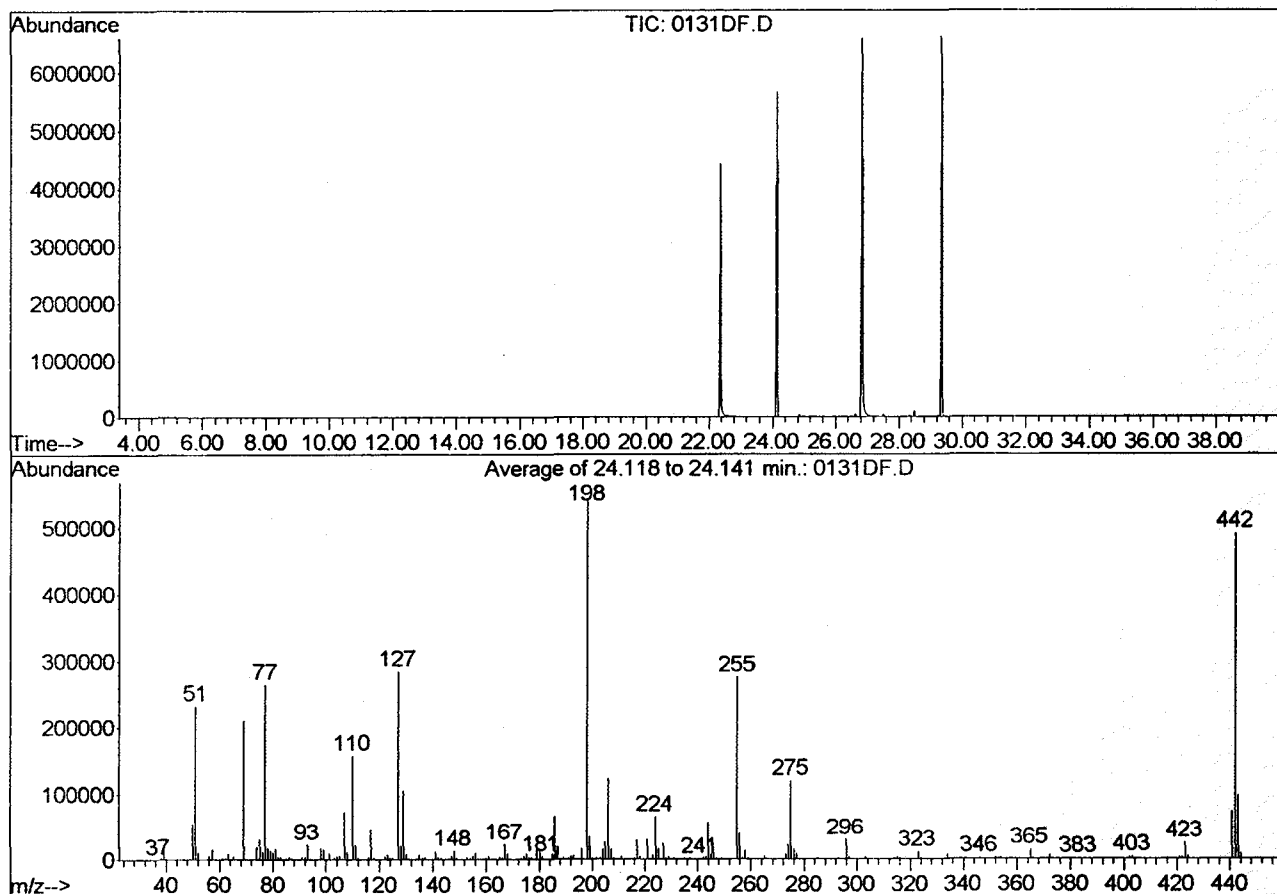

Spectrum Information: Average of 24.118 to 24.141 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	43.0	232874	PASS
68	69	0.00	2	0.5	1134	PASS
69	198	0.00	100	38.9	210858	PASS
70	69	0.00	2	0.5	1132	PASS
127	198	40	60	52.6	285184	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	541824	PASS
199	198	5	9	6.5	35112	PASS
275	198	10	30	22.1	119605	PASS
365	198	1	99	2.6	14278	PASS
441	443	1	99	75.7	73469	PASS
442	198	40	110	90.6	490858	PASS
443	442	17	23	19.8	97093	PASS

0131DF.D SCAN508.M Thu Jan 31 10:19:40 2002