

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 03/14/2002 Time: 15:49:29

Sample: AE04243
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 3/14/02 15:35 Ended: 3/14/02 15:35 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		111		5.0

Comments for Sample AE04243 - Analysis \$GCMS

Westchester Dept. of Labs & Research
User: Vinci, David L
Date: 03-14-2002 Time: 15:49:34

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was below its acceptance range.

Data File : C:\MSDCHEM\1\DATA\022802\04243.D

Vial: 11

Acq On : 28 Feb 2002 7:10 pm

Operator: McLean

Sample : GC MS SCAN 2/27

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 13 11:11:54 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	150	1144812	20.00	ug/L	0.00
10) Naphthalene-d8	13.05	136	2998789	20.00	ug/L	0.00
17) Acenaphthene-d10	18.16	164	1677829	20.00	ug/L	0.00
29) Phenanthrene-d10	22.52	188	2575618	20.00	ug/L	0.00
38) Chrysene-d12	30.33	240	2428633	20.00	ug/L	-0.03
44) Perylene-d12	34.21	264	1589513	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-ddd surr	27.46	235	227210	5.56	ug/L	0.00
Spiked Amount	5.000		Recovery	= 111.20%		

Target Compounds

						Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2 ' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	24.67	149	4149	0.02	ug/L	79
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo (a) anthracene	30.34	228	6253	0.04	ug/L	53
42) Bis (2-ethylhexyl) phthala	30.94	149	20276	0.18	ug/L	84
43) Chrysene	0.00	228	0	N.D.	d	
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo (b) fluoranthene	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

04243.D 5080202.M Wed Mar 13 11:12:46 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\022802\04243.D Vial: 11
 Acq On : 28 Feb 2002 7:10 pm Operator: McLean
 Sample : GC MS SCAN 2/27 Inst : Instrumen
 Misc : Multiplr: 1.00
 MS Integration Params: BENZO.P
 Quant Time: Mar 13 11:11:54 2002 Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Last Update : Mon Feb 25 19:17:14 2002
 Response via : Initial Calibration
 DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration
 04243.D 5080202.M Wed Mar 13 11:12:46 2002

Data File : C:\MSDCHEM\1\DATA\022802\04243.D

Vial: 11

Acq On : 28 Feb 2002 7:10 pm

Operator: McLean

Sample : GC MS SCAN 2/27

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 13 11:12 2002


Quant Results File: 5080202.RES

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

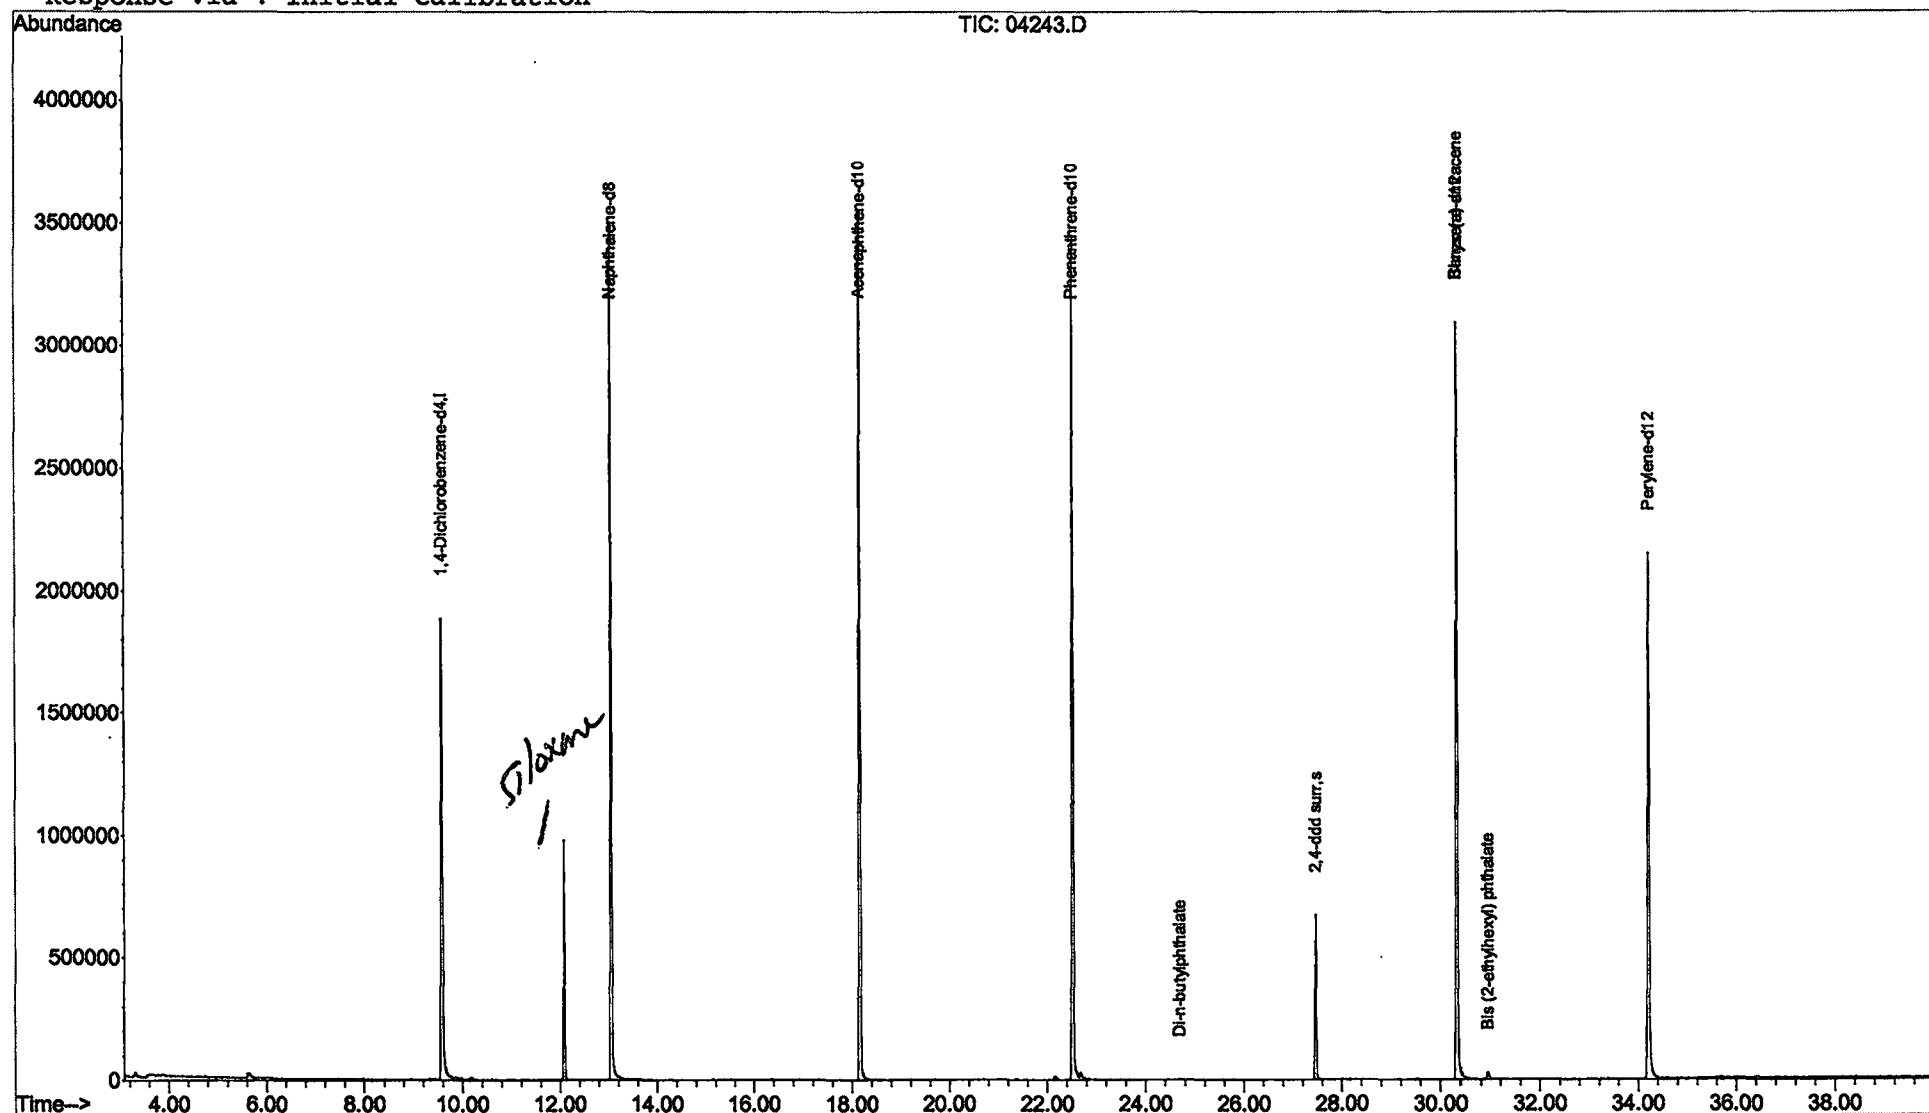

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\022802\04243.D

Vial: 11

Acq On : 28 Feb 2002 7:10 pm

Operator: McLean

Sample : GC MS SCAN 2/27

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.579	711	717	732	rBV	1885715	4738143	66.57%	11.700%
2	12.083	988	993	999	rBV	980381	1640906	23.06%	4.052%
3	13.053	1095	1100	1123	rBV	3478816	6474133	90.97%	15.987%
4	18.160	1657	1663	1678	rBV	3549132	6979413	98.07%	17.235%
5	22.523	2138	2144	2156	rBV2	3446417	7117039	100.00%	17.574%
6	27.457	2683	2688	2697	rBB	672426	1212092	17.03%	2.993%
7	30.332	2998	3005	3023	rBV2	3093422	7032741	98.82%	17.366%
8	30.940	3065	3072	3083	rBV2	29080	80466	1.13%	0.199%
9	34.214	3425	3433	3456	rBV	2150331	5221756	73.37%	12.894%

Sum of corrected areas: 40496689

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\022802\04243.D
Operator : McLean
Acquired : 28 Feb 2002 7:10 pm using AcqMethod 508SCAN
Instrument : Instrumen
Sample Name: GC MS SCAN 2/27
Misc Info :
Vial Number: 11
Quant File :5080202.RES (RTE Integrator)

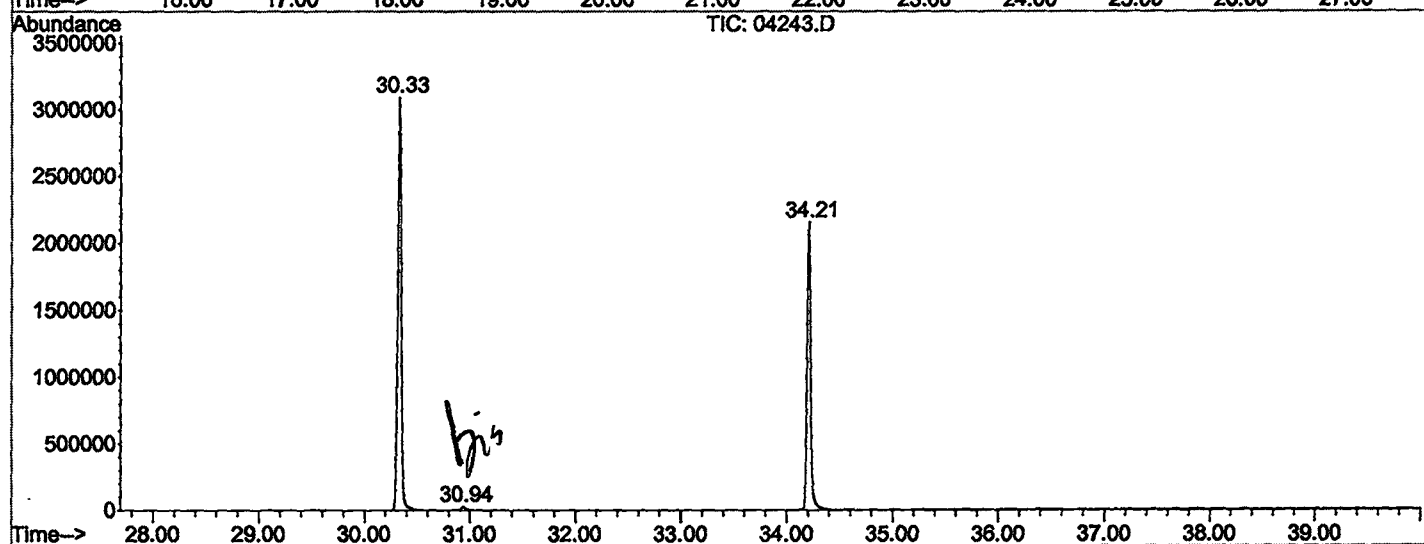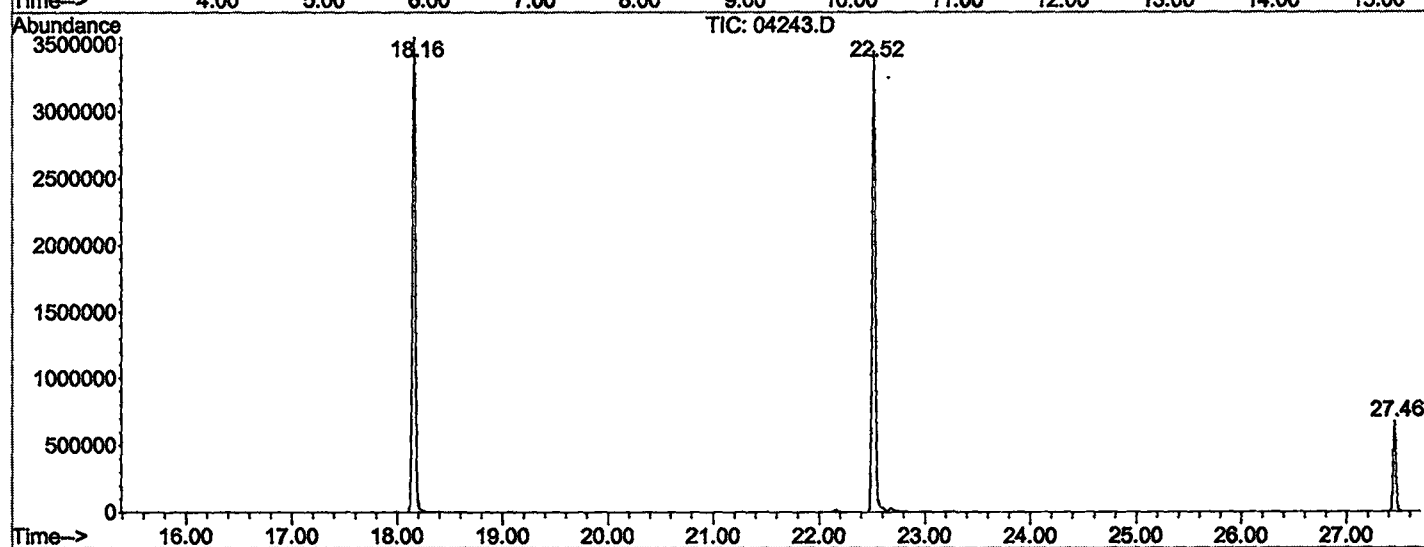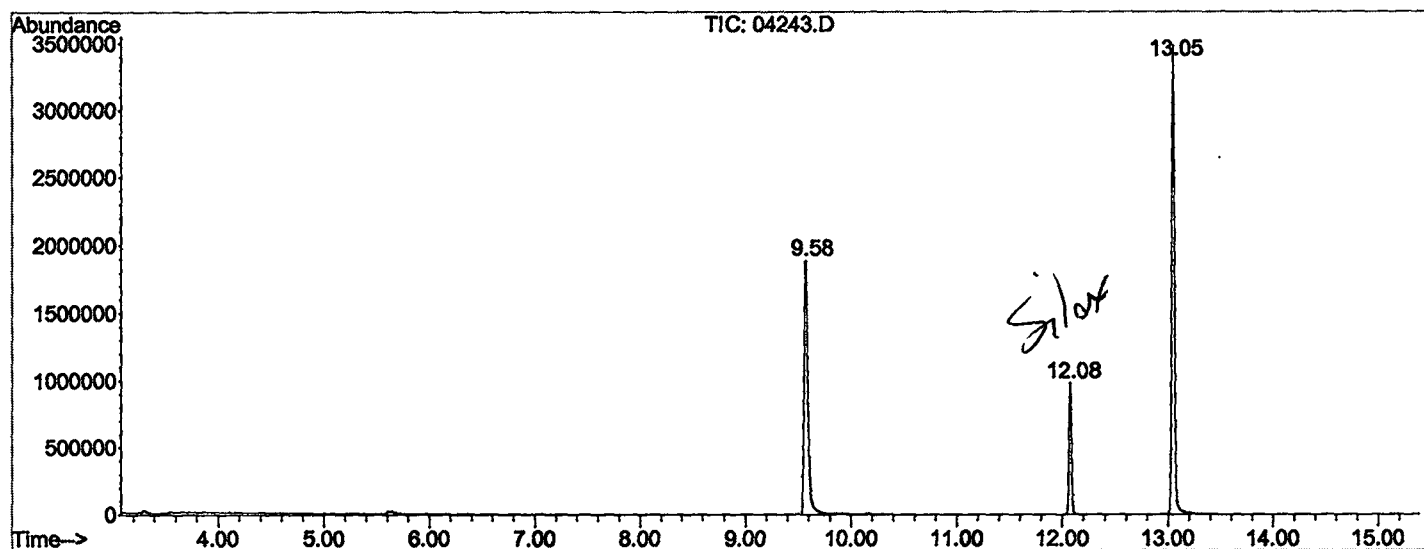

Data File : C:\MSDCHEM\1\DATA\022802\04243.D
 Acq On : 28 Feb 2002 7:10 pm
 Sample : GC MS SCAN 2/27
 Misc :
 MS Integration Params: LSCINT.P










Vial: 11
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Library : C:\DATABASE\WILEY7N.L

 Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.08	5.07 ug/L	1640910	Naphthalene-d8	13.05

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	62
2	Benzoic acid, 2-[(trimethylsilyl)oxy]-, trimethyl...	282	C13H22O3Si2	003789-85-3	47
3	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	46
4	N-(Trifluoroacetyl)-N,O,O',O'-t...	553	C22H42F3NO4Si4	000000-00-0	32

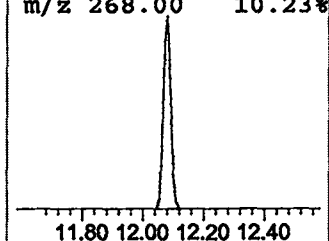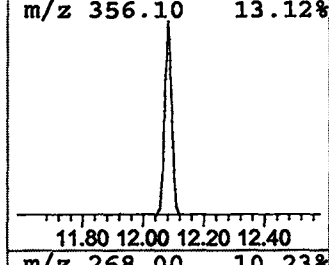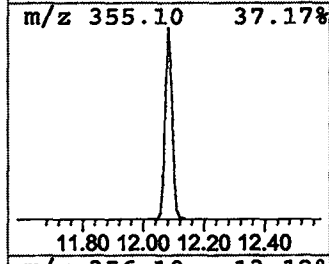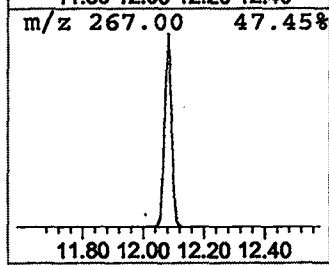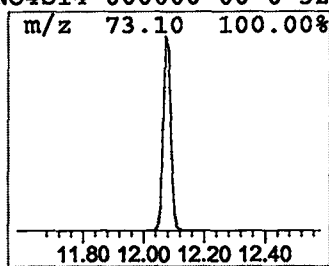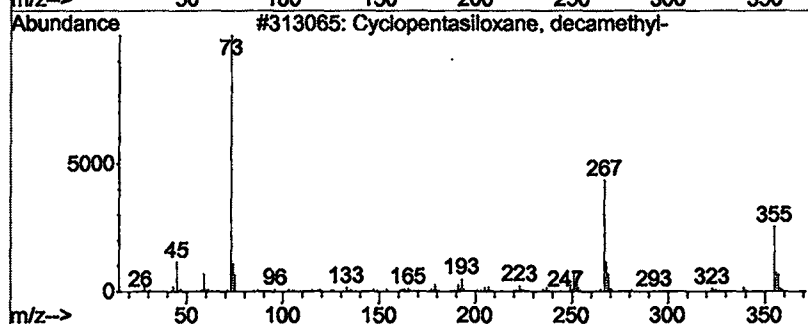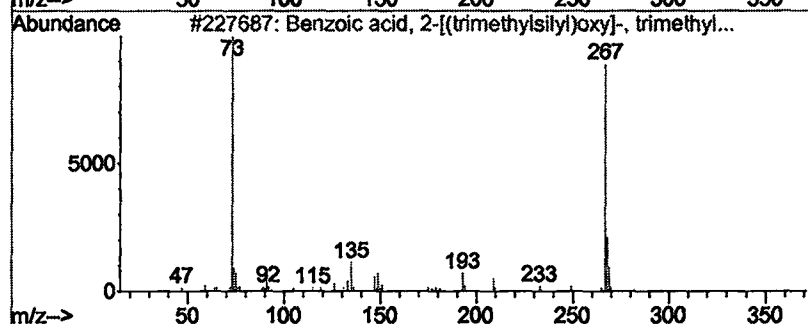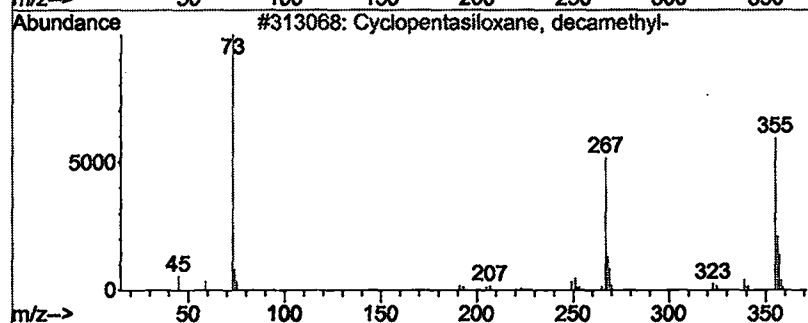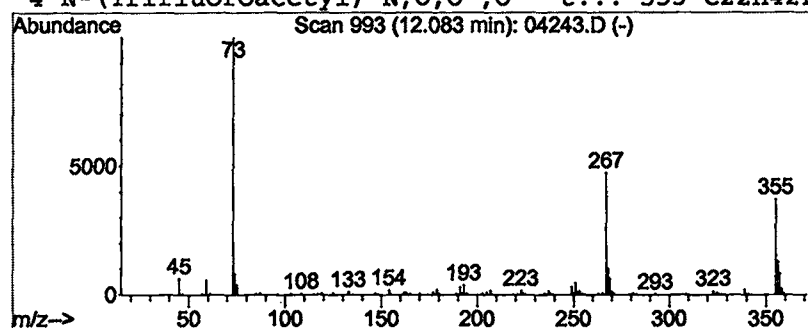

Operator ID: McLean Date Acquired: 28 Feb 2002 7:10 pm
 Data File: C:\MSDCHEM\1\DATA\022802\04243.D
 Name: GC MS SCAN 2/27
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasiloxan...	12.08	5.1	ug/L	1640910	2	13.05	6474130	20.0