

Data File : C:\HPCHEM\1\DATA\FEB1102\830.D

Acq On : 12 Feb 2002 4:41 am

Sample : GC/MS SCAN 1/15

Misc :

MS Integration Params: GOOFY.P

Quant Time: Feb 19 10:00 2002

Vial: 20

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Feb 13 11:43:23 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0208

*Sum
not needed*

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.35	152	319597	20.00	ug/l	0.00
10) Naphthalene-d8	15.99	136	1236098	20.00	ug/l	-0.01
17) Acenaphthene-d10	21.30	164	672486	20.00	ug/l	-0.01
29) Phenanthrene-d10	25.76	188	983496	20.00	ug/l	-0.01
38) Chrysene-d12	33.82	240	698427	20.00	ug/l	-0.02
44) Perylene-d12	38.11	264	453054	20.00	ug/l	-0.01

System Monitoring Compounds

37) 2,4-DDD	30.83	235	52951	5.36	ug/mL	0.33
Spiked Amount	5.000		Recovery	= 107.20%		

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	16.05	128	927	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.78	149	353	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#) = qualifier out of range (m) = manual integration

830.D GCMS0208.M

Tue Feb 19 10:01:40 2002

Page 1

Data File : C:\HPCHEM\1\DATA\FEB1102\830.D
Acq On : 12 Feb 2002 4:41 am
Sample : GC/MS SCAN 1/15
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 19 10:00 2002

Vial: 20
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 13 11:43:23 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.76	178	230	N.D.		
34) Anthracene	25.76	178	230	N.D.		
35) Di-n-butylphthalate	27.72	149	4349	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.82	228	1719	N.D.		
42) Bis(2-ethylhexyl)phthalate	34.03	149	1566	N.D.		
43) Chrysene	33.82	228	1719	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.12	252	1790	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration
830.D GCMS0208.M Tue Feb 19 10:01:44 2002


Page 2

Data File : C:\HPCHEM\1\DATA\FEB1102\830.D
 Acq On : 12 Feb 2002 4:41 am
 Sample : GC/MS SCAN 1/15
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 19 10:00 2002

Vial: 20
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Feb 13 11:43:23 2002
 Response via : Initial Calibration

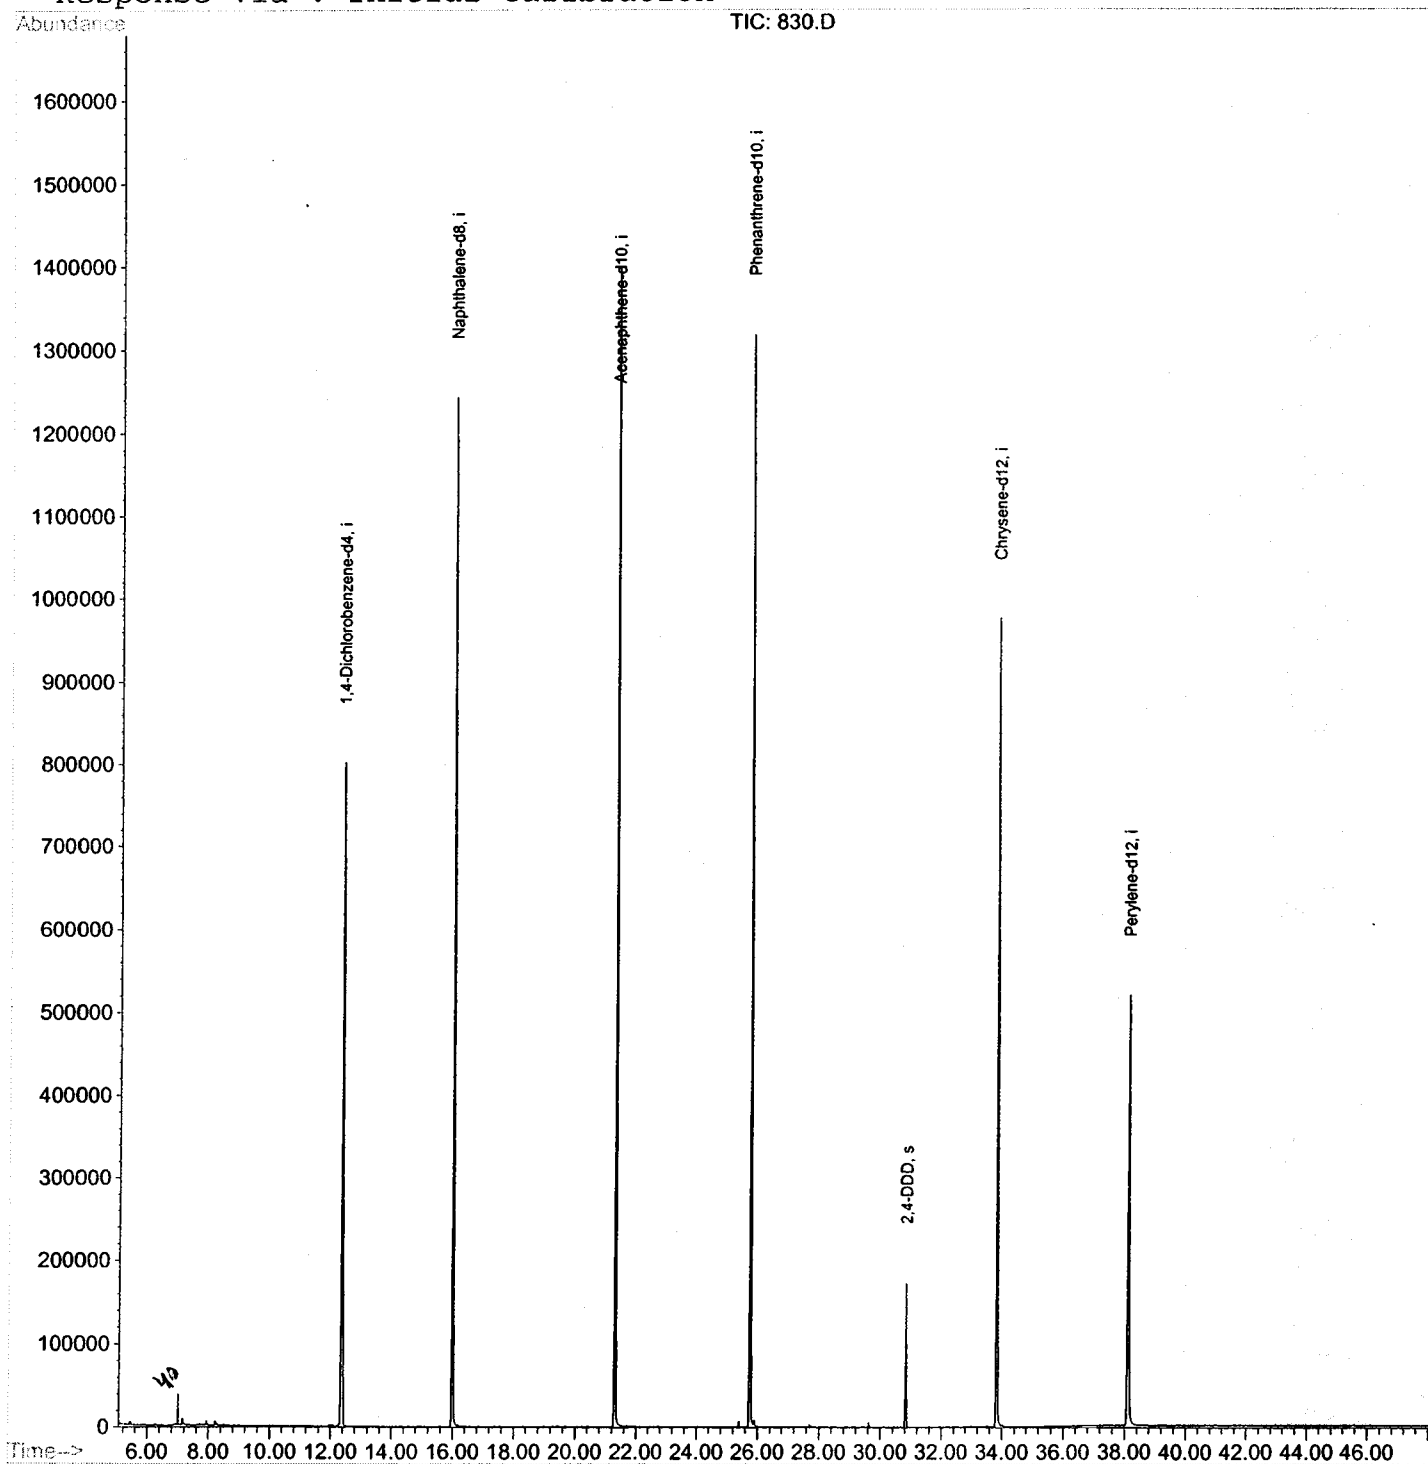

830.D GCMS0208.M

Tue Feb 19 10:01:51 2002


Page 3

Data File : C:\HPCHEM\1\DATA\FEB1102\830.D
 Acq On : 12 Feb 2002 4:41 am
 Sample : GC/MS SCAN 1/15
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 19 10:00 2002

Vial: 20
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Feb 13 11:43:23 2002
 Response via : Initial Calibration

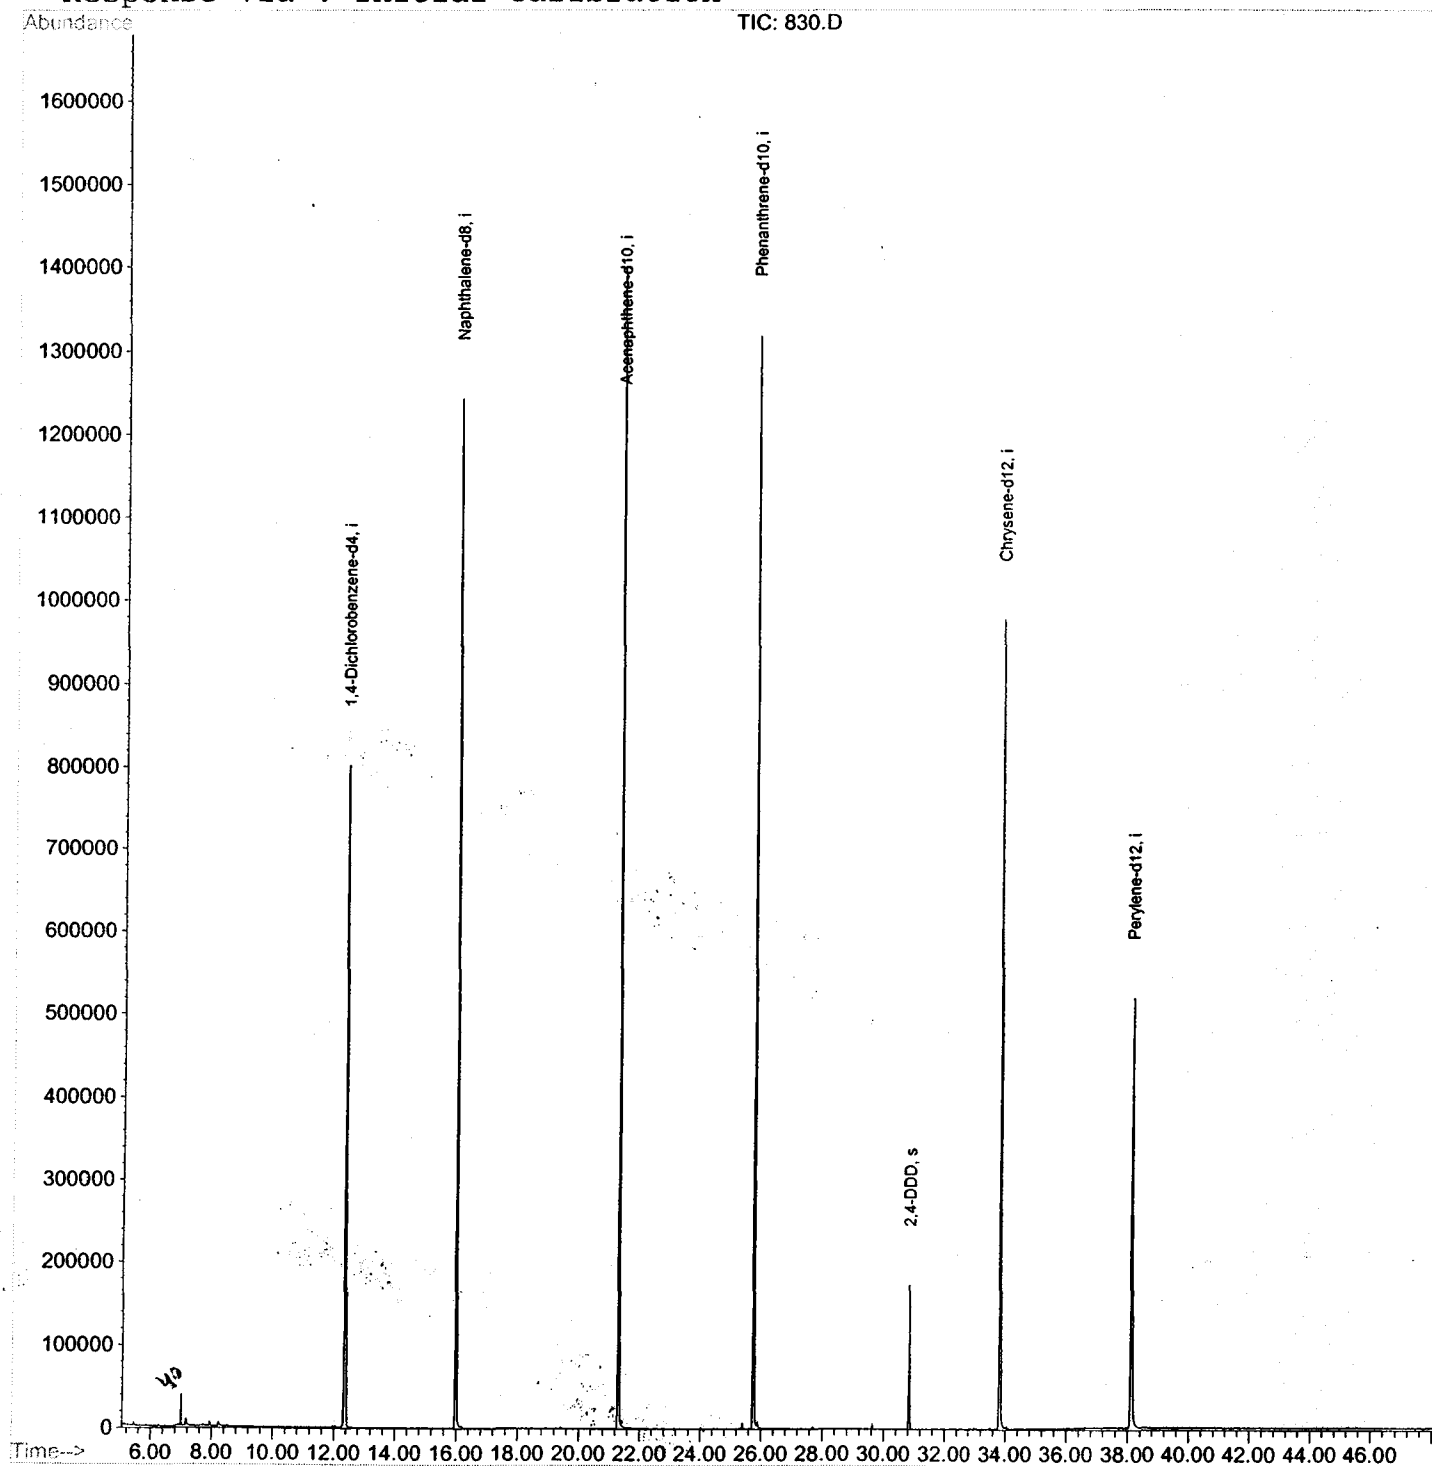


830.D GCMS0208.M

Tue Feb 19 10:01:51 2002

Page 3

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB1102\830.D
 Operator : 209 GALOS
 Acquired : 12 Feb 2002 4:41 am using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: GC/MS SCAN 1/15
 Misc Info :
 Vial Number: 20
 Quant File :GCMS0208.RES (RTE Integrator)

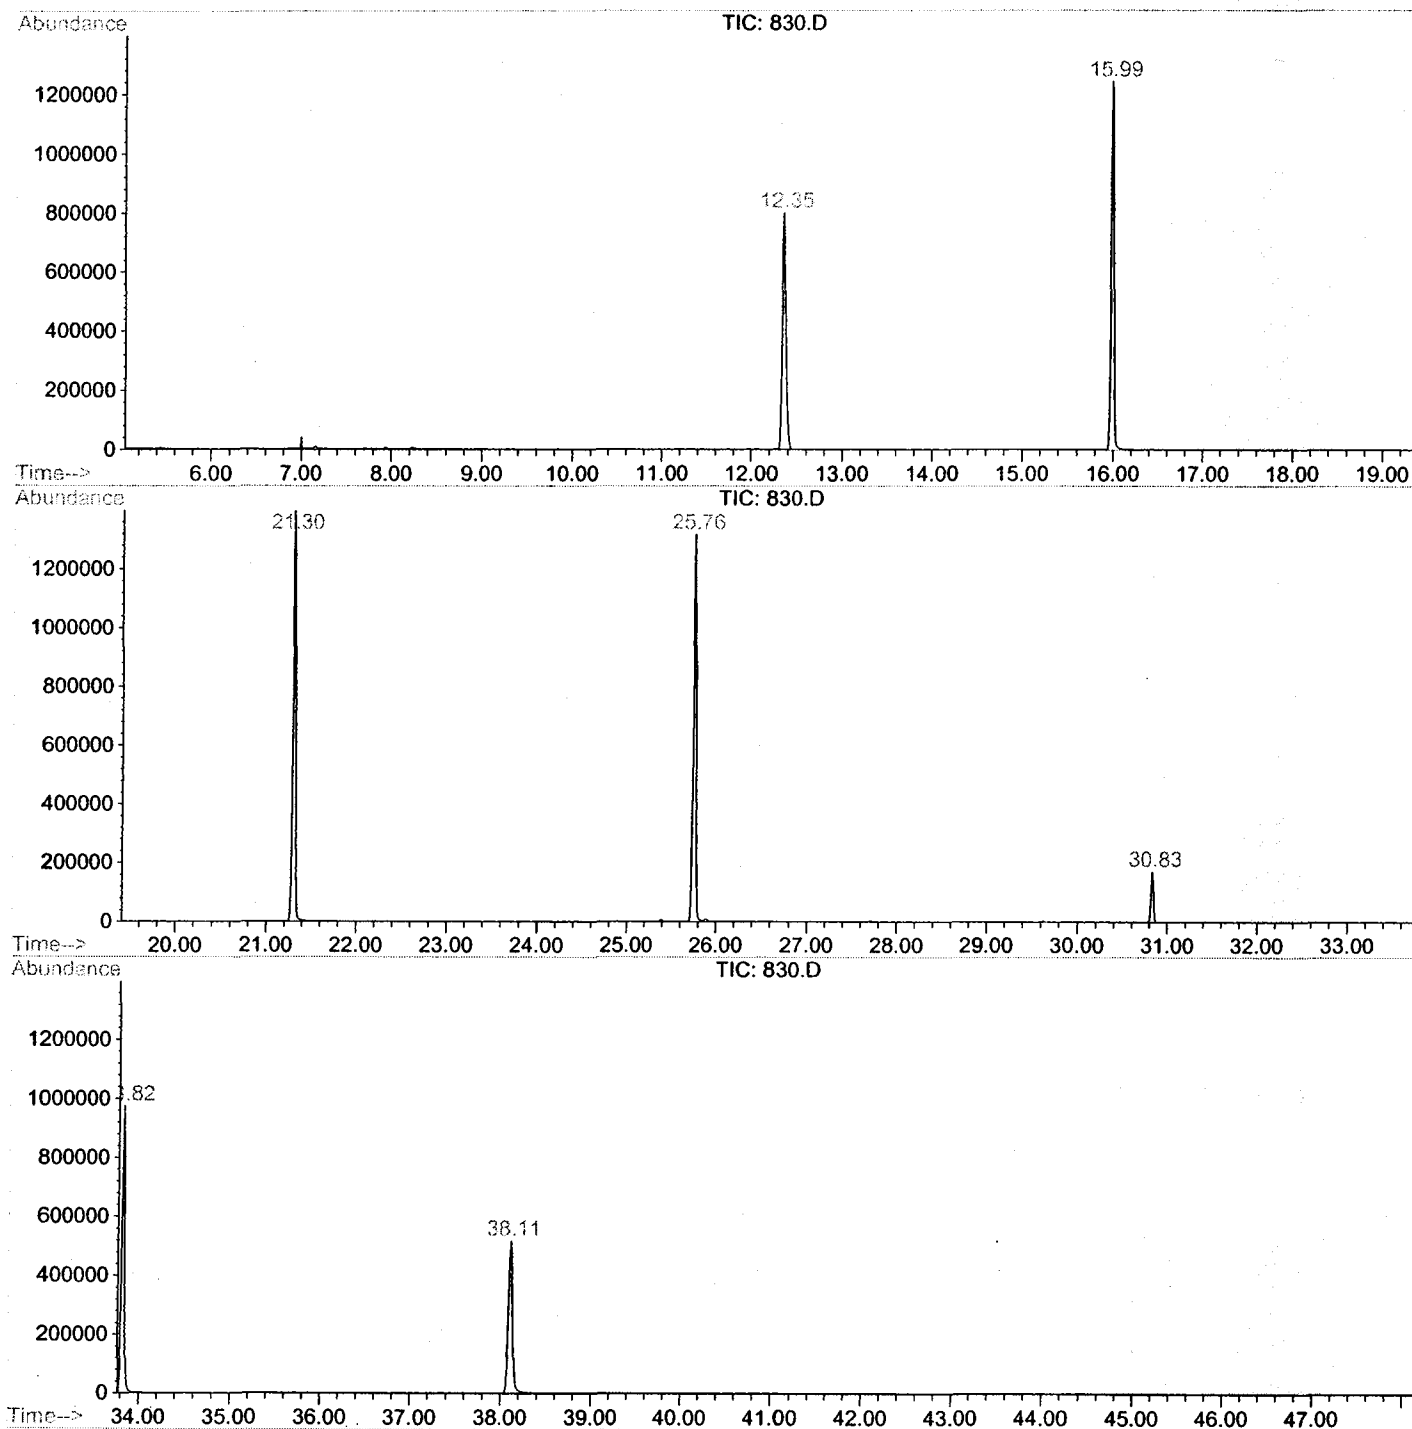

830.D GCMS0208.M

Tue Feb 19 10:34:49 2002

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 12 Feb 2002 4:41 am
Data File: C:\HPCHEM\1\DATA\FEB1102\830.D
Name: GC/MS SCAN 1/15
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC	Top	Hit	name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

830.D			GCMS0208.M								
				Tue Feb 19 10:34:53 2002							