

SEQUENCE NAME: C:\HPCHEM\1\SEQUENCE\FEB1902.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\feb1902\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch

(X) Full Method (X) Inject Anyway

() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0208	
2	Sample	2	CAL10	GCMS0208	
3	Sample	3	LB	GCMS0208	gc/ms scan 1/18
4	Sample	4	REF	GCMS0208	gc/ms scan 1/18
5	Sample	16	LBA	GCMS0208	reinject 1/15
6	Sample	5	1332	GCMS0208	gc/ms scan 1/18
7	Sample	6	1231	GCMS0208	gc/ms scan 1/18
8	Sample	7	1333	GCMS0208	gc/ms scan 1/18
9	Sample	8	1334	GCMS0208	gc/ms scan 1/18
10	Sample	9	1335	GCMS0208	gc/ms scan 1/18
11	Sample	10	1336	GCMS0208	gc/ms scan 1/18
12	Sample	11	1402	GCMS0208	gc/ms scan 1/18
13	Sample	12	1403	GCMS0208	gc/ms scan 1/18
14	Sample	13	1404	GCMS0208	gc/ms scan 1/18
15	Sample	14	1405	GCMS0208	gc/ms scan 1/18
16	Sample	15	1330	GCMS0208	gc/ms scan 1/18


Last Modified: Tue Feb 19 15:23:10 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB1902\DFTPP.D
Acq On : 19 Feb 2002 9:17 am
Sample :
Misc :
MS Integration Params: GOOFY.P
Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table

Vial: 1
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

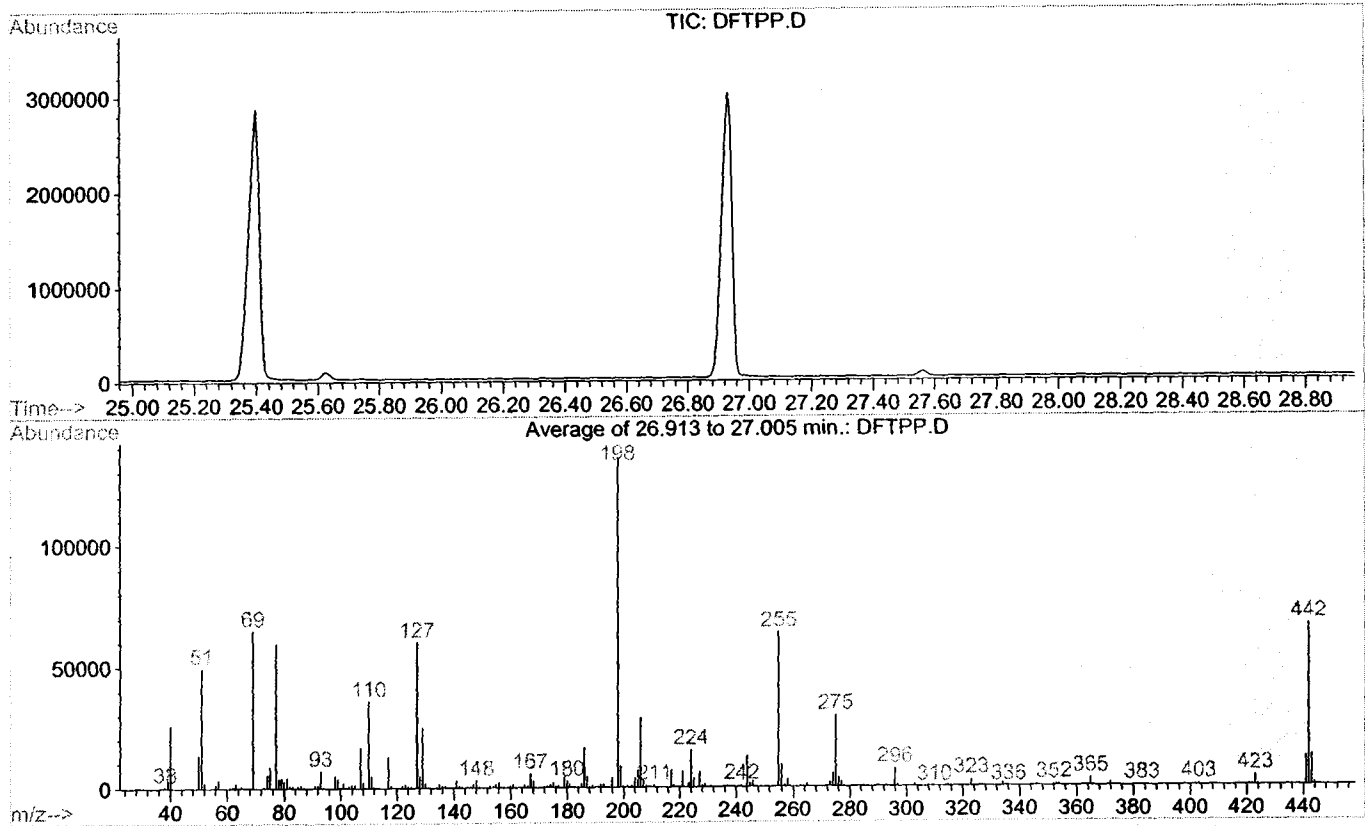

Spectrum Information: Average of 26.913 to 27.005 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.7	49765	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.1	65203	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.6	60492	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	135574	PASS
199	198	5	9	6.5	8857	PASS
275	198	10	30	21.8	29579	PASS
365	198	1	100	2.4	3303	PASS
441	443	0.01	100	93.4	11914	PASS
442	198	40	110	49.3	66864	PASS
443	442	17	23	19.1	12761	PASS